


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU110118\
Data File : VU027891.D
Acq On : 01 Nov 2018 08:52
Operator : MD/SY
Sample : BFB52
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB52

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR103018WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Nov 02 08:02:52 2018

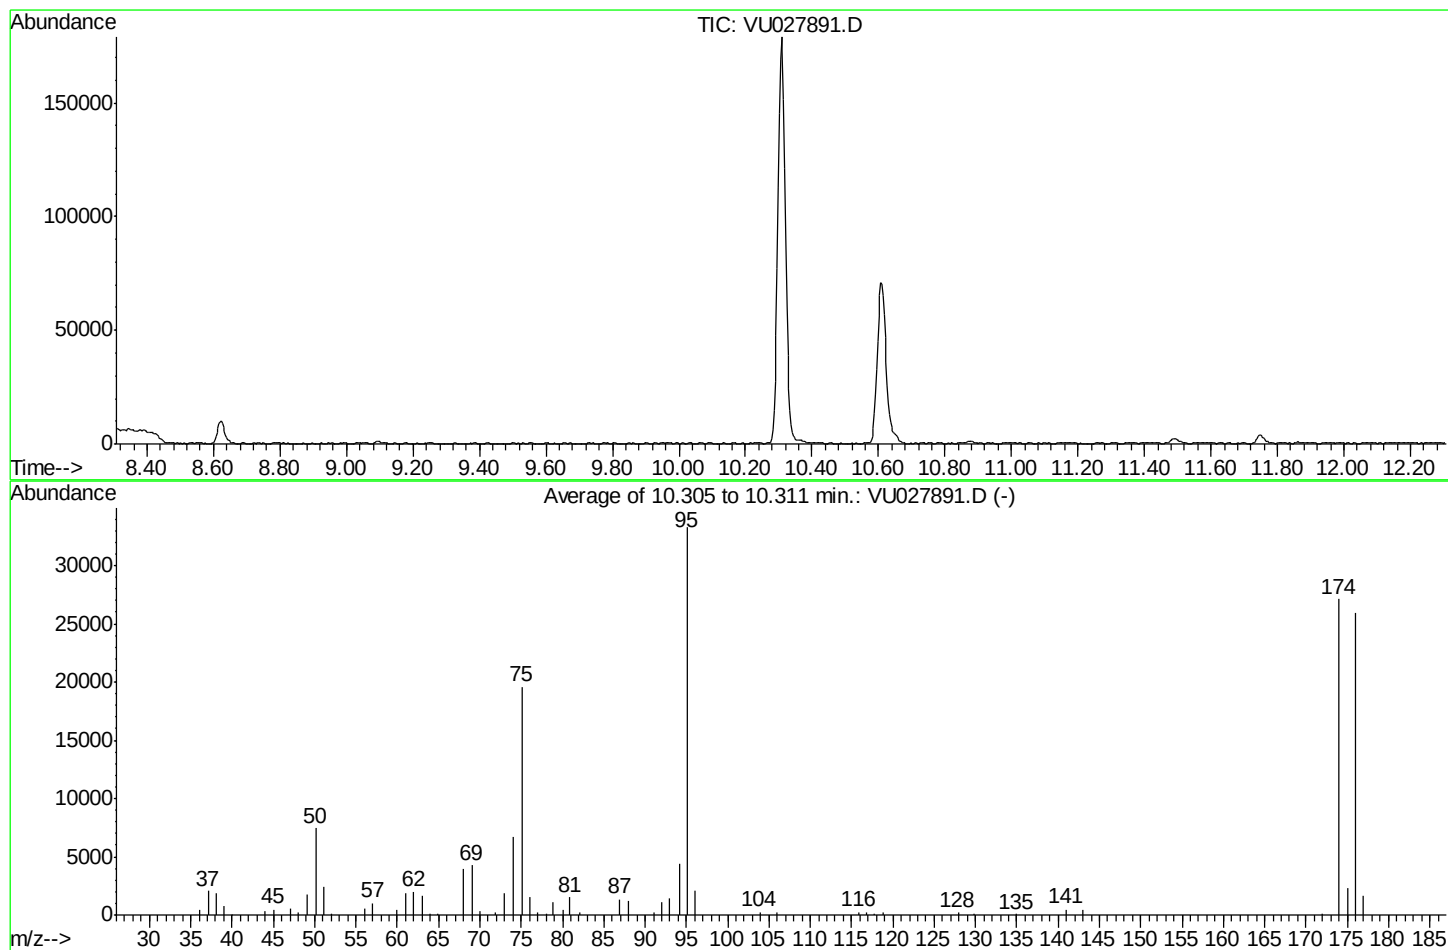

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	7448	PASS
75	95	30	80	58.8	19573	PASS
95	95	100	100	100.0	33288	PASS
96	95	5	9	6.3	2104	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	81.4	27101	PASS
175	174	5	9	8.5	2299	PASS
176	174	95	101	95.9	25994	PASS
177	176	5	9	6.4	1673	PASS

Scan 2828 (10.266 min): VU027891.D
BFB52

m/z	Abundance
43.90	325.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
36.00	426.0
37.10	2002.0
38.10	1839.0
39.00	802.0
44.00	693.0
45.00	481.0
47.10	483.0
48.10	284.0
49.10	1774.0
50.10	7250.0
51.10	2452.0
52.00	106.0
56.00	659.0
57.10	1060.0
60.00	475.0
61.00	1979.0
62.00	1929.0
63.00	1459.0
64.00	167.0
68.00	3830.0
69.00	4045.0
70.10	280.0
71.90	198.0
73.00	1794.0
74.10	6521.0
75.10	19192.0
76.00	1579.0
77.00	136.0
78.10	106.0
78.90	1156.0
80.00	423.0
80.90	1476.0
82.10	239.0
86.90	1354.0
88.00	1184.0
91.00	172.0
92.00	1165.0
93.00	1335.0
94.10	4218.0
95.10	32392.0
96.10	2176.0
103.90	297.0
106.00	140.0
115.90	227.0
116.90	222.0
117.80	145.0
118.80	169.0
127.90	255.0
129.80	110.0
141.00	471.0
142.90	441.0
171.90	165.0
174.00	26400.0
175.10	2255.0
176.00	24624.0
177.00	1733.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
36.00	425.0
37.10	2094.0
38.10	1988.0
39.10	842.0
44.00	641.0
45.00	484.0
47.10	541.0
48.10	302.0
49.10	1804.0
50.10	7574.0
51.10	2456.0
52.00	120.0
56.00	621.0
57.00	1046.0
60.00	479.0
61.00	1974.0
62.00	2062.0
63.00	1686.0
63.90	129.0
64.90	132.0
68.00	4052.0
69.00	4461.0
70.10	291.0
71.90	247.0
73.00	1883.0
74.10	6930.0
75.10	20344.0
76.00	1657.0
77.00	179.0
78.00	149.0
78.90	1167.0
80.00	430.0
80.90	1547.0
82.10	218.0
86.90	1362.0
88.00	1301.0
91.00	175.0
92.00	1149.0
93.00	1418.0
94.10	4511.0
95.10	34360.0
96.00	2096.0
103.90	276.0
106.00	197.0
115.90	266.0
116.80	229.0
117.80	190.0
118.80	230.0
127.90	228.0
129.90	122.0
134.90	120.0
141.00	492.0
143.00	483.0
172.00	160.0
174.00	27792.0
175.10	2377.0
176.00	26768.0
177.00	1748.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52

m/z	Abundance
36.00	356.0
37.10	2028.0
38.10	1951.0
39.10	808.0
40.00	111.0
44.00	539.0
45.00	389.0
47.00	541.0
48.00	241.0
49.00	1773.0
50.10	7521.0
51.00	2399.0
52.00	124.0
56.00	504.0
57.00	975.0
60.00	389.0
61.00	1776.0
62.00	2026.0
63.00	1681.0
65.00	158.0
68.00	3869.0
69.00	4294.0
70.00	289.0
71.90	198.0
73.00	1976.0
74.10	6637.0
75.10	19184.0
76.00	1512.0
77.00	204.0
78.00	141.0
78.90	1117.0
80.00	419.0
80.90	1454.0
82.00	204.0
86.90	1287.0
87.90	1307.0
91.10	182.0
92.10	1062.0
93.00	1489.0
94.10	4546.0
95.10	33112.0
96.00	2040.0
103.90	190.0
106.00	254.0
115.90	225.0
116.80	210.0
117.80	151.0
118.80	251.0
127.90	152.0
129.90	115.0
135.00	129.0
141.00	429.0
143.00	444.0
172.00	154.0
174.00	27112.0
175.10	2266.0
176.00	26592.0
177.00	1538.0

Instrument :
MSVOA_U
ClientSampleId :
BFB52