

Data Path : Z:\VOASRV\HPCHEM1\MSVOA\_U\DATA\VU110119\  
 Data File : VU035596.D  
 Acq On : 01 Nov 2019 12:39  
 Operator : JC/SP  
 Sample : K5631-06  
 Misc : 5.0mL/MSVOA\_U/WATER  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 BE881

Quant Time: Nov 01 17:07:23 2019  
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_U\METHOD\SOMULM103119WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Fri Nov 01 17:03:18 2019  
 Response via : Initial Calibration

| Internal Standards         | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|----------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Difluorobenzene     | 6.29  | 114  | 657521   | 50.00 | ug/L  | 0.00     |
| 28) Chlorobenzene-d5       | 9.45  | 117  | 626363   | 50.00 | ug/L  | 0.00     |
| 60) 1,4-Dichlorobenzene-d4 | 11.84 | 152  | 196660   | 50.00 | ug/L  | 0.00     |

## System Monitoring Compounds

|                                |         |       |          |          |      |         |
|--------------------------------|---------|-------|----------|----------|------|---------|
| 4) Vinyl Chloride-d3           | 1.62    | 65    | 211197   | 39.77    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 60 - 135 | Recovery | =    | 79.54%  |
| 7) Chloroethane-d5             | 1.93    | 69    | 184611   | 43.53    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 70 - 130 | Recovery | =    | 87.06%  |
| 11) 1,1-Dichloroethene-d2      | 2.60    | 63    | 268895   | 32.56    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 60 - 125 | Recovery | =    | 65.12%  |
| 21) 2-Butanone-d5              | 4.69    | 46    | 295274   | 95.19    | ug/L | 0.00    |
| Spiked Amount                  | 100.000 | Range | 40 - 130 | Recovery | =    | 95.19%  |
| 24) Chloroform-d               | 5.11    | 84    | 385201   | 46.97    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 70 - 125 | Recovery | =    | 93.94%  |
| 26) 1,2-Dichloroethane-d4      | 5.75    | 65    | 239045   | 47.58    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 70 - 125 | Recovery | =    | 95.16%  |
| 32) Benzene-d6                 | 5.77    | 84    | 814068   | 49.86    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 70 - 125 | Recovery | =    | 99.72%  |
| 36) 1,2-Dichloropropane-d6     | 6.74    | 67    | 265774   | 50.20    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 70 - 120 | Recovery | =    | 100.40% |
| 41) Toluene-d8                 | 7.93    | 98    | 731462   | 47.50    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 80 - 120 | Recovery | =    | 95.00%  |
| 43) trans-1,3-Dichloropropene- | 8.21    | 79    | 118916   | 48.76    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 60 - 125 | Recovery | =    | 97.52%  |
| 47) 2-Hexanone-d5              | 8.68    | 63    | 190305   | 93.78    | ug/L | 0.00    |
| Spiked Amount                  | 100.000 | Range | 45 - 130 | Recovery | =    | 93.78%  |
| 57) 1,1,2,2-Tetrachloroethane- | 10.79   | 84    | 356423   | 47.34    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 65 - 120 | Recovery | =    | 94.68%  |
| 64) 1,2-Dichlorobenzene-d4     | 12.22   | 152   | 202992   | 51.18    | ug/L | 0.00    |
| Spiked Amount                  | 50.000  | Range | 80 - 120 | Recovery | =    | 102.36% |

## Target Compounds


|                            |       |     |       |              | Qvalue |
|----------------------------|-------|-----|-------|--------------|--------|
| 13) Acetone                | 2.67  | 43  | 18210 | 6.672 ug/L   | 98     |
| 42) Toluene                | 8.01  | 91  | 23433 | 1.270 ug/L   | 97     |
| 48) 2-Hexanone             | 8.73  | 43  | 19761 | 3.853 ug/L # | 86     |
| 52) Ethylbenzene           | 9.60  | 91  | 26971 | 1.367 ug/L   | 96     |
| 53) m,p-Xylene             | 9.72  | 106 | 65686 | 8.875 ug/L   | 95     |
| 54) o-xylene               | 10.13 | 106 | 22775 | 3.148 ug/L   | 99     |
| 59) 1,2,3-Trichloropropane | 11.84 | 75  | 21617 | 3.517 ug/L   | 97     |
| 61) Bromoform              | 10.32 | 173 | 9548  | 3.182 ug/L # | 95     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_U\DATA\VU110119\  
Data File : VU035596.D  
Acq On : 01 Nov 2019 12:39  
Operator : JC/SP  
Sample : K5631-06  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BE881

Quant Time: Nov 01 17:07:23 2019  
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_U\METHOD\SOMULM103119WMA.M  
Quant Title : VOC Analysis  
QLast Update : Fri Nov 01 17:03:18 2019  
Response via : Initial Calibration

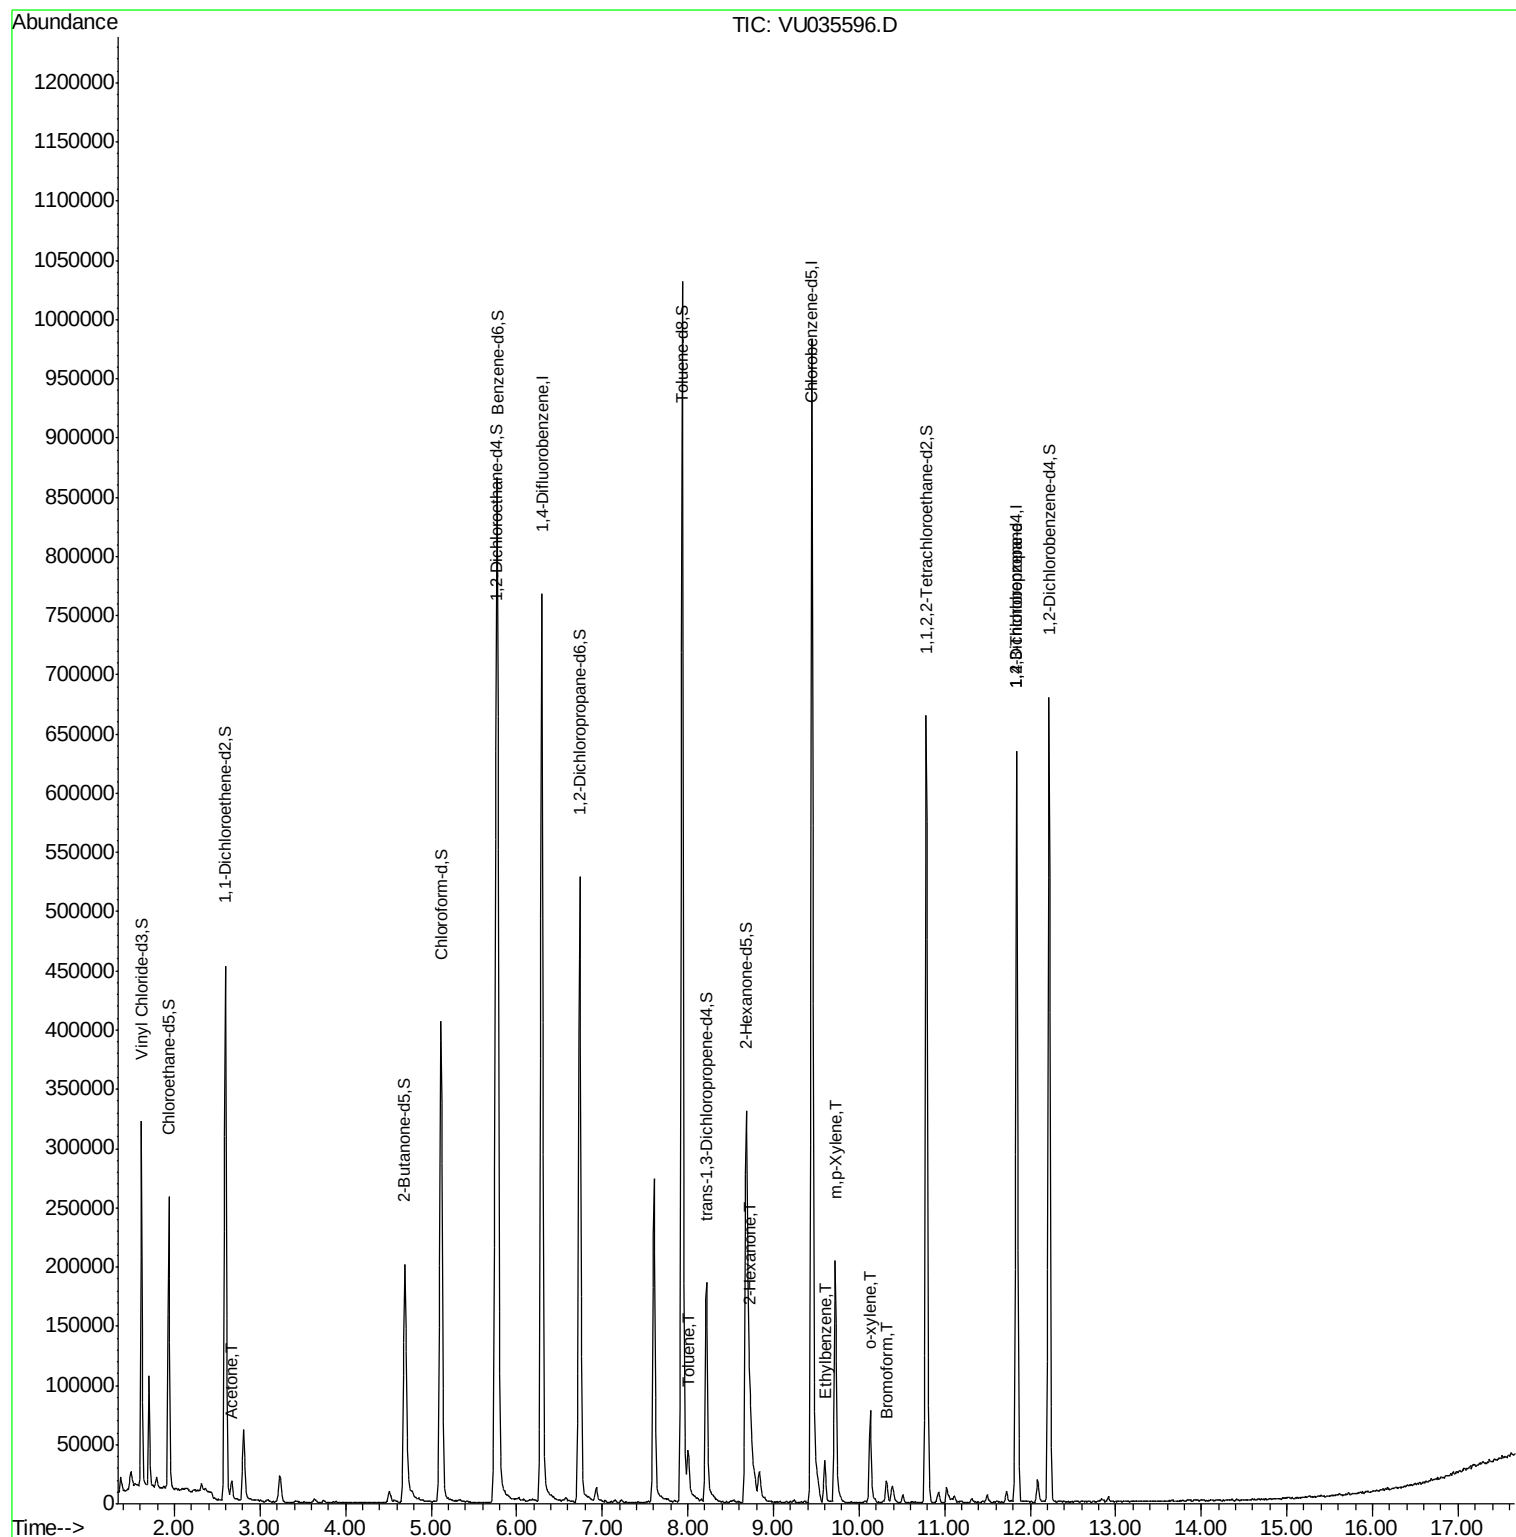

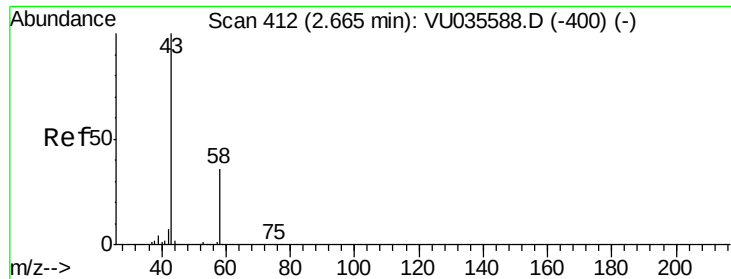

#13

Acetone

Concen: 6.672 ug/L

RT: 2.67 min Scan# 414

Delta R.T. 0.00 min

Lab File: VU035596.D

Acq: 01 Nov 2019 12:39

Instrument :

MSVOA\_U

ClientSampleId :





BE881

Tgt Ion: 43 Resp: 18210

Ion Ratio Lower Upper

43 100

58 33.7 0.0 70.0

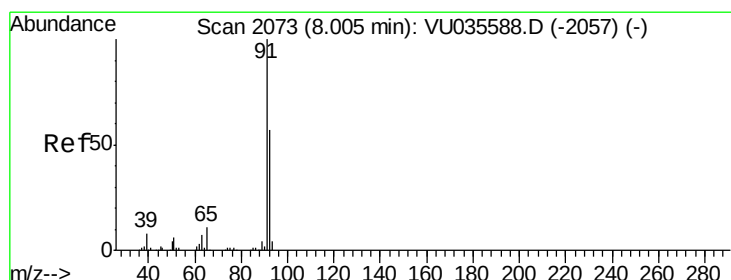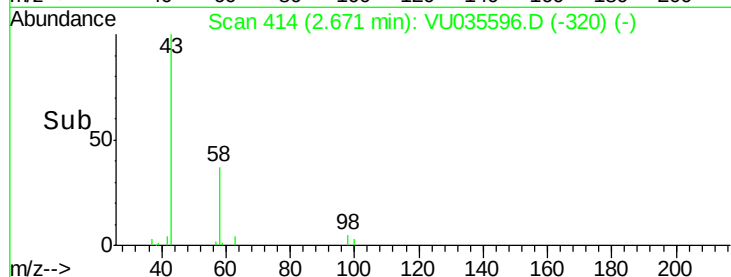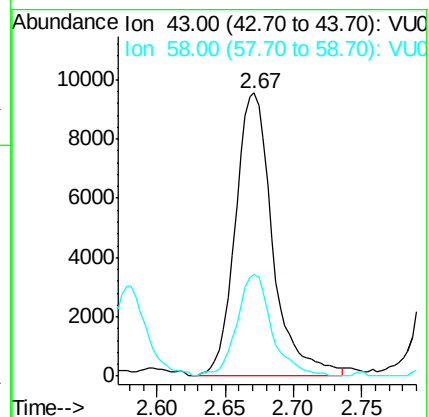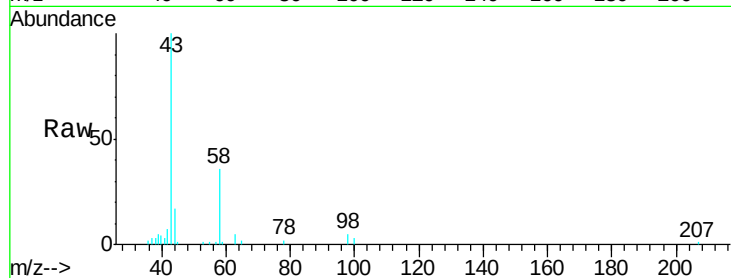

#42

Toluene

Concen: 1.270 ug/L

RT: 8.01 min Scan# 2073

Delta R.T. -0.00 min

Lab File: VU035596.D




Acq: 01 Nov 2019 12:39


Tgt Ion: 91 Resp: 23433

Ion Ratio Lower Upper

91 100

92 55.6 40.5 75.1


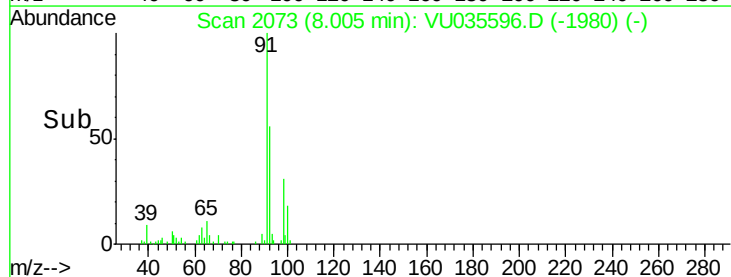
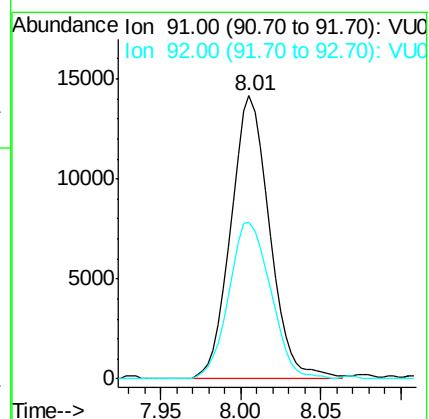
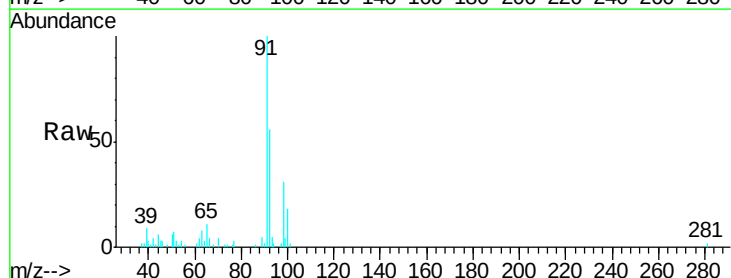


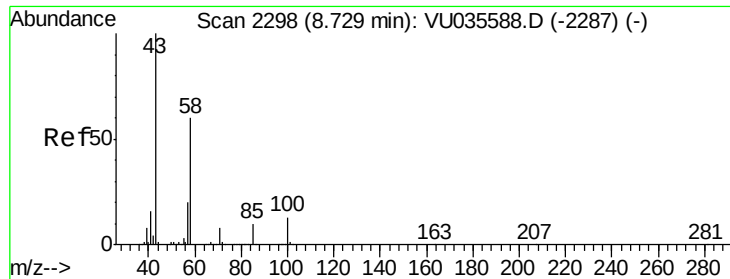

#48  
2-Hexanone  
Concen: 3.853 ug/L  
RT: 8.73 min Scan# 2298  
Delta R.T. -0.00 min  
Lab File: VU035596.D  
Acq: 01 Nov 2019 12:39




Instrument :  
MSVOA\_U  
ClientSampleId :  
BE881


Tgt Ion: 43 Resp: 19761  
Ion Ratio Lower Upper  
43 100  
58 61.7 50.4 75.6  
57 0.0 17.4 26.0#  
100 5.8 10.5 15.7#

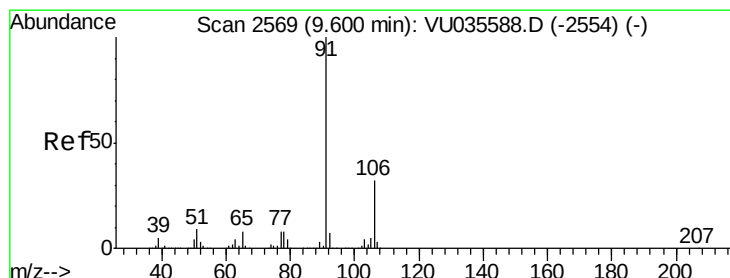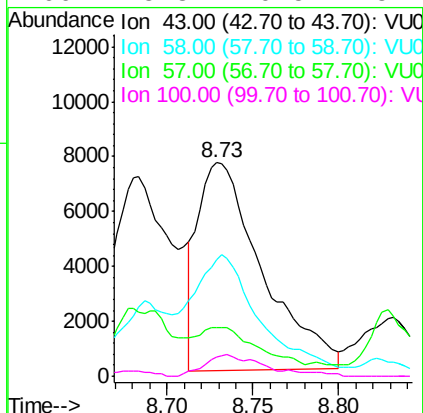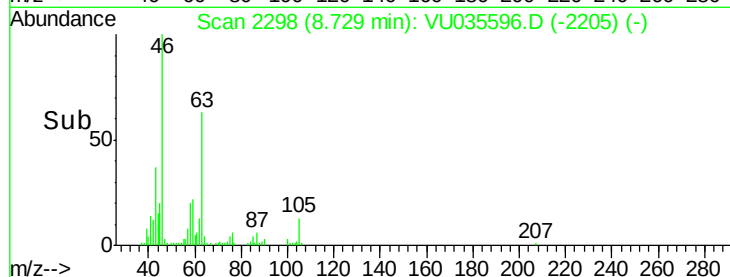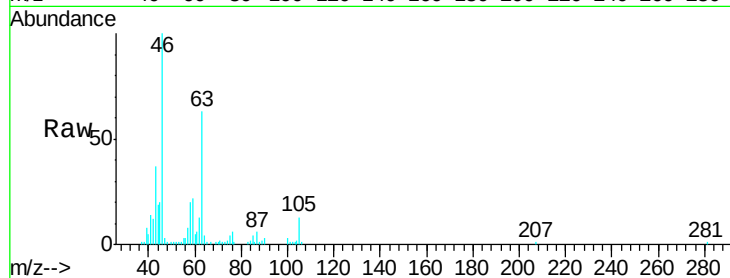

#52  
Ethylbenzene  
Concen: 1.367 ug/L  
RT: 9.60 min Scan# 2569  
Delta R.T. -0.00 min  
Lab File: VU035596.D  
Acq: 01 Nov 2019 12:39

Tgt Ion: 91 Resp: 26971  
Ion Ratio Lower Upper  
91 100  
106 32.7 21.6 40.0

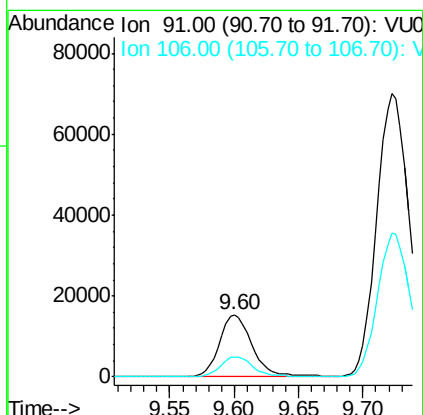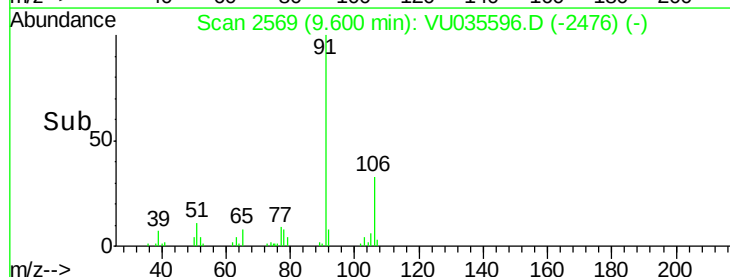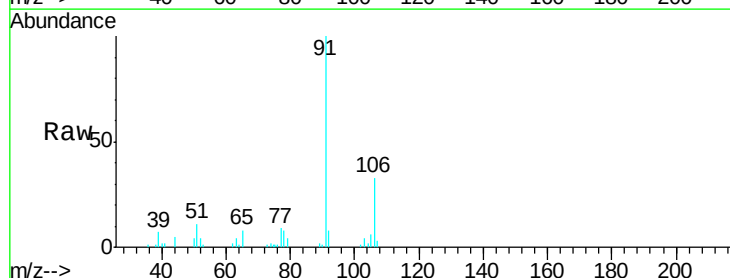

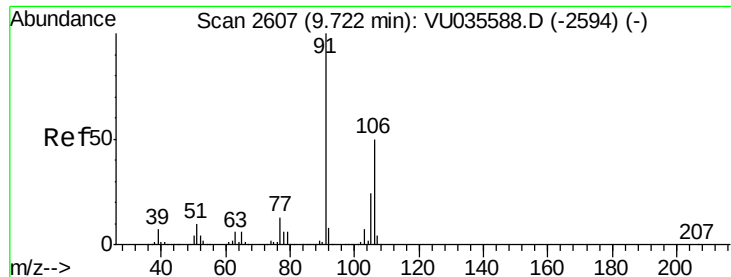

#53

m,p-Xylene

Concen: 8.875 ug/L

RT: 9.72 min Scan# 2607

Delta R.T. -0.00 min

Lab File: VU035596.D

Acq: 01 Nov 2019 12:39

Instrument :

MSVOA\_U

ClientSampled :


BE881

Tgt Ion:106 Resp: 65686

Ion Ratio Lower Upper




106 100

91 196.6 142.7 264.9

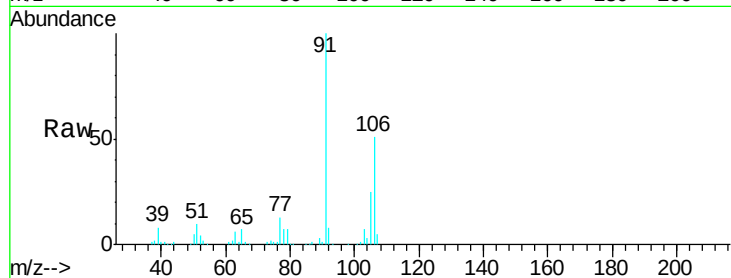

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VU0

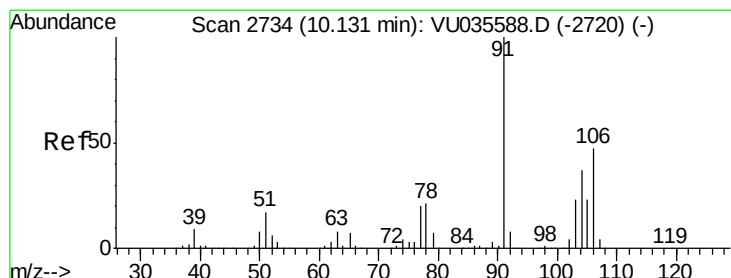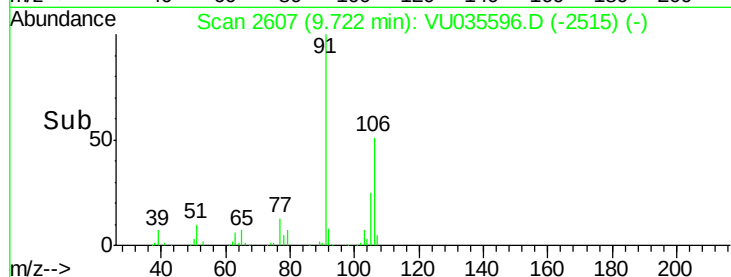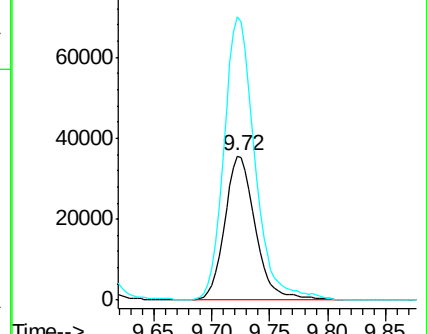

#54

o-xylene

Concen: 3.148 ug/L

RT: 10.13 min Scan# 2734

Delta R.T. -0.00 min

Lab File: VU035596.D


Acq: 01 Nov 2019 12:39

Tgt Ion:106 Resp: 22775

Ion Ratio Lower Upper



106 100


91 207.9 147.1 273.1

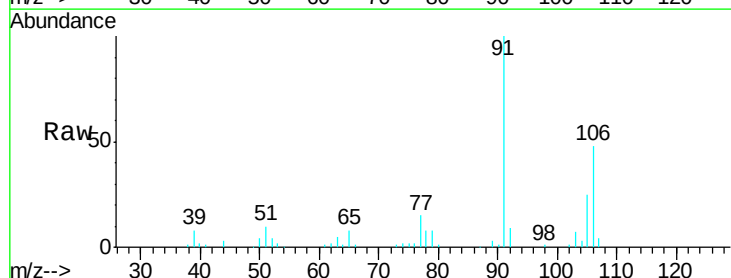

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VU0



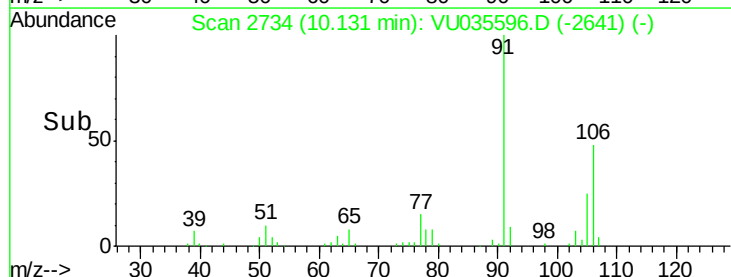
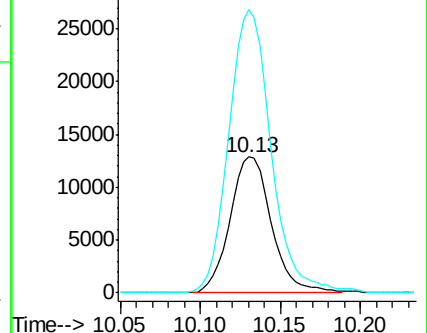


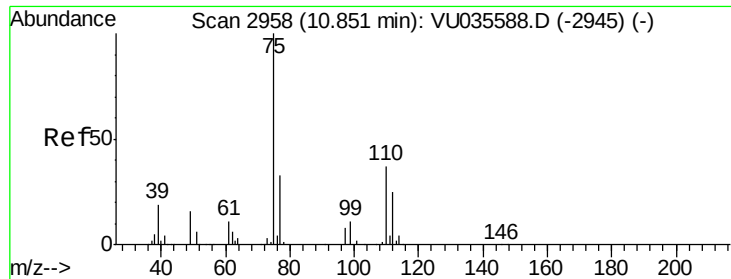

#59  
 1,2,3-Trichloropropane  
 Concen: 3.517 ug/L  
 RT: 11.84 min Scan# 3267  
 Delta R.T. 0.99 min  
 Lab File: VU035596.D  
 Acq: 01 Nov 2019 12:39

Instrument :  
 MSVOA\_U  
 ClientSampled :  
 BE881

Tgt Ion: 75 Resp: 21617  
 Ion Ratio Lower Upper  
 75 100  
 77 33.6 25.7 38.5

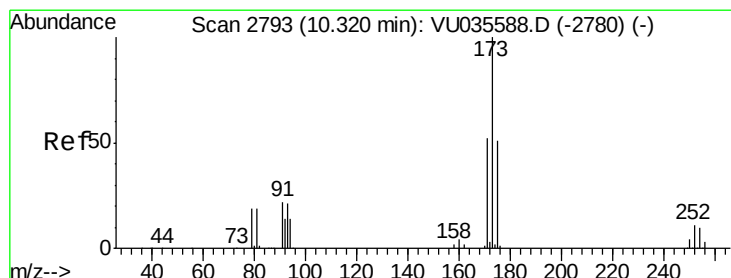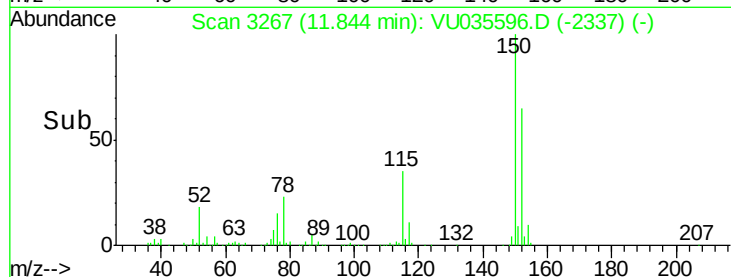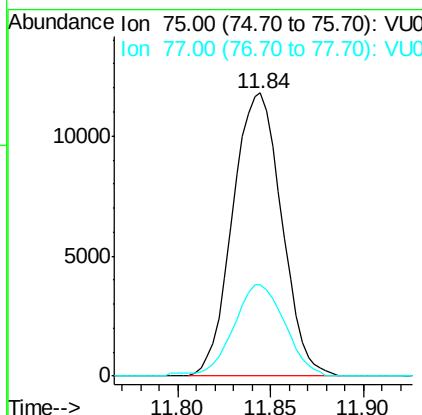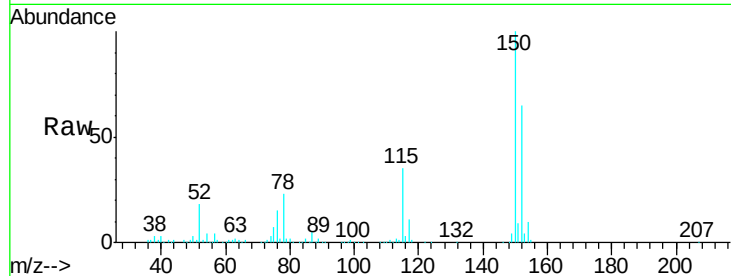

#61  
 Bromoform  
 Concen: 3.182 ug/L  
 RT: 10.32 min Scan# 2794  
 Delta R.T. -0.00 min  
 Lab File: VU035596.D  
 Acq: 01 Nov 2019 12:39

Tgt Ion: 173 Resp: 9548  
 Ion Ratio Lower Upper  
 173 100  
 175 46.3 39.4 59.0  
 254 6.3 8.1 12.1#

