

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU110119\
 Data File : VU035583.D
 Acq On : 31 Oct 2019 09:17
 Operator : JC/SP
 Sample : VU1101WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK45

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.617	78	86	100	rBV	378301	427477	16.97%	2.332%
2	1.932	176	184	198	rVB	297793	388654	15.43%	2.120%
3	2.594	377	390	409	rBV	531913	884892	35.12%	4.828%
4	2.826	456	462	474	rVB2	3781	6338	0.25%	0.035%
5	2.871	474	476	479	rBV3	728	421	0.02%	0.002%
6	2.941	496	498	503	rBV5	434	419	0.02%	0.002%
7	2.986	508	512	514	rBV3	379	327	0.01%	0.002%
8	3.002	515	517	519	rBV3	724	319	0.01%	0.002%
9	3.073	533	539	540	rBV3	1549	1275	0.05%	0.007%
10	3.228	575	587	603	rVB2	8449	19714	0.78%	0.108%
11	3.324	614	617	624	rBV3	558	672	0.03%	0.004%
12	3.356	624	627	630	rBV	373	328	0.01%	0.002%
13	3.385	630	636	638	rBV4	1153	990	0.04%	0.005%
14	3.449	653	656	662	rVB4	555	473	0.02%	0.003%
15	3.533	679	682	687	rBV	453	371	0.01%	0.002%
16	3.597	698	702	705	rBV2	357	332	0.01%	0.002%
17	3.867	781	786	788	rBV3	471	408	0.02%	0.002%
18	3.977	816	820	823	rBV2	381	291	0.01%	0.002%
19	4.019	831	833	839	rVB3	546	336	0.01%	0.002%
20	4.070	845	849	854	rVB2	525	613	0.02%	0.003%
21	4.102	854	859	863	rBV2	447	506	0.02%	0.003%
22	4.311	921	924	927	rBV	424	283	0.01%	0.002%
23	4.353	935	937	943	rVV	421	294	0.01%	0.002%
24	4.440	959	964	970	rVB	331	398	0.02%	0.002%
25	4.691	1026	1042	1067	rBV	220668	550480	21.85%	3.003%
26	5.112	1156	1173	1207	rBV	445218	982104	38.98%	5.358%
27	5.401	1261	1263	1264	rBV2	598	289	0.01%	0.002%
28	5.633	1332	1335	1340	rBV2	433	304	0.01%	0.002%
29	5.771	1349	1378	1408	rBV2	965197	2519530	100.00%	13.746%
30	6.292	1525	1540	1565	rBV	798636	1548325	61.45%	8.447%
31	6.671	1655	1658	1661	rVB2	662	453	0.02%	0.002%
32	6.732	1661	1677	1703	rBV	574574	1142664	45.35%	6.234%
33	7.073	1780	1783	1788	rVB4	893	797	0.03%	0.004%
34	7.105	1788	1793	1797	rVB4	610	723	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU110119\
 Data File : VU035583.D
 Acq On : 31 Oct 2019 09:17
 Operator : JC/SP
 Sample : VU1101WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK45

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
 Title : VOC Analysis

35	7.144	1797	1805	1810	rBV3	906	1472	0.06%	0.008%
36	7.227	1822	1831	1840	rVB5	2580	4166	0.17%	0.023%
37	7.398	1879	1884	1885	rBV2	535	370	0.01%	0.002%
38	7.478	1902	1909	1914	rVB2	703	896	0.04%	0.005%
39	7.507	1914	1918	1920	rBV2	350	284	0.01%	0.002%
40	7.520	1920	1922	1926	rVB	446	301	0.01%	0.002%
41	7.549	1926	1931	1933	rBV3	699	669	0.03%	0.004%
42	7.604	1934	1948	1977	rBV	300470	560489	22.25%	3.058%
43	7.838	2015	2021	2033	rVB3	6651	11805	0.47%	0.064%
44	7.935	2033	2051	2070	rBV	1125891	2026068	80.41%	11.053%
45	8.214	2126	2138	2165	rBV	203525	387153	15.37%	2.112%
46	8.436	2202	2207	2213	rVB4	1102	1309	0.05%	0.007%
47	8.517	2230	2232	2236	rVB3	598	304	0.01%	0.002%
48	8.587	2247	2254	2260	rBV6	1766	2527	0.10%	0.014%
49	8.681	2268	2283	2335	rBV	351996	1111819	44.13%	6.066%
50	8.877	2341	2344	2347	rBV5	620	527	0.02%	0.003%
51	8.915	2353	2356	2357	rBV	409	292	0.01%	0.002%
52	9.089	2405	2410	2412	rBV2	358	324	0.01%	0.002%
53	9.134	2422	2424	2428	rVV2	285	263	0.01%	0.001%
54	9.218	2446	2450	2453	rVB3	539	377	0.01%	0.002%
55	9.333	2484	2486	2490	rBV2	421	272	0.01%	0.001%
56	9.359	2490	2494	2496	rBV2	421	285	0.01%	0.002%
57	9.449	2508	2522	2559	rBV	1039779	1906852	75.68%	10.403%
58	9.600	2560	2569	2578	rVB3	2803	4506	0.18%	0.025%
59	9.677	2589	2593	2594	rBV	436	294	0.01%	0.002%
60	9.687	2594	2596	2599	rVV3	809	568	0.02%	0.003%
61	9.722	2601	2607	2616	rVV6	3507	5137	0.20%	0.028%
62	9.809	2631	2634	2637	rVB2	483	278	0.01%	0.002%
63	9.903	2659	2663	2667	rVB3	520	519	0.02%	0.003%
64	10.041	2701	2706	2709	rBV2	567	467	0.02%	0.003%
65	10.134	2725	2735	2748	rBV8	4426	10204	0.40%	0.056%
66	10.185	2748	2751	2753	rVB2	548	272	0.01%	0.001%
67	10.292	2780	2784	2787	rVV2	431	347	0.01%	0.002%
68	10.317	2787	2792	2803	rVV5	1061	1579	0.06%	0.009%
69	10.507	2843	2851	2861	rBV6	3811	6407	0.25%	0.035%
70	10.584	2871	2875	2881	rVB4	399	439	0.02%	0.002%
71	10.639	2888	2892	2894	rBV	560	342	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU110119\
 Data File : VU035583.D
 Acq On : 31 Oct 2019 09:17
 Operator : JC/SP
 Sample : VU1101WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK45

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
 Title : VOC Analysis

72	10.655	2894	2897	2900	rBV3	998	818	0.03%	0.004%
73	10.787	2925	2938	2957	rBV	709566	1228373	48.75%	6.701%
74	10.999	3000	3004	3007	rBV	450	334	0.01%	0.002%
75	11.070	3021	3026	3028	rBV2	523	420	0.02%	0.002%
76	11.115	3029	3040	3052	rVV5	4072	7087	0.28%	0.039%
77	11.292	3090	3095	3099	rBV	444	513	0.02%	0.003%
78	11.320	3100	3104	3106	rBV2	599	375	0.01%	0.002%
79	11.372	3117	3120	3124	rBV	465	273	0.01%	0.001%
80	11.439	3135	3141	3147	rBV4	1013	1143	0.05%	0.006%
81	11.494	3147	3158	3170	rBV3	5204	9802	0.39%	0.053%
82	11.620	3194	3197	3201	rBV2	358	263	0.01%	0.001%
83	11.774	3237	3245	3253	rBV4	6037	10064	0.40%	0.055%
84	11.841	3253	3266	3286	rVB	669361	1184314	47.01%	6.461%
85	11.957	3300	3302	3307	rVB3	621	511	0.02%	0.003%
86	12.050	3327	3331	3333	rBV3	708	519	0.02%	0.003%
87	12.224	3370	3385	3401	rBV	735124	1276324	50.66%	6.963%
88	12.314	3409	3413	3415	rBV3	360	363	0.01%	0.002%
89	12.340	3419	3421	3426	rVB4	763	465	0.02%	0.003%
90	12.417	3442	3445	3451	rBV4	506	620	0.02%	0.003%
91	12.600	3500	3502	3508	rVB2	498	414	0.02%	0.002%
92	13.028	3628	3635	3646	rVB6	2167	3443	0.14%	0.019%
93	13.246	3694	3703	3711	rVB3	8241	12626	0.50%	0.069%
94	13.420	3754	3757	3758	rBV4	615	377	0.01%	0.002%
95	13.864	3879	3895	3905	rBV5	10635	18167	0.72%	0.099%
96	13.989	3929	3934	3939	rBV4	887	995	0.04%	0.005%
97	14.108	3963	3971	3982	rBV2	10867	17376	0.69%	0.095%
98	14.240	4006	4012	4016	rBV3	1122	1336	0.05%	0.007%
99	14.353	4038	4047	4057	rBV3	13494	20082	0.80%	0.110%
100	14.484	4086	4088	4090	rBV	879	470	0.02%	0.003%


Sum of corrected areas: 18329850

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU110119\
Data File : VU035583.D
Acq On : 31 Oct 2019 09:17
Operator : JC/SP
Sample : VU1101WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
VBLK45

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

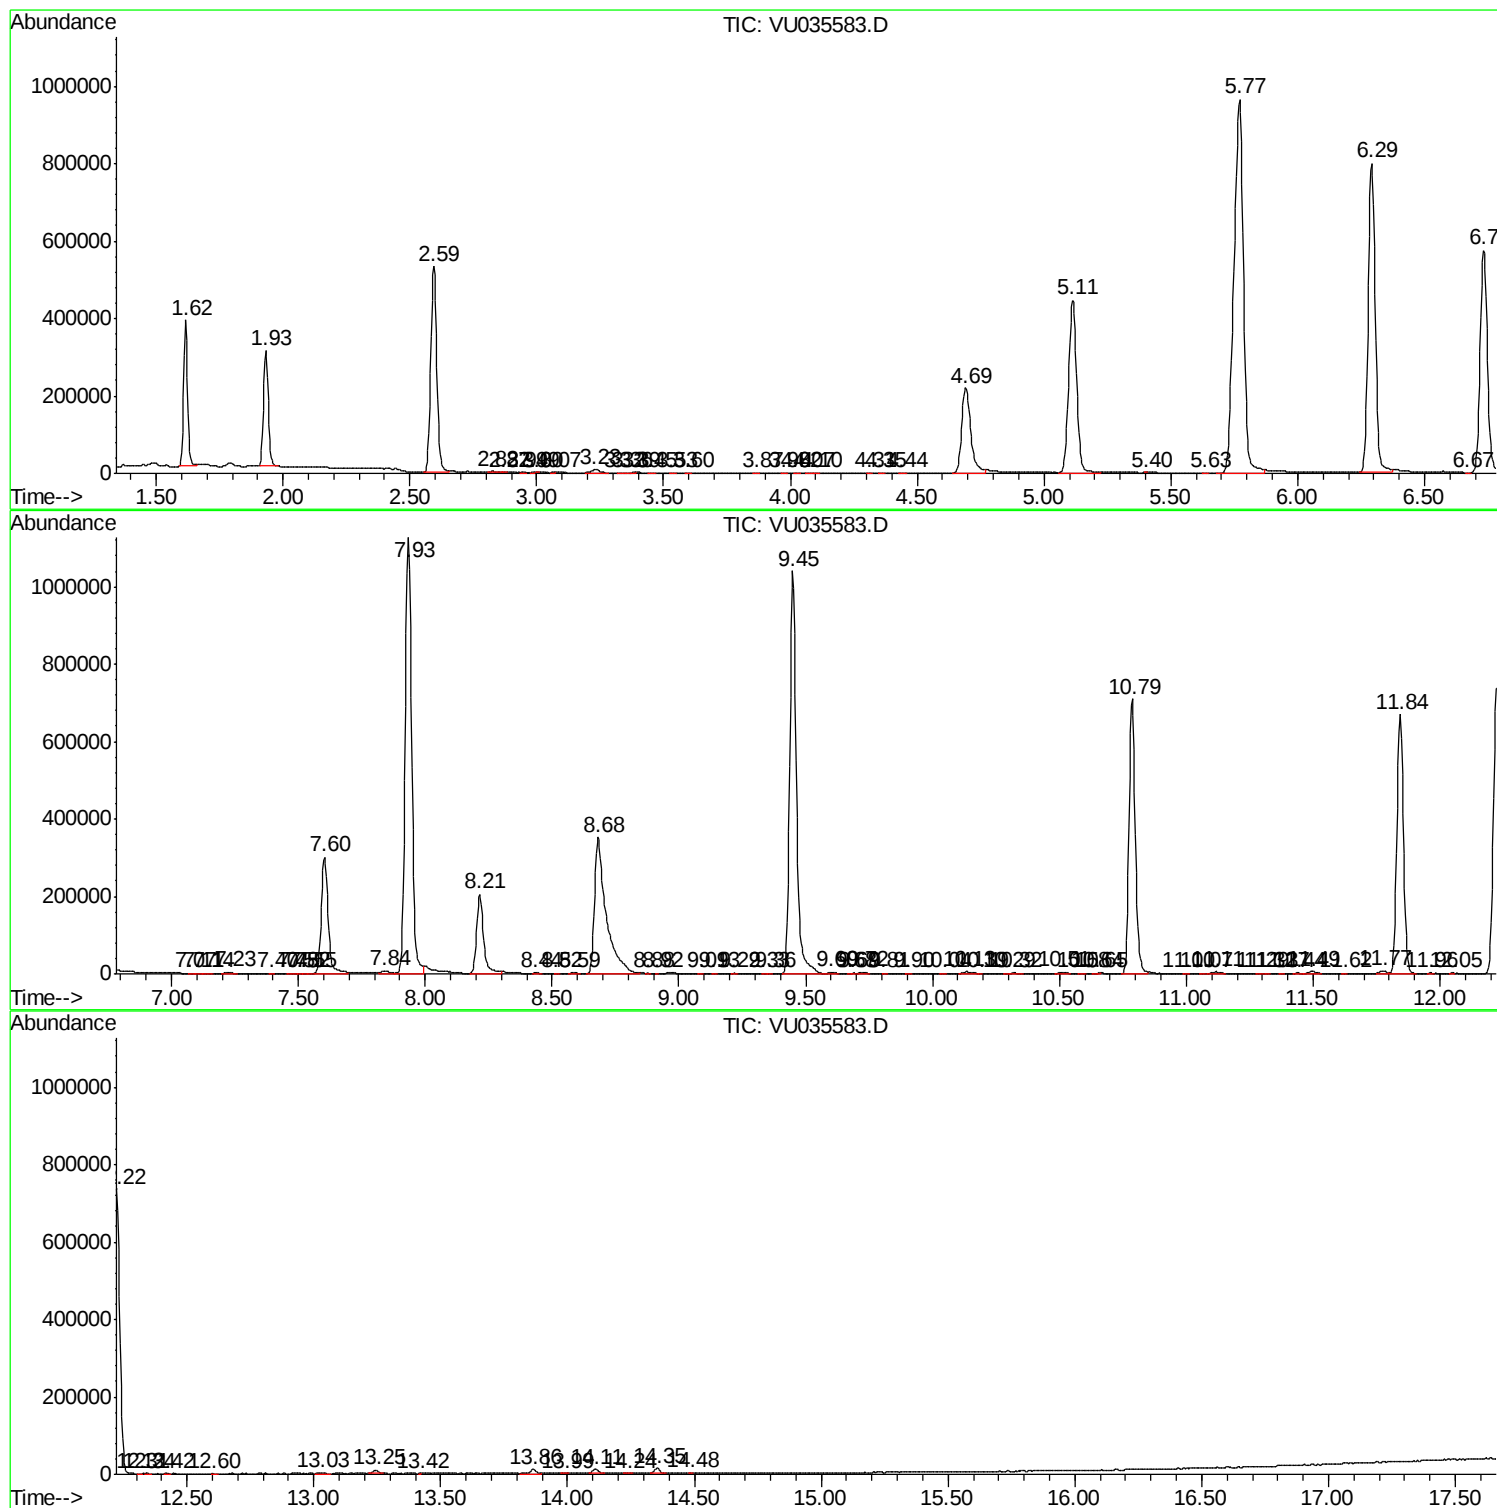

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU110119\
Data File : VU035583.D
Acq On : 31 Oct 2019 09:17
Operator : JC/SP
Sample : VU1101WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK45

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU110119\
Data File : VU035583.D
Acq On : 31 Oct 2019 09:17
Operator : JC/SP
Sample : VU1101WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK45

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc