

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU110119\
 Data File : VU035591.D
 Acq On : 01 Nov 2019 10:42
 Operator : JC/SP
 Sample : K5631-01 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BE878

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.373	6	10	22	rVB2	12475	12593	0.55%	0.076%
2	1.617	78	86	101	rVB	301213	330211	14.55%	1.986%
3	1.932	176	184	200	rVB	245619	325626	14.34%	1.959%
4	2.594	378	390	406	rBV	448989	743486	32.75%	4.472%
5	2.810	449	457	468	rVB3	8155	15633	0.69%	0.094%
6	3.080	536	541	545	rBV5	2277	2647	0.12%	0.016%
7	3.234	574	589	605	rBV2	28309	66171	2.92%	0.398%
8	3.366	626	630	632	rBV2	588	373	0.02%	0.002%
9	3.434	649	651	654	rVB2	814	427	0.02%	0.003%
10	3.456	654	658	661	rBV2	708	472	0.02%	0.003%
11	3.524	677	679	683	rBV2	498	373	0.02%	0.002%
12	3.572	688	694	700	rVB4	575	468	0.02%	0.003%
13	3.617	704	708	712	rBV4	441	456	0.02%	0.003%
14	3.639	712	715	719	rBV4	774	542	0.02%	0.003%
15	3.710	735	737	741	rVB2	525	364	0.02%	0.002%
16	3.913	797	800	804	rVB3	535	410	0.02%	0.002%
17	4.093	853	856	859	rVV2	370	319	0.01%	0.002%
18	4.163	872	878	881	rBV3	362	358	0.02%	0.002%
19	4.279	911	914	918	rVV	590	548	0.02%	0.003%
20	4.299	918	920	927	rVV2	488	499	0.02%	0.003%
21	4.475	970	975	978	rBV2	512	488	0.02%	0.003%
22	4.514	978	987	996	rVB6	1956	3910	0.17%	0.024%
23	4.607	1013	1016	1019	rBV2	526	311	0.01%	0.002%
24	4.694	1027	1043	1068	rBV	208826	512100	22.56%	3.080%
25	5.115	1157	1174	1198	rBV	402618	881546	38.83%	5.303%
26	5.311	1232	1235	1238	rBV3	1016	810	0.04%	0.005%
27	5.327	1238	1240	1241	rBV2	1085	516	0.02%	0.003%
28	5.553	1307	1310	1314	rVB2	465	305	0.01%	0.002%
29	5.578	1314	1318	1324	rBV4	459	511	0.02%	0.003%
30	5.623	1330	1332	1335	rVV2	487	308	0.01%	0.002%
31	5.649	1338	1340	1344	rVB3	411	307	0.01%	0.002%
32	5.771	1355	1378	1409	rBV2	864817	2270005	100.00%	13.655%
33	6.138	1489	1492	1493	rBV2	852	513	0.02%	0.003%
34	6.292	1525	1540	1565	rBV	772629	1479923	65.19%	8.902%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU110119\
 Data File : VU035591.D
 Acq On : 01 Nov 2019 10:42
 Operator : JC/SP
 Sample : K5631-01 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleID :
 BE878

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
 Title : VOC Analysis

35	6.642	1647	1649	1652	rVB3	563	335	0.01%	0.002%
36	6.736	1662	1678	1702	rBV	516478	1024418	45.13%	6.162%
37	6.922	1733	1736	1740	rBV5	1315	1356	0.06%	0.008%
38	6.977	1751	1753	1756	rBV2	756	399	0.02%	0.002%
39	7.032	1767	1770	1772	rVB2	664	365	0.02%	0.002%
40	7.070	1778	1782	1786	rBV	645	659	0.03%	0.004%
41	7.192	1818	1820	1824	rVB3	464	315	0.01%	0.002%
42	7.221	1824	1829	1831	rBV3	1905	1751	0.08%	0.011%
43	7.260	1839	1841	1845	rBV3	608	383	0.02%	0.002%
44	7.414	1885	1889	1895	rBV4	364	405	0.02%	0.002%
45	7.604	1935	1948	1976	rBV	278703	511029	22.51%	3.074%
46	7.842	2015	2022	2034	rVB5	2906	5096	0.22%	0.031%
47	7.935	2037	2051	2067	rBV	1045003	1829114	80.58%	11.003%
48	8.215	2125	2138	2165	rBV	191990	350064	15.42%	2.106%
49	8.485	2218	2222	2224	rBV2	681	521	0.02%	0.003%
50	8.504	2224	2228	2232	rVV2	416	462	0.02%	0.003%
51	8.585	2249	2253	2255	rBV3	689	562	0.02%	0.003%
52	8.678	2269	2282	2326	rBV	375515	1007343	44.38%	6.059%
53	8.903	2351	2352	2355	rVB3	1055	421	0.02%	0.003%
54	8.948	2363	2366	2369	rBV2	590	513	0.02%	0.003%
55	9.006	2380	2384	2386	rVB2	503	343	0.02%	0.002%
56	9.031	2386	2392	2394	rBV3	558	367	0.02%	0.002%
57	9.057	2398	2400	2405	rVB2	498	347	0.02%	0.002%
58	9.147	2424	2428	2431	rBV2	898	598	0.03%	0.004%
59	9.195	2439	2443	2445	rBV2	870	687	0.03%	0.004%
60	9.231	2449	2454	2457	rBV4	333	312	0.01%	0.002%
61	9.263	2461	2464	2470	rBV4	415	508	0.02%	0.003%
62	9.356	2490	2493	2497	rVB3	532	415	0.02%	0.002%
63	9.385	2499	2502	2505	rVV3	393	309	0.01%	0.002%
64	9.449	2507	2522	2559	rVV	990540	1787752	78.76%	10.754%
65	9.601	2559	2569	2582	rVV	9338	15441	0.68%	0.093%
66	9.652	2582	2585	2587	rVV2	583	404	0.02%	0.002%
67	9.723	2595	2607	2634	rBV	45530	85058	3.75%	0.512%
68	9.858	2644	2649	2653	rBV2	645	606	0.03%	0.004%
69	10.060	2708	2712	2717	rBV2	491	397	0.02%	0.002%
70	10.089	2717	2721	2724	rBV3	474	376	0.02%	0.002%
71	10.131	2724	2734	2754	rVV	19597	33219	1.46%	0.200%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU110119\
 Data File : VU035591.D
 Acq On : 01 Nov 2019 10:42
 Operator : JC/SP
 Sample : K5631-01 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BE878

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
 Title : VOC Analysis

72	10.388	2810	2814	2818	rVV4	416	335	0.01%	0.002%
73	10.511	2846	2852	2861	rVB5	2342	2669	0.12%	0.016%
74	10.787	2922	2938	2957	rBV	645446	1115176	49.13%	6.708%
75	10.880	2965	2967	2972	rVB2	738	467	0.02%	0.003%
76	10.919	2972	2979	2980	rBV6	847	830	0.04%	0.005%
77	10.983	2995	2999	3004	rBV3	776	598	0.03%	0.004%
78	11.019	3004	3010	3018	rVV6	1836	2555	0.11%	0.015%
79	11.051	3018	3020	3024	rVB2	498	366	0.02%	0.002%
80	11.115	3034	3040	3045	rBV4	1556	2139	0.09%	0.013%
81	11.295	3093	3096	3098	rBV	938	582	0.03%	0.004%
82	11.498	3150	3159	3165	rVV5	1957	2953	0.13%	0.018%
83	11.584	3183	3186	3189	rBV2	444	311	0.01%	0.002%
84	11.774	3238	3245	3253	rBV4	1498	2084	0.09%	0.013%
85	11.842	3253	3266	3282	rBV	593354	1061561	46.76%	6.386%
86	11.919	3287	3290	3291	rBV	518	319	0.01%	0.002%
87	11.993	3311	3313	3317	rBV	411	358	0.02%	0.002%
88	12.031	3323	3325	3328	rVB2	668	306	0.01%	0.002%
89	12.086	3335	3342	3352	rBV4	3988	6249	0.28%	0.038%
90	12.221	3371	3384	3408	rVB	640886	1103380	48.61%	6.637%
91	12.311	3408	3412	3417	rVB3	450	486	0.02%	0.003%
92	12.353	3423	3425	3429	rBV2	427	315	0.01%	0.002%
93	12.498	3467	3470	3474	rBV2	547	517	0.02%	0.003%
94	12.613	3503	3506	3511	rBV3	586	502	0.02%	0.003%
95	12.793	3558	3562	3565	rVB4	487	348	0.02%	0.002%
96	13.047	3637	3641	3644	rBV4	696	556	0.02%	0.003%
97	13.080	3648	3651	3658	rVB3	754	546	0.02%	0.003%
98	13.237	3697	3700	3703	rBV	898	718	0.03%	0.004%
99	13.276	3710	3712	3717	rBV3	540	377	0.02%	0.002%
100	13.600	3810	3813	3815	rBV3	738	527	0.02%	0.003%


Sum of corrected areas: 16624309

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU110119\
Data File : VU035591.D
Acq On : 01 Nov 2019 10:42
Operator : JC/SP
Sample : K5631-01 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
BE878

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

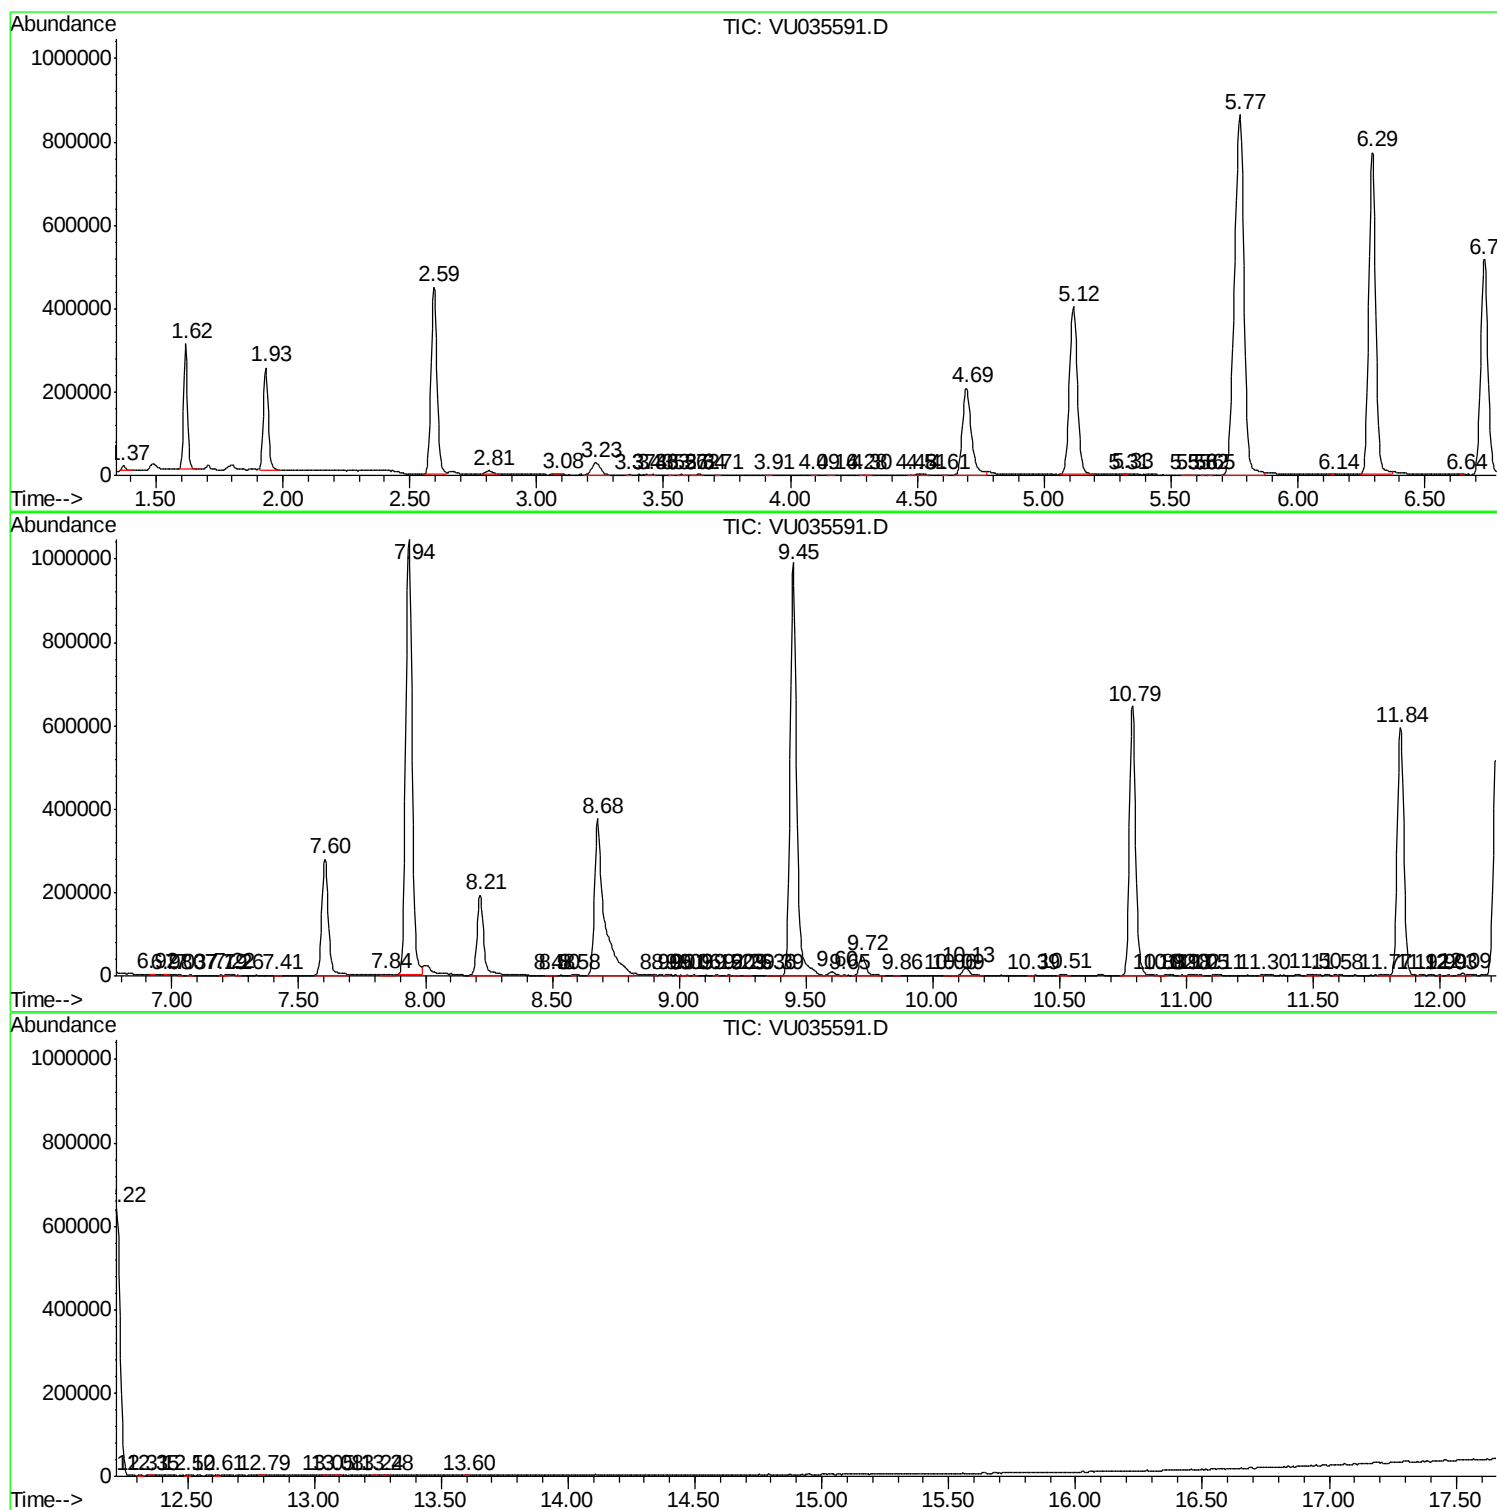

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU110119\
Data File : VU035591.D
Acq On : 01 Nov 2019 10:42
Operator : JC/SP
Sample : K5631-01 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BE878

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU110119\
Data File : VU035591.D
Acq On : 01 Nov 2019 10:42
Operator : JC/SP
Sample : K5631-01 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BE878

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc