

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU110119\
 Data File : VU035593.D
 Acq On : 01 Nov 2019 11:30
 Operator : JC/SP
 Sample : K5631-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BE890

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.617	79	86	102	rVB	293407	318173	14.11%	1.940%
2	1.935	176	185	199	rVB	241018	319654	14.18%	1.950%
3	2.488	354	357	360	rBV4	999	852	0.04%	0.005%
4	2.597	378	391	405	rBV	441369	729895	32.38%	4.452%
5	2.806	447	456	472	rBV2	12694	25495	1.13%	0.155%
6	2.999	513	516	522	rVB5	1395	1351	0.06%	0.008%
7	3.086	535	543	553	rVB5	3802	7014	0.31%	0.043%
8	3.128	553	556	560	rVB2	747	421	0.02%	0.003%
9	3.157	560	565	567	rBV4	870	746	0.03%	0.005%
10	3.231	575	588	606	rVB	17423	41578	1.84%	0.254%
11	3.395	633	639	641	rBV4	475	478	0.02%	0.003%
12	3.456	654	658	663	rVB3	734	688	0.03%	0.004%
13	3.542	683	685	693	rVB3	368	377	0.02%	0.002%
14	3.713	734	738	742	rBV2	435	363	0.02%	0.002%
15	3.877	786	789	793	rBV3	403	276	0.01%	0.002%
16	3.938	805	808	816	rVB2	317	285	0.01%	0.002%
17	4.227	894	898	904	rBV2	652	561	0.02%	0.003%
18	4.288	914	917	923	rVB	314	327	0.01%	0.002%
19	4.324	923	928	931	rBV	347	355	0.02%	0.002%
20	4.362	936	940	946	rVB3	317	263	0.01%	0.002%
21	4.459	967	970	974	rBV	456	317	0.01%	0.002%
22	4.513	984	987	993	rVB3	981	871	0.04%	0.005%
23	4.600	1009	1014	1020	rBV2	432	503	0.02%	0.003%
24	4.694	1026	1043	1062	rBV	188243	473986	21.03%	2.891%
25	5.115	1157	1174	1201	rVV	395907	894567	39.68%	5.456%
26	5.423	1261	1270	1273	rBV3	1143	1388	0.06%	0.008%
27	5.449	1275	1278	1282	rVB3	615	436	0.02%	0.003%
28	5.620	1329	1331	1334	rVV3	403	264	0.01%	0.002%
29	5.771	1354	1378	1415	rBV2	850736	2254218	100.00%	13.748%
30	6.153	1493	1497	1501	rBV5	1082	1013	0.04%	0.006%
31	6.234	1520	1522	1525	rBV3	473	296	0.01%	0.002%
32	6.292	1525	1540	1575	rBV	760776	1485458	65.90%	9.060%
33	6.539	1614	1617	1619	rBV3	1098	601	0.03%	0.004%
34	6.584	1622	1631	1637	rBV3	5860	11532	0.51%	0.070%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU110119\
 Data File : VU035593.D
 Acq On : 01 Nov 2019 11:30
 Operator : JC/SP
 Sample : K5631-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BE890

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
 Title : VOC Analysis

35	6.735	1663	1678	1703	rBV	504198	1014290	45.00%	6.186%
36	7.009	1756	1763	1775	rVB6	4239	7337	0.33%	0.045%
37	7.118	1790	1797	1801	rBV3	882	1050	0.05%	0.006%
38	7.173	1811	1814	1817	rBV3	641	539	0.02%	0.003%
39	7.218	1823	1828	1836	rVB6	2266	3003	0.13%	0.018%
40	7.369	1872	1875	1879	rVB3	620	454	0.02%	0.003%
41	7.398	1879	1884	1890	rVB2	755	1053	0.05%	0.006%
42	7.430	1890	1894	1898	rBV4	836	821	0.04%	0.005%
43	7.468	1903	1906	1911	rBV2	439	423	0.02%	0.003%
44	7.507	1914	1918	1920	rBV2	521	372	0.02%	0.002%
45	7.603	1934	1948	1974	rBV	267064	500910	22.22%	3.055%
46	7.841	2013	2022	2030	rBV3	6956	12072	0.54%	0.074%
47	7.935	2037	2051	2090	rBV	1012761	1845959	81.89%	11.258%
48	8.214	2125	2138	2161	rBV	179320	341797	15.16%	2.085%
49	8.414	2195	2200	2205	rBV5	599	695	0.03%	0.004%
50	8.443	2207	2209	2213	rVB2	477	267	0.01%	0.002%
51	8.500	2219	2227	2238	rBV5	2169	4213	0.19%	0.026%
52	8.584	2248	2253	2261	rVB6	2282	3055	0.14%	0.019%
53	8.616	2261	2263	2270	rVB3	443	431	0.02%	0.003%
54	8.684	2270	2284	2326	rBV	278044	955918	42.41%	5.830%
55	8.944	2364	2365	2370	rVB3	677	389	0.02%	0.002%
56	9.205	2441	2446	2449	rBV5	623	632	0.03%	0.004%
57	9.240	2455	2457	2460	rVB2	482	283	0.01%	0.002%
58	9.285	2468	2471	2475	rVB2	589	377	0.02%	0.002%
59	9.449	2507	2522	2562	rBV	969585	1797252	79.73%	10.961%
60	9.597	2564	2568	2575	rBV2	742	809	0.04%	0.005%
61	9.671	2589	2591	2594	rBV	564	299	0.01%	0.002%
62	9.719	2600	2606	2617	rVB6	1948	3639	0.16%	0.022%
63	10.134	2731	2735	2738	rBV4	786	705	0.03%	0.004%
64	10.172	2745	2747	2753	rVB2	647	467	0.02%	0.003%
65	10.221	2759	2762	2767	rBV	383	287	0.01%	0.002%
66	10.262	2770	2775	2779	rVB2	566	527	0.02%	0.003%
67	10.291	2780	2784	2790	rBV3	452	587	0.03%	0.004%
68	10.343	2795	2800	2804	rBV4	422	378	0.02%	0.002%
69	10.362	2804	2806	2810	rBV2	407	310	0.01%	0.002%
70	10.497	2846	2848	2850	rBV2	556	308	0.01%	0.002%
71	10.610	2880	2883	2884	rBV	712	428	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU110119\
 Data File : VU035593.D
 Acq On : 01 Nov 2019 11:30
 Operator : JC/SP
 Sample : K5631-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BE890

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
 Title : VOC Analysis

72	10.787	2924	2938	2964	rVB	628695	1095026	48.58%	6.678%
73	10.893	2964	2971	2974	rBV4	790	973	0.04%	0.006%
74	10.918	2974	2979	2987	rBV5	2422	3450	0.15%	0.021%
75	11.073	3021	3027	3029	rBV3	488	444	0.02%	0.003%
76	11.111	3036	3039	3042	rBV2	747	582	0.03%	0.004%
77	11.176	3053	3059	3060	rBV	524	397	0.02%	0.002%
78	11.278	3088	3091	3092	rBV2	503	274	0.01%	0.002%
79	11.433	3136	3139	3143	rBV2	615	519	0.02%	0.003%
80	11.494	3153	3158	3159	rBV3	1326	1016	0.05%	0.006%
81	11.735	3230	3233	3239	rVB5	385	349	0.02%	0.002%
82	11.777	3240	3246	3252	rBV4	1272	1615	0.07%	0.010%
83	11.844	3252	3267	3282	rBV	615292	1087805	48.26%	6.634%
84	11.957	3299	3302	3305	rBV3	568	406	0.02%	0.002%
85	12.089	3335	3343	3355	rVB4	5766	9493	0.42%	0.058%
86	12.140	3356	3359	3362	rBV2	406	324	0.01%	0.002%
87	12.224	3371	3385	3400	rBV	645866	1111753	49.32%	6.780%
88	12.327	3414	3417	3419	rBV3	434	280	0.01%	0.002%
89	12.378	3430	3433	3436	rBV2	528	297	0.01%	0.002%
90	12.423	3445	3447	3450	rBV	400	267	0.01%	0.002%
91	12.487	3462	3467	3470	rBV4	508	574	0.03%	0.004%
92	12.561	3488	3490	3494	rVB3	490	267	0.01%	0.002%
93	12.600	3499	3502	3504	rBV	532	299	0.01%	0.002%
94	12.680	3524	3527	3530	rBV	439	359	0.02%	0.002%
95	13.098	3655	3657	3660	rBV2	542	398	0.02%	0.002%
96	13.195	3684	3687	3688	rBV2	542	327	0.01%	0.002%
97	13.783	3868	3870	3875	rBV4	671	418	0.02%	0.003%
98	13.909	3907	3909	3913	rBV	714	488	0.02%	0.003%
99	14.195	3996	3998	4000	rBV2	697	337	0.01%	0.002%
100	14.510	4094	4096	4099	rBV3	1041	771	0.03%	0.005%


Sum of corrected areas: 16396446

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU110119\
Data File : VU035593.D
Acq On : 01 Nov 2019 11:30
Operator : JC/SP
Sample : K5631-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
BE890

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

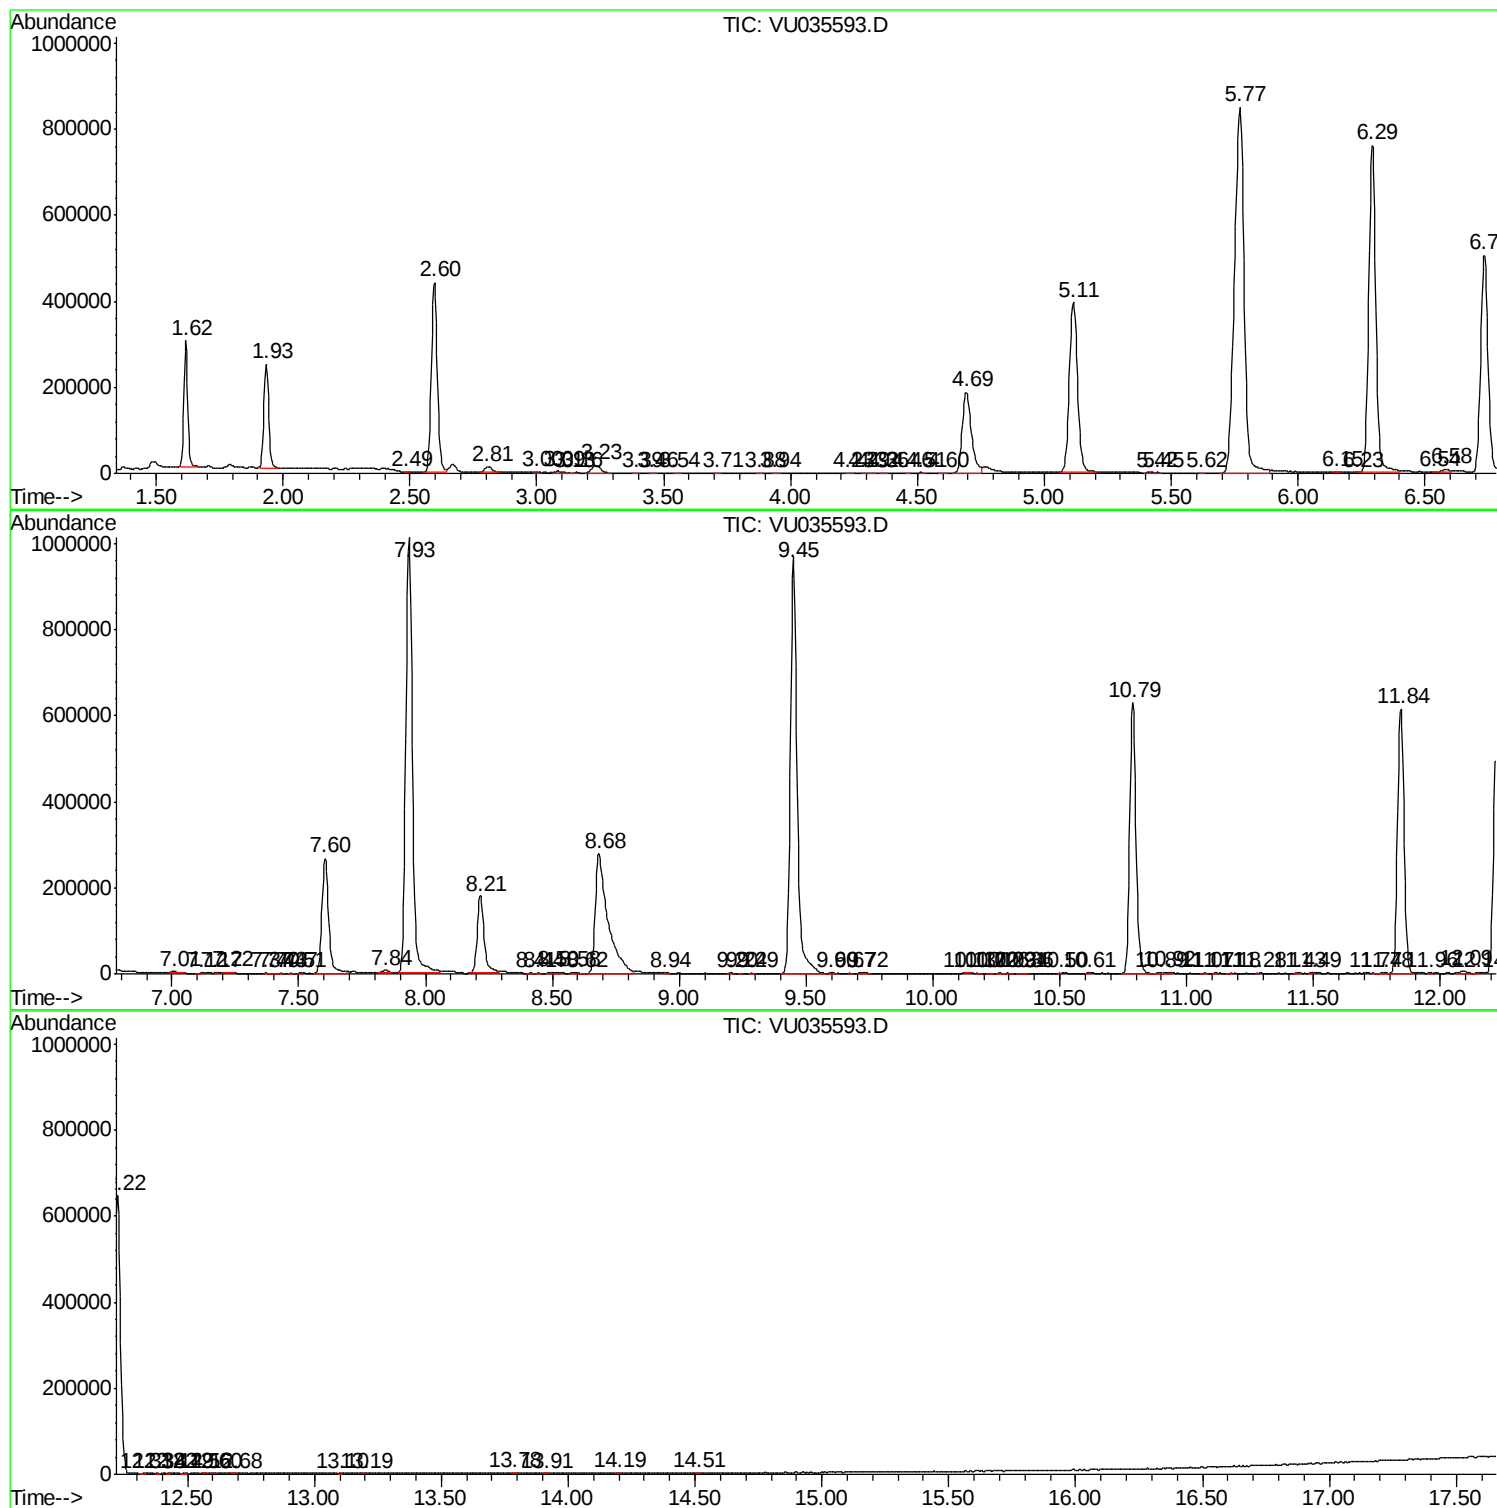

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU110119\
Data File : VU035593.D
Acq On : 01 Nov 2019 11:30
Operator : JC/SP
Sample : K5631-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BE890

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU110119\
Data File : VU035593.D
Acq On : 01 Nov 2019 11:30
Operator : JC/SP
Sample : K5631-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BE890

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc