


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110119\
 Data File : VU035581.D
 Acq On : 31 Oct 2019 08:17
 Operator : JC/SP
 Sample : BFB48
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB48

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
 Title : VOC Analysis
 Last Update : Fri Nov 01 17:03:18 2019

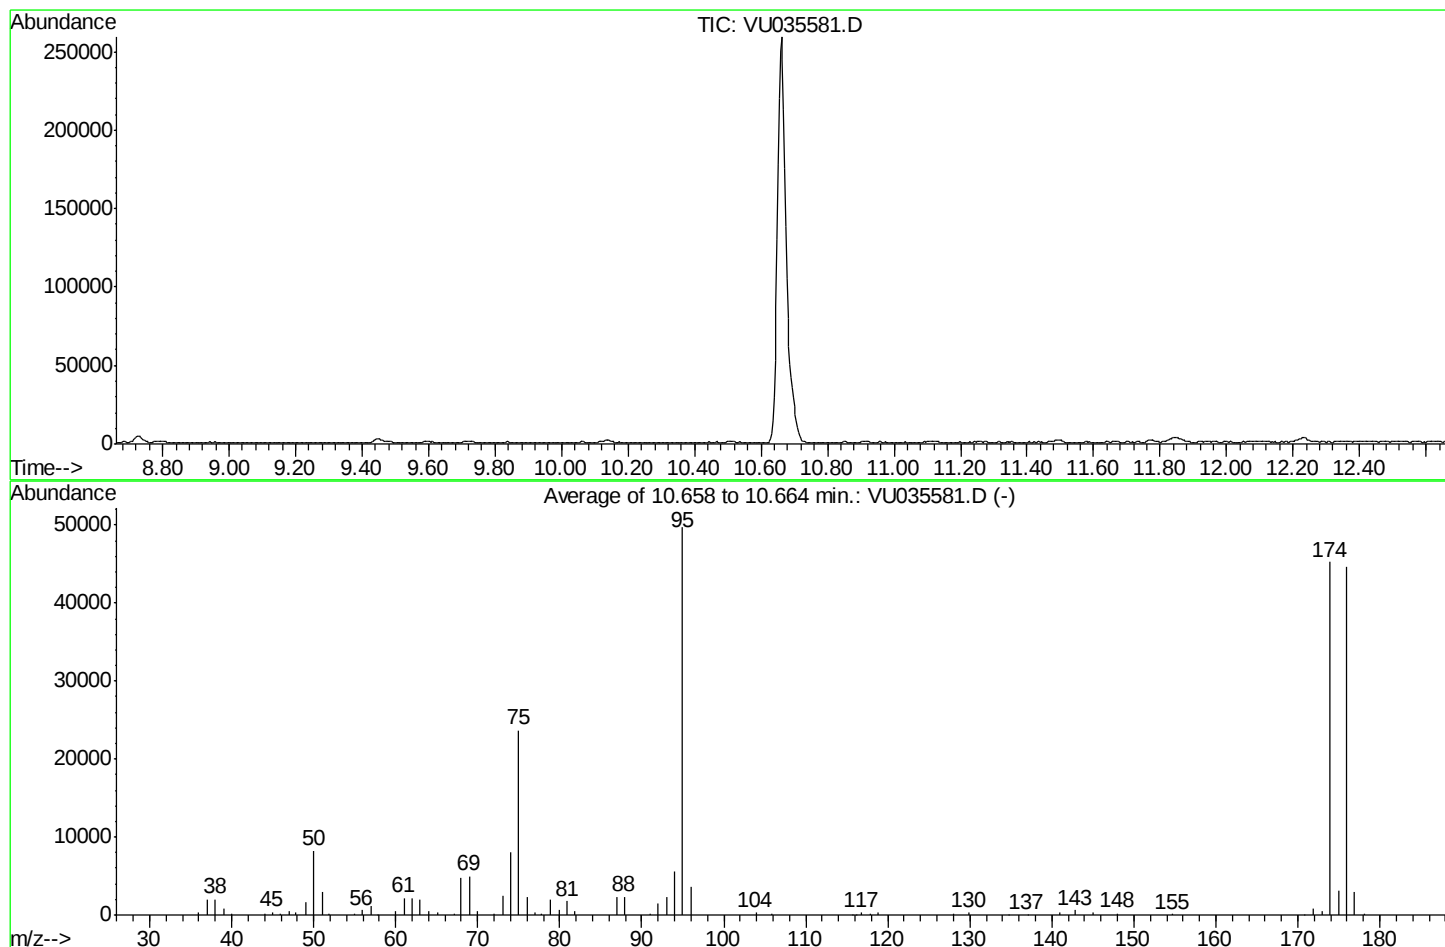

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2886

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	8229	PASS
75	95	30	80	47.7	23712	PASS
95	95	100	100	100.0	49714	PASS
96	95	5	9	7.4	3694	PASS
173	174	0.00	2	1.2	536	PASS
174	95	50	120	91.0	45232	PASS
175	174	5	9	7.0	3166	PASS
176	174	95	101	98.7	44656	PASS
177	176	5	9	6.8	3035	PASS

m/z	Abundance
35.90	229.0
37.00	1872.0
38.00	1905.0
39.00	766.0
40.00	312.0
44.00	1030.0
44.90	330.0
45.90	127.0
47.00	446.0
47.80	346.0
49.00	1563.0
50.00	7947.0
51.00	2826.0
51.90	116.0
54.90	206.0
55.90	625.0
57.10	1028.0
60.00	367.0
61.00	2160.0
62.00	2115.0
63.00	1810.0
64.00	352.0
65.10	361.0
67.00	180.0
68.00	4613.0
69.00	4928.0
69.90	326.0
72.00	255.0
73.00	2336.0
74.00	7552.0
75.00	22408.0
76.00	1974.0
77.00	363.0
77.80	217.0
78.90	1819.0
80.00	589.0
80.90	1771.0
81.90	413.0
86.90	2082.0
87.90	2218.0
90.90	213.0
92.00	1442.0
93.00	2160.0
94.00	5487.0
95.00	48728.0
96.00	3371.0
103.90	231.0
105.80	231.0
116.10	116.0
116.80	262.0
117.80	143.0
118.80	311.0
128.00	125.0
130.00	217.0
140.90	438.0
142.90	644.0
144.90	292.0
148.00	156.0
154.70	111.0
170.70	130.0
171.90	816.0
173.00	537.0
173.90	44904.0
175.00	3121.0
175.90	44440.0
176.90	2962.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
36.00	346.0
37.00	1928.0
38.00	2018.0
39.00	785.0
40.10	289.0
44.00	915.0
45.00	386.0
46.00	120.0
47.00	609.0
47.90	355.0
49.00	1683.0
50.00	8345.0
51.00	3101.0
51.90	145.0
55.00	211.0
55.90	672.0
57.00	1189.0
57.80	101.0
60.00	477.0
61.00	2213.0
62.00	2139.0
63.00	1890.0
64.00	489.0
65.00	461.0
67.20	136.0
68.00	4893.0
69.00	4884.0
70.00	521.0
72.10	199.0
73.00	2634.0
74.00	8139.0
75.00	24216.0
76.10	2418.0
77.00	332.0
77.80	263.0
78.90	2148.0
80.00	703.0
80.90	1750.0
81.80	414.0
87.00	2309.0
87.90	2423.0
91.00	226.0
92.00	1410.0
93.00	2214.0
94.00	5583.0
95.00	49232.0
96.00	3857.0
103.90	322.0
105.80	237.0
115.70	146.0
116.90	359.0
117.80	170.0
118.90	270.0
128.00	100.0
129.90	290.0
134.70	110.0
137.00	105.0
141.00	368.0
142.90	639.0
145.00	251.0
148.00	176.0
154.90	157.0
171.90	685.0
173.00	537.0
173.90	44288.0
174.90	3114.0
175.90	43400.0
176.90	2987.0
178.10	163.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

Scan 2886 (10.619 min): VU035581.D
BFB48

m/z	Abundance
40.00	201.0
44.00	799.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
36.00	297.0
37.00	2019.0
38.00	2042.0
39.00	836.0
40.00	283.0
44.00	977.0
44.90	386.0
45.90	149.0
47.10	525.0
47.80	370.0
49.00	1680.0
50.00	8397.0
51.00	3000.0
51.90	161.0
54.90	235.0
55.90	651.0
57.10	1132.0
60.00	464.0
61.00	2269.0
62.00	2277.0
63.00	1984.0
64.00	451.0
65.00	407.0
67.10	184.0
68.00	4854.0
69.00	5190.0
70.00	407.0
72.00	231.0
73.00	2636.0
74.00	8334.0
75.00	24512.0
76.10	2344.0
77.00	357.0
77.80	267.0
78.90	2134.0
80.00	716.0
80.90	1866.0
81.80	427.0
87.00	2356.0
87.90	2431.0
90.90	222.0
92.00	1451.0
93.00	2346.0
94.00	5748.0
95.00	51184.0
96.00	3855.0
103.90	312.0
105.80	233.0
115.60	116.0
116.10	119.0
116.80	322.0
117.80	158.0
118.80	287.0
128.00	121.0
129.90	260.0
137.00	107.0
141.00	411.0
142.90	675.0
144.90	292.0
148.00	190.0
154.70	131.0
170.80	132.0
171.90	818.0
173.00	535.0
173.90	46504.0
174.90	3264.0
175.90	46128.0
176.90	3157.0
178.10	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48