


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU110119\
 Data File : VU035587.D
 Acq On : 01 Nov 2019 08:52
 Operator : JC/SP
 Sample : BFB49
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB49

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
 Title : VOC Analysis
 Last Update : Fri Nov 01 17:03:18 2019

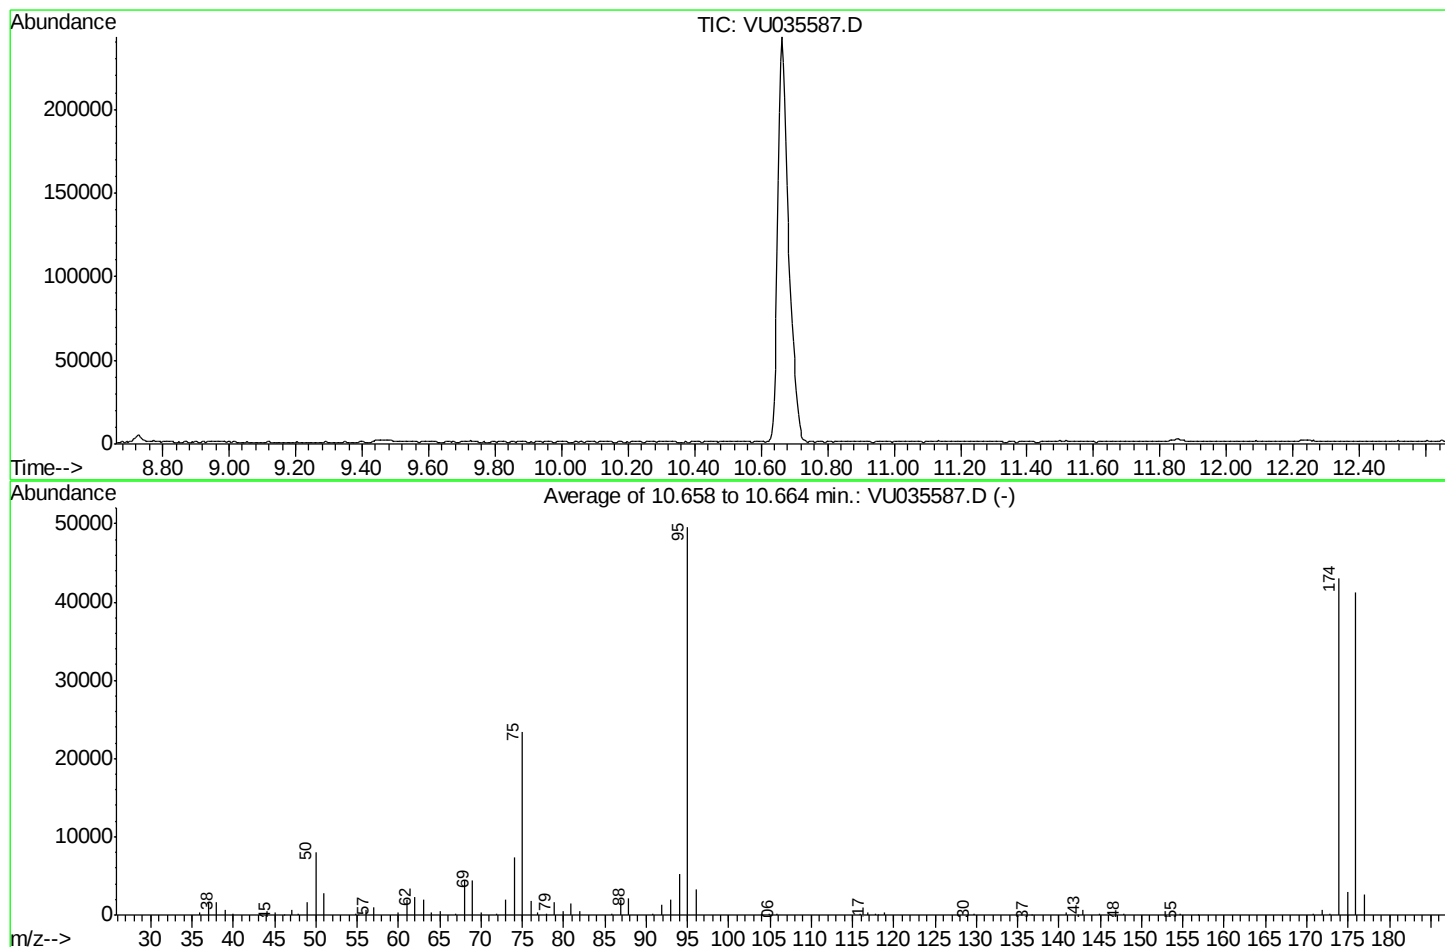

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2886

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	8043	PASS
75	95	30	80	47.2	23386	PASS
95	95	100	100	100.0	49544	PASS
96	95	5	9	6.5	3201	PASS
173	174	0.00	2	0.4	165	PASS
174	95	50	120	86.7	42962	PASS
175	174	5	9	7.0	2998	PASS
176	174	95	101	95.9	41184	PASS
177	176	5	9	6.3	2576	PASS

Scan 2886 (10.619 min): VU035587.D
BFB49

m/z	Abundance
39.90	230.0
44.00	1057.0
73.10	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
35.90	316.0
36.90	1555.0
38.00	1596.0
38.90	776.0
39.90	374.0
44.00	1078.0
45.00	382.0
47.10	540.0
47.90	270.0
49.00	1786.0
50.00	8389.0
51.00	2784.0
55.20	104.0
56.00	648.0
57.00	948.0
60.10	262.0
61.00	1965.0
62.00	2146.0
63.00	1762.0
64.00	348.0
65.00	486.0
66.90	231.0
68.00	4292.0
69.00	4639.0
70.00	276.0
71.80	224.0
73.00	1937.0
74.00	7193.0
75.00	23240.0
76.00	1700.0
76.90	385.0
77.80	269.0
78.90	1498.0
79.90	602.0
80.90	1549.0
81.90	476.0
85.90	141.0
86.90	1879.0
87.90	2208.0
90.80	163.0
92.00	1339.0
93.00	1948.0
94.00	5608.0
95.00	50256.0
96.00	3312.0
103.90	189.0
104.80	128.0
105.90	239.0
115.90	181.0
116.90	373.0
117.80	186.0
118.90	375.0
129.70	192.0
136.70	100.0
140.90	403.0
142.90	789.0
144.90	189.0
147.80	137.0
171.90	632.0
173.90	44704.0
174.90	3089.0
175.90	42720.0
176.90	2681.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
35.90	339.0
36.90	1708.0
37.90	1728.0
39.00	701.0
39.90	388.0
44.00	1138.0
45.00	384.0
46.10	102.0
47.10	626.0
47.80	249.0
49.00	1669.0
50.00	8251.0
51.00	2862.0
54.80	143.0
55.20	112.0
56.00	714.0
57.00	1065.0
59.80	257.0
60.10	256.0
61.00	1928.0
62.00	2243.0
63.00	2010.0
63.90	393.0
65.00	503.0
66.90	171.0
68.00	4486.0
69.00	4579.0
70.00	289.0
71.90	203.0
73.00	2071.0
74.00	7486.0
75.00	23944.0
76.00	1871.0
76.80	355.0
77.80	229.0
78.90	1626.0
79.90	562.0
80.90	1565.0
81.90	505.0
85.80	159.0
86.90	1911.0
87.90	2232.0
90.80	155.0
91.90	1387.0
93.00	1900.0
94.00	5383.0
95.00	50936.0
96.00	3272.0
103.90	224.0
104.80	135.0
105.80	227.0
116.00	219.0
116.90	402.0
117.80	160.0
118.90	313.0
127.70	106.0
129.70	204.0
140.90	405.0
142.90	790.0
145.00	196.0
147.80	184.0
154.70	135.0
156.90	117.0
170.80	129.0
171.90	604.0
174.00	43696.0
174.90	3042.0
175.90	42304.0
176.90	2599.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
35.90	309.0
37.00	1717.0
37.90	1770.0
39.00	659.0
39.90	363.0
44.00	1140.0
45.00	416.0
47.10	621.0
47.90	223.0
49.00	1553.0
50.00	7490.0
51.00	2646.0
54.80	181.0
56.00	667.0
57.00	1180.0
60.00	280.0
61.00	1806.0
62.00	2271.0
63.00	2018.0
63.90	387.0
65.00	439.0
66.90	129.0
68.00	4526.0
69.00	4107.0
70.10	268.0
72.00	172.0
73.00	2098.0
74.00	7395.0
75.00	22976.0
76.00	1952.0
76.80	322.0
78.00	172.0
78.90	1622.0
79.90	483.0
80.80	1442.0
81.90	490.0
85.80	125.0
86.90	1917.0
87.90	2004.0
90.70	134.0
92.00	1305.0
93.00	1882.0
94.00	4938.0
95.00	47440.0
96.00	3019.0
103.90	241.0
104.90	104.0
105.80	216.0
116.00	220.0
116.90	355.0
117.80	129.0
118.10	120.0
118.80	314.0
127.70	146.0
129.70	202.0
140.80	394.0
142.90	632.0
144.90	193.0
147.80	157.0
154.70	170.0
156.80	122.0
170.90	201.0
171.90	553.0
172.80	496.0
173.90	40488.0
175.00	2864.0
175.90	38528.0
176.90	2448.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49