

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110121\
 Data File : VU045481.D
 Acq On : 01 Nov 2021 11:37
 Operator : SY/MD
 Sample : VU1101WBL03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK036

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M

Title : VOC Analysis

Signal : TIC: VU045481.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	96	rVB	159714	175333	13.51%	1.726%
2	1.916	170	179	196	rBV	135248	173471	13.37%	1.707%
3	2.572	370	383	408	rBV	255879	429188	33.08%	4.224%
4	2.713	424	427	430	rBV	112	80	0.01%	0.001%
5	2.797	445	453	462	rBV2	1371	2193	0.17%	0.022%
6	2.935	492	496	497	rBV2	143	106	0.01%	0.001%
7	3.051	526	532	542	rVB2	1175	1823	0.14%	0.018%
8	3.202	576	579	582	rVB2	265	194	0.01%	0.002%
9	3.231	582	588	590	rBV2	180	196	0.02%	0.002%
10	3.244	590	592	598	rVV2	87	93	0.01%	0.001%
11	3.292	604	607	610	rBV2	164	122	0.01%	0.001%
12	3.359	623	628	633	rVB2	701	770	0.06%	0.008%
13	3.549	682	687	692	rBV2	167	236	0.02%	0.002%
14	3.575	692	695	699	rVV2	116	90	0.01%	0.001%
15	3.658	717	721	729	rBV2	98	154	0.01%	0.002%
16	3.758	749	752	754	rBV	155	120	0.01%	0.001%
17	3.842	773	778	781	rBV2	125	132	0.01%	0.001%
18	3.861	781	784	788	rVB2	138	104	0.01%	0.001%
19	3.928	802	805	809	rBV	154	117	0.01%	0.001%
20	3.970	815	818	824	rVV	85	87	0.01%	0.001%
21	4.228	894	898	905	rVB2	135	178	0.01%	0.002%
22	4.395	944	950	957	rBV	171	342	0.03%	0.003%
23	4.633	1009	1024	1063	rBV	142217	365085	28.14%	3.594%
24	4.858	1091	1094	1101	rBV2	241	296	0.02%	0.003%
25	4.922	1112	1114	1116	rBV2	167	107	0.01%	0.001%
26	4.941	1117	1120	1125	rVB3	277	267	0.02%	0.003%
27	5.070	1143	1160	1182	rBV	230729	498670	38.44%	4.908%
28	5.205	1200	1202	1205	rVV	214	102	0.01%	0.001%
29	5.224	1205	1208	1210	rVV	192	84	0.01%	0.001%
30	5.234	1210	1211	1216	rVV	167	95	0.01%	0.001%
31	5.292	1223	1229	1241	rVB3	533	1003	0.08%	0.010%
32	5.359	1246	1250	1256	rBV2	445	440	0.03%	0.004%
33	5.391	1256	1260	1263	rBV	254	141	0.01%	0.001%
34	5.594	1320	1323	1327	rBV2	112	124	0.01%	0.001%
35	5.729	1342	1365	1397	rBV2	479785	1297379	100.00%	12.770%
36	6.108	1479	1483	1484	rBV	211	121	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110121\
 Data File : VU045481.D
 Acq On : 01 Nov 2021 11:37
 Operator : SY/MD
 Sample : VU1101WBL03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK036

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
 Title : VOC Analysis

37	6.195	1507	1510	1511	rBV2	309	184	0.01%	0.002%
38	6.253	1512	1528	1549	rVV	398238	756552	58.31%	7.447%
39	6.536	1606	1616	1630	rVB5	2540	4550	0.35%	0.045%
40	6.620	1637	1642	1645	rBV	149	155	0.01%	0.002%
41	6.697	1650	1666	1688	rBV	308003	593240	45.73%	5.839%
42	6.813	1696	1702	1711	rBV3	685	1017	0.08%	0.010%
43	7.044	1766	1774	1785	rVB4	772	1289	0.10%	0.013%
44	7.092	1785	1789	1792	rBV	156	138	0.01%	0.001%
45	7.186	1810	1818	1826	rBV3	3124	5038	0.39%	0.050%
46	7.449	1896	1900	1903	rBV	191	148	0.01%	0.001%
47	7.568	1923	1937	1959	rBV	178270	307635	23.71%	3.028%
48	7.687	1966	1974	1985	rVB4	2260	3570	0.28%	0.035%
49	7.800	2004	2009	2015	rBV	579	617	0.05%	0.006%
50	7.903	2026	2041	2056	rBV	588092	1011801	77.99%	9.959%
51	7.973	2058	2063	2076	rVB	9689	15898	1.23%	0.156%
52	8.182	2117	2128	2144	rBV	123035	204108	15.73%	2.009%
53	8.472	2213	2218	2219	rBV3	249	204	0.02%	0.002%
54	8.523	2230	2234	2236	rBV	142	104	0.01%	0.001%
55	8.555	2241	2244	2248	rVB3	254	211	0.02%	0.002%
56	8.636	2256	2269	2305	rBV	455621	761656	58.71%	7.497%
57	8.848	2332	2335	2338	rBV2	181	161	0.01%	0.002%
58	8.922	2355	2358	2362	rBV3	270	243	0.02%	0.002%
59	9.295	2469	2474	2478	rBV2	182	170	0.01%	0.002%
60	9.420	2500	2513	2533	rBV	561621	934435	72.02%	9.198%
61	9.546	2549	2552	2554	rBV	171	113	0.01%	0.001%
62	9.571	2554	2560	2561	rBV	1139	835	0.06%	0.008%
63	9.694	2592	2598	2610	rBV4	1643	2897	0.22%	0.029%
64	9.819	2634	2637	2639	rBV	170	116	0.01%	0.001%
65	10.031	2700	2703	2708	rBV2	159	147	0.01%	0.001%
66	10.115	2721	2729	2738	rVB5	1680	2833	0.22%	0.028%
67	10.491	2838	2846	2852	rBV4	1074	1364	0.11%	0.013%
68	10.578	2870	2873	2878	rBV2	121	122	0.01%	0.001%
69	10.639	2886	2892	2897	rBV3	908	1272	0.10%	0.013%
70	10.674	2897	2903	2913	rVB	3025	4230	0.33%	0.042%
71	10.761	2913	2930	2946	rBV	419676	672778	51.86%	6.622%
72	10.829	2948	2951	2958	rVV4	837	740	0.06%	0.007%
73	10.870	2958	2964	2968	rVV4	757	807	0.06%	0.008%
74	10.893	2968	2971	2977	rVB4	738	778	0.06%	0.008%
75	10.970	2992	2995	3001	rBV2	177	184	0.01%	0.002%
76	11.092	3027	3033	3036	rBV2	1008	1124	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110121\
 Data File : VU045481.D
 Acq On : 01 Nov 2021 11:37
 Operator : SY/MD
 Sample : VU1101WBL03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK036

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
 Title : VOC Analysis

77	11.153	3050	3052	3057	rVB3	331	155	0.01%	0.002%
78	11.195	3062	3065	3068	rBV2	150	105	0.01%	0.001%
79	11.211	3068	3070	3075	rVB2	196	138	0.01%	0.001%
80	11.465	3140	3149	3160	rVB5	2630	4836	0.37%	0.048%
81	11.539	3169	3172	3175	rBV	154	105	0.01%	0.001%
82	11.584	3184	3186	3191	rVB2	422	274	0.02%	0.003%
83	11.703	3217	3223	3229	rVB3	1257	1445	0.11%	0.014%
84	11.751	3231	3238	3245	rVB4	1802	2581	0.20%	0.025%
85	11.816	3245	3258	3280	rBV	607119	945299	72.86%	9.305%
86	11.915	3285	3289	3290	rBV3	181	118	0.01%	0.001%
87	12.060	3332	3334	3336	rBV	207	97	0.01%	0.001%
88	12.073	3336	3338	3341	rVV	206	99	0.01%	0.001%
89	12.198	3361	3377	3394	rBV	580946	933662	71.97%	9.190%
90	12.337	3416	3420	3424	rBV4	544	543	0.04%	0.005%
91	12.398	3437	3439	3444	rBV2	434	289	0.02%	0.003%
92	12.774	3548	3556	3562	rVB	623	844	0.07%	0.008%
93	13.002	3623	3627	3628	rBV2	463	237	0.02%	0.002%
94	13.221	3690	3695	3704	rVB5	1990	2609	0.20%	0.026%
95	13.844	3882	3889	3897	rBV3	4079	5533	0.43%	0.054%
96	14.092	3955	3966	3980	rBV2	6874	10313	0.79%	0.102%
97	14.279	4021	4024	4025	rBV2	258	150	0.01%	0.001%
98	14.333	4034	4041	4051	rVB4	4027	5976	0.46%	0.059%
99	14.398	4058	4061	4066	rBV2	262	166	0.01%	0.002%
100	14.584	4111	4119	4126	rBV2	828	1484	0.11%	0.015%




Sum of corrected areas: 10159565

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110121\
Data File : VU045481.D
Acq On : 01 Nov 2021 11:37
Operator : SY/MD
Sample : VU1101WBL03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK036

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

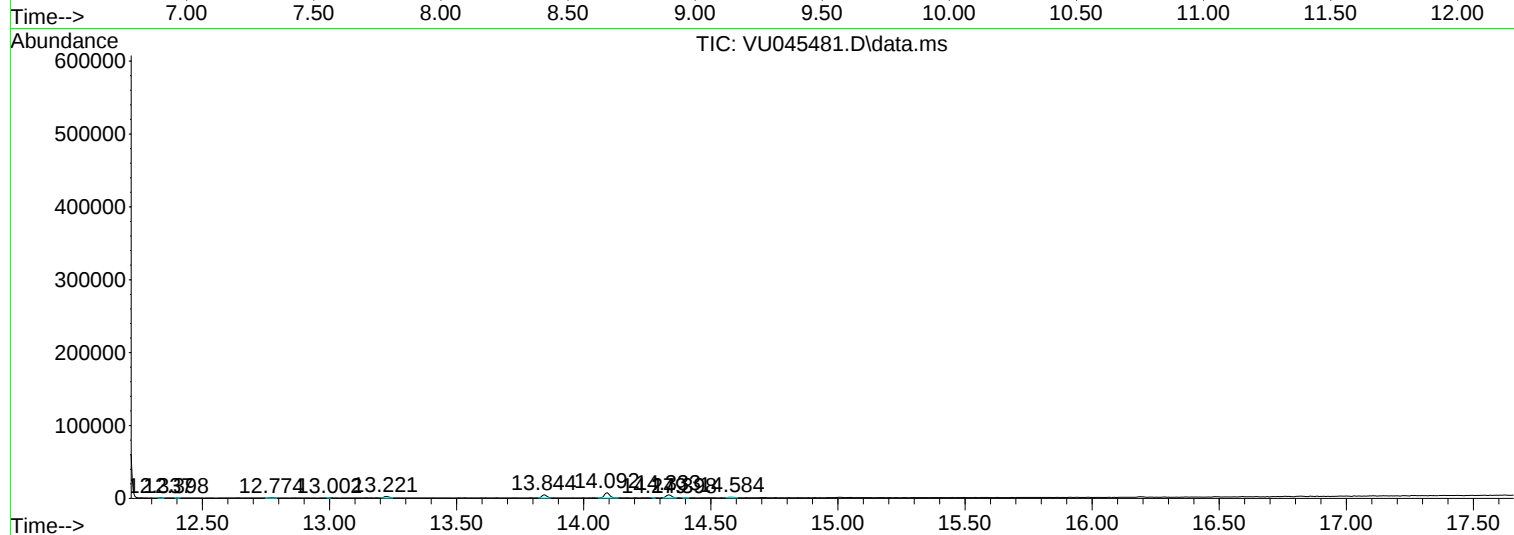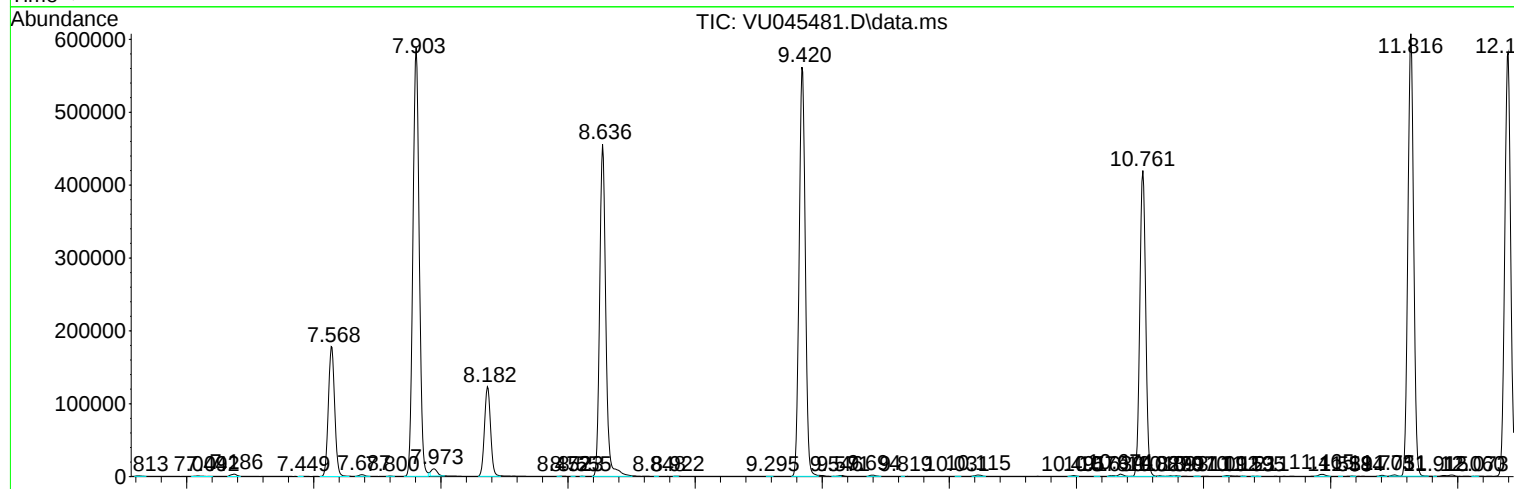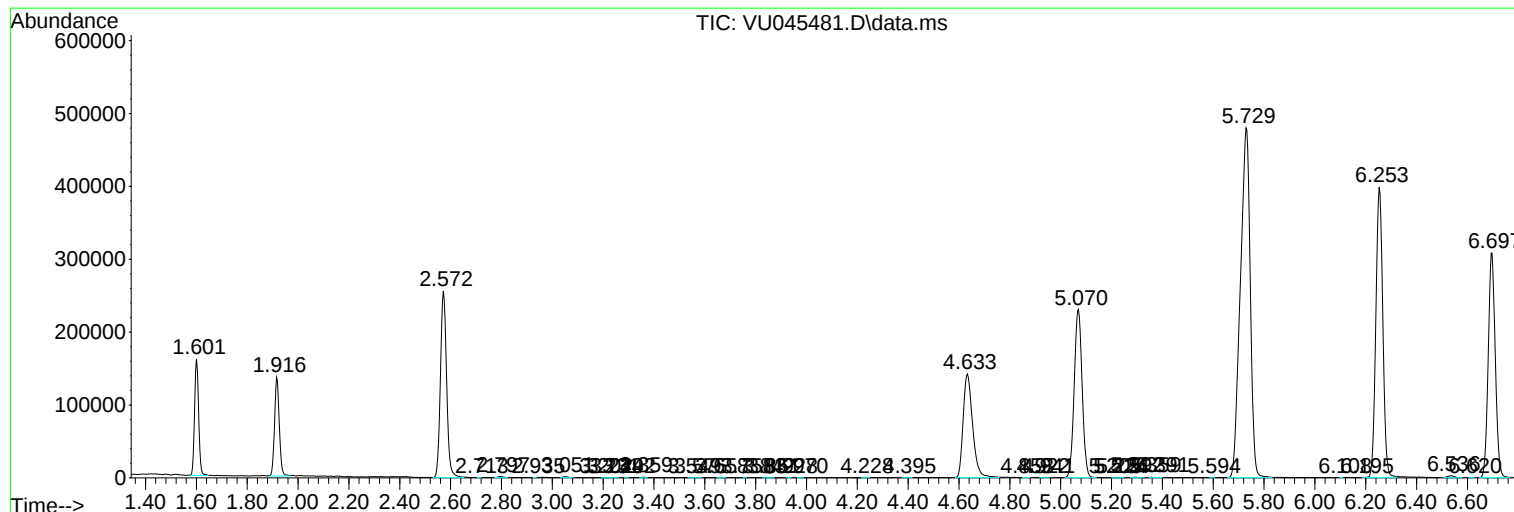

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110121\
Data File : VU045481.D
Acq On : 01 Nov 2021 11:37
Operator : SY/MD
Sample : VU1101WBL03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK036

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110121\
Data File : VU045481.D
Acq On : 01 Nov 2021 11:37
Operator : SY/MD
Sample : VU1101WBL03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK036

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc