

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110121\
 Data File : VU045482.D
 Acq On : 01 Nov 2021 12:00
 Operator : SY/MD
 Sample : VU1101WBL04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK037

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M

Title : VOC Analysis

Signal : TIC: VU045482.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	93	rBV	153206	167635	13.10%	1.686%
2	1.916	170	179	194	rVB	130911	164590	12.87%	1.655%
3	2.572	370	383	409	rBV	250908	416631	32.57%	4.190%
4	2.752	436	439	441	rBV	136	77	0.01%	0.001%
5	2.768	441	444	446	rVV	118	77	0.01%	0.001%
6	2.797	446	453	461	rVB2	958	1544	0.12%	0.016%
7	2.919	488	491	494	rBV2	146	104	0.01%	0.001%
8	2.954	496	502	503	rBV2	222	212	0.02%	0.002%
9	3.006	513	518	520	rBV2	145	149	0.01%	0.001%
10	3.051	526	532	533	rBV5	904	972	0.08%	0.010%
11	3.160	563	566	570	rVB2	173	155	0.01%	0.002%
12	3.186	570	574	580	rBV2	189	277	0.02%	0.003%
13	3.260	591	597	599	rBV	143	182	0.01%	0.002%
14	3.301	608	610	615	rBV2	122	117	0.01%	0.001%
15	3.356	623	627	629	rBV	249	148	0.01%	0.001%
16	3.391	636	638	640	rBV	131	92	0.01%	0.001%
17	3.481	660	666	671	rBV2	170	205	0.02%	0.002%
18	3.571	690	694	699	rVB2	224	242	0.02%	0.002%
19	3.600	699	703	705	rBV2	191	163	0.01%	0.002%
20	3.806	764	767	768	rBV	135	72	0.01%	0.001%
21	4.150	870	874	879	rBV	217	264	0.02%	0.003%
22	4.514	982	987	991	rBV2	132	125	0.01%	0.001%
23	4.629	1007	1023	1050	rBV	141653	350328	27.38%	3.523%
24	4.977	1127	1131	1134	rVB2	187	83	0.01%	0.001%
25	4.996	1134	1137	1142	rBB2	181	90	0.01%	0.001%
26	5.067	1142	1159	1183	rBV	224596	488988	38.22%	4.918%
27	5.176	1190	1193	1195	rBV	143	109	0.01%	0.001%
28	5.208	1200	1203	1205	rBV	214	171	0.01%	0.002%
29	5.298	1226	1231	1236	rVB3	392	484	0.04%	0.005%
30	5.395	1258	1261	1264	rVB2	149	93	0.01%	0.001%
31	5.729	1342	1365	1395	rBV2	472804	1279306	100.00%	12.866%
32	5.858	1402	1405	1409	rVB3	312	184	0.01%	0.002%
33	5.964	1435	1438	1440	rBV2	225	184	0.01%	0.002%
34	6.009	1449	1452	1454	rVB	158	94	0.01%	0.001%
35	6.031	1454	1459	1460	rBV2	295	175	0.01%	0.002%
36	6.060	1466	1468	1471	rVB	272	114	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110121\
 Data File : VU045482.D
 Acq On : 01 Nov 2021 12:00
 Operator : SY/MD
 Sample : VU1101WBL04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK037

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
 Title : VOC Analysis

37	6.079	1471	1474	1479	rBV2	137	112	0.01%	0.001%
38	6.121	1481	1487	1493	rVV2	232	286	0.02%	0.003%
39	6.186	1502	1507	1508	rBV	226	166	0.01%	0.002%
40	6.253	1513	1528	1550	rBV	397517	745252	58.25%	7.495%
41	6.452	1588	1590	1591	rBV	239	77	0.01%	0.001%
42	6.523	1606	1612	1614	rBV3	2099	2005	0.16%	0.020%
43	6.694	1650	1665	1688	rBV	304938	583789	45.63%	5.871%
44	6.806	1693	1700	1706	rBV5	696	917	0.07%	0.009%
45	6.858	1713	1716	1721	rBV	104	80	0.01%	0.001%
46	7.028	1763	1769	1770	rBV	517	469	0.04%	0.005%
47	7.041	1770	1773	1785	rVB	767	1071	0.08%	0.011%
48	7.182	1808	1817	1827	rVB3	2992	4848	0.38%	0.049%
49	7.298	1850	1853	1856	rBV	98	90	0.01%	0.001%
50	7.568	1923	1937	1964	rBV	172493	300512	23.49%	3.022%
51	7.687	1964	1974	1985	rBV5	2106	3488	0.27%	0.035%
52	7.745	1990	1992	1997	rVB2	168	134	0.01%	0.001%
53	7.899	2026	2040	2056	rBV	572769	997315	77.96%	10.030%
54	8.137	2111	2114	2116	rBV	121	89	0.01%	0.001%
55	8.182	2116	2128	2148	rVV	121861	202476	15.83%	2.036%
56	8.388	2186	2192	2194	rBV2	157	148	0.01%	0.001%
57	8.472	2213	2218	2221	rBV3	312	377	0.03%	0.004%
58	8.636	2255	2269	2307	rBV	437737	740487	57.88%	7.447%
59	8.925	2356	2359	2362	rVB	139	85	0.01%	0.001%
60	8.986	2375	2378	2380	rBV	129	82	0.01%	0.001%
61	9.250	2457	2460	2467	rBV2	170	239	0.02%	0.002%
62	9.420	2500	2513	2549	rVB	562009	926811	72.45%	9.321%
63	9.571	2553	2560	2567	rVB2	753	1033	0.08%	0.010%
64	9.697	2592	2599	2607	rBV4	1205	1523	0.12%	0.015%
65	10.115	2720	2729	2732	rBV4	1146	1472	0.12%	0.015%
66	10.446	2829	2832	2833	rBV	174	95	0.01%	0.001%
67	10.481	2838	2843	2844	rBV2	343	267	0.02%	0.003%
68	10.642	2886	2893	2897	rBV3	1025	1302	0.10%	0.013%
69	10.671	2897	2902	2911	rVB3	3314	4212	0.33%	0.042%
70	10.758	2917	2929	2947	rVB	412367	661721	51.72%	6.655%
71	10.828	2947	2951	2955	rBV2	329	367	0.03%	0.004%
72	10.873	2958	2965	2969	rBV4	642	829	0.06%	0.008%
73	10.928	2980	2982	2986	rVB2	543	368	0.03%	0.004%
74	10.957	2988	2991	2993	rBV2	161	92	0.01%	0.001%
75	11.005	3003	3006	3010	rBV2	234	161	0.01%	0.002%
76	11.028	3010	3013	3016	rVB	190	114	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110121\
 Data File : VU045482.D
 Acq On : 01 Nov 2021 12:00
 Operator : SY/MD
 Sample : VU1101WBL04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK037

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
 Title : VOC Analysis

77	11.095	3027	3034	3039	rBV4	521	784	0.06%	0.008%
78	11.150	3048	3051	3052	rBV2	273	142	0.01%	0.001%
79	11.195	3062	3065	3067	rBV	150	77	0.01%	0.001%
80	11.214	3067	3071	3076	rVB	303	250	0.02%	0.003%
81	11.465	3140	3149	3162	rVB4	2478	4531	0.35%	0.046%
82	11.584	3182	3186	3190	rVB3	331	304	0.02%	0.003%
83	11.700	3216	3222	3229	rVB5	1295	1762	0.14%	0.018%
84	11.751	3232	3238	3245	rVB3	1071	1447	0.11%	0.015%
85	11.812	3245	3257	3275	rBV	594278	938219	73.34%	9.436%
86	11.941	3294	3297	3299	rBV3	770	567	0.04%	0.006%
87	12.028	3321	3324	3327	rBV2	255	220	0.02%	0.002%
88	12.195	3360	3376	3393	rBV	578895	922769	72.13%	9.281%
89	12.282	3400	3403	3406	rBV	200	111	0.01%	0.001%
90	12.336	3417	3420	3423	rVB2	422	283	0.02%	0.003%
91	12.407	3440	3442	3445	rVB3	448	235	0.02%	0.002%
92	12.426	3445	3448	3453	rVB2	228	196	0.02%	0.002%
93	12.629	3508	3511	3513	rBV	243	172	0.01%	0.002%
94	12.780	3549	3558	3563	rBV	401	692	0.05%	0.007%
95	13.105	3653	3659	3663	rBV	305	417	0.03%	0.004%
96	13.221	3689	3695	3703	rBV3	969	1271	0.10%	0.013%
97	13.844	3883	3889	3900	rBV3	2140	2732	0.21%	0.027%
98	14.089	3958	3965	3977	rBV4	2268	3779	0.30%	0.038%
99	14.333	4035	4041	4048	rVB3	1969	2332	0.18%	0.023%
100	14.545	4104	4107	4110	rBV	323	251	0.02%	0.003%




Sum of corrected areas: 9942940

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110121\
Data File : VU045482.D
Acq On : 01 Nov 2021 12:00
Operator : SY/MD
Sample : VU1101WBL04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK037

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

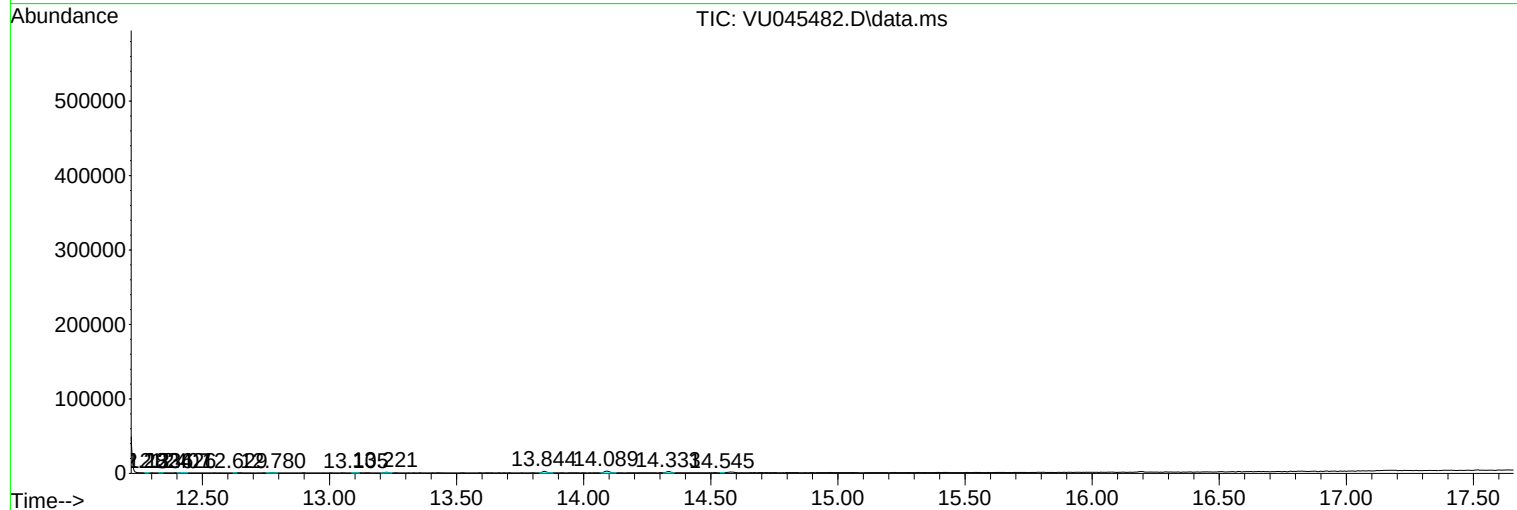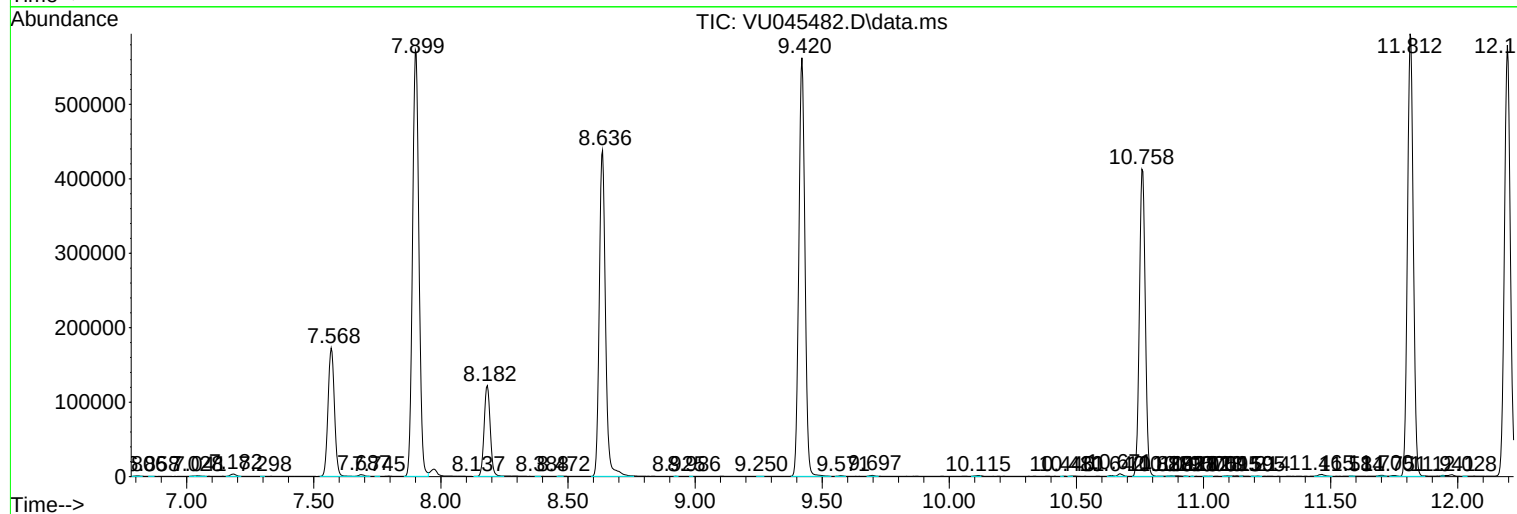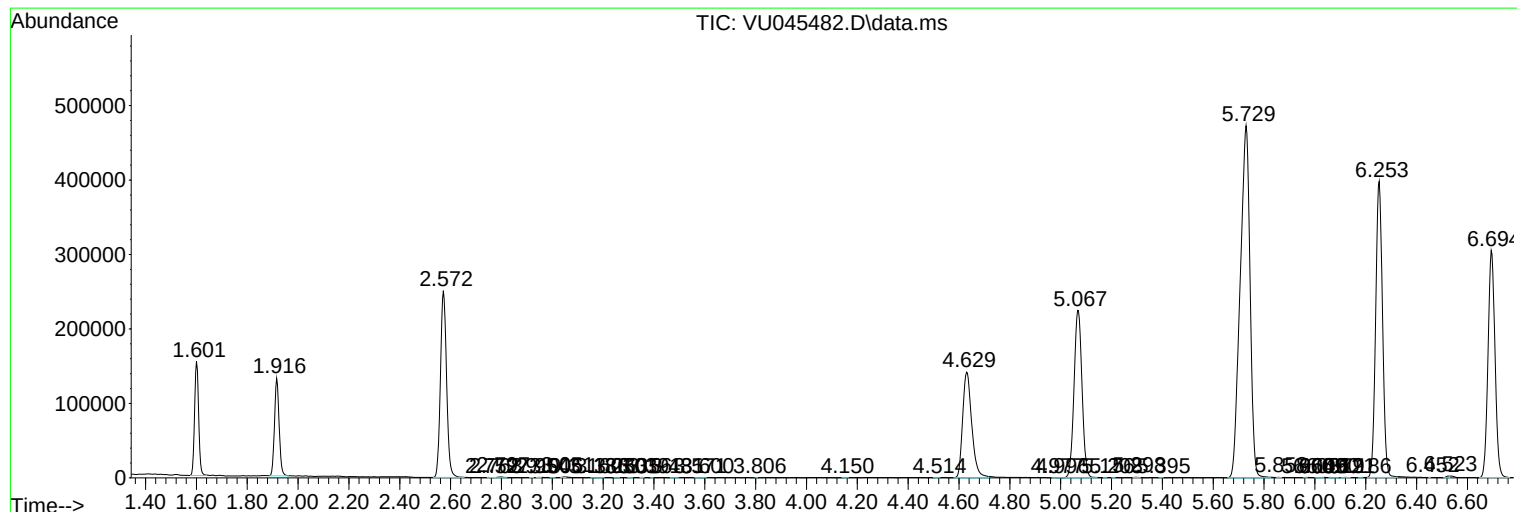

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110121\
Data File : VU045482.D
Acq On : 01 Nov 2021 12:00
Operator : SY/MD
Sample : VU1101WBL04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK037

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110121\
Data File : VU045482.D
Acq On : 01 Nov 2021 12:00
Operator : SY/MD
Sample : VU1101WBL04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK037

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc