

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110121\
 Data File : VU045483.D
 Acq On : 01 Nov 2021 12:22
 Operator : SY/MD
 Sample : VU1101WBL05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK038

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
 Title : VOC Analysis

Signal : TIC: VU045483.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	104	rVB	156928	173867	13.56%	1.745%
2	1.916	170	179	190	rBV	131182	163395	12.74%	1.640%
3	2.244	279	281	285	rBV2	517	294	0.02%	0.003%
4	2.572	370	383	405	rBV	251991	419157	32.69%	4.207%
5	2.700	418	423	427	rVB	259	202	0.02%	0.002%
6	2.723	427	430	433	rBV	152	113	0.01%	0.001%
7	3.051	524	532	540	rVB3	1140	1811	0.14%	0.018%
8	3.196	574	577	579	rBV	150	89	0.01%	0.001%
9	3.565	689	692	697	rBV2	102	102	0.01%	0.001%
10	3.700	728	734	737	rVB2	240	304	0.02%	0.003%
11	3.716	737	739	740	rBV	145	76	0.01%	0.001%
12	3.749	746	749	751	rBV	141	106	0.01%	0.001%
13	3.797	759	764	768	rBV2	120	122	0.01%	0.001%
14	3.986	819	823	828	rBV2	221	212	0.02%	0.002%
15	4.093	851	856	859	rVB2	164	180	0.01%	0.002%
16	4.112	859	862	864	rBV	127	113	0.01%	0.001%
17	4.167	875	879	884	rVB2	209	257	0.02%	0.003%
18	4.192	884	887	890	rBV2	269	236	0.02%	0.002%
19	4.263	904	909	911	rBV2	133	123	0.01%	0.001%
20	4.308	920	923	927	rBV	102	79	0.01%	0.001%
21	4.350	933	936	938	rVB2	127	70	0.01%	0.001%
22	4.392	945	949	952	rBV	258	238	0.02%	0.002%
23	4.411	953	955	962	rVB2	172	161	0.01%	0.002%
24	4.630	1007	1023	1056	rBV	144055	353974	27.60%	3.553%
25	4.967	1124	1128	1132	rBV2	146	163	0.01%	0.002%
26	5.067	1143	1159	1180	rVV	226367	491750	38.35%	4.936%
27	5.202	1195	1201	1208	rBV2	184	315	0.02%	0.003%
28	5.292	1223	1229	1237	rVB3	464	793	0.06%	0.008%
29	5.530	1298	1303	1304	rBV2	104	87	0.01%	0.001%
30	5.559	1310	1312	1316	rVB2	131	78	0.01%	0.001%
31	5.581	1316	1319	1322	rBV2	105	75	0.01%	0.001%
32	5.604	1323	1326	1332	rVB2	117	120	0.01%	0.001%
33	5.729	1342	1365	1390	rBV2	476842	1282320	100.00%	12.871%
34	5.970	1437	1440	1444	rVV	169	145	0.01%	0.001%
35	6.035	1456	1460	1463	rBV3	407	313	0.02%	0.003%
36	6.080	1469	1474	1477	rBV2	148	137	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110121\
 Data File : VU045483.D
 Acq On : 01 Nov 2021 12:22
 Operator : SY/MD
 Sample : VU1101WBL05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK038

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
 Title : VOC Analysis

37	6.118	1481	1486	1491	rBV2	415	456	0.04%	0.005%
38	6.192	1506	1509	1513	rBV2	305	297	0.02%	0.003%
39	6.253	1513	1528	1549	rBV	396225	748165	58.34%	7.509%
40	6.459	1590	1592	1596	rVV3	282	189	0.01%	0.002%
41	6.533	1607	1615	1630	rVB5	2353	4225	0.33%	0.042%
42	6.591	1630	1633	1635	rBV	131	89	0.01%	0.001%
43	6.694	1651	1665	1685	rBV	305850	587209	45.79%	5.894%
44	6.806	1695	1700	1707	rBV2	766	1058	0.08%	0.011%
45	6.890	1720	1726	1729	rBV	168	211	0.02%	0.002%
46	6.964	1746	1749	1754	rBV	151	126	0.01%	0.001%
47	7.041	1767	1773	1775	rBV3	518	499	0.04%	0.005%
48	7.099	1787	1791	1795	rBV2	240	288	0.02%	0.003%
49	7.186	1808	1818	1827	rVB3	3050	4948	0.39%	0.050%
50	7.382	1876	1879	1882	rBV	118	81	0.01%	0.001%
51	7.507	1914	1918	1920	rBV	144	116	0.01%	0.001%
52	7.568	1924	1937	1962	rVV	171973	301179	23.49%	3.023%
53	7.687	1964	1974	1984	rVB3	2313	3686	0.29%	0.037%
54	7.748	1990	1993	1997	rBV2	133	117	0.01%	0.001%
55	7.790	2003	2006	2008	rBV3	221	166	0.01%	0.002%
56	7.900	2026	2040	2056	rBV	584168	1004760	78.35%	10.085%
57	8.073	2092	2094	2099	rVB3	375	315	0.02%	0.003%
58	8.099	2099	2102	2106	rBV2	136	119	0.01%	0.001%
59	8.182	2115	2128	2146	rBV	118999	198931	15.51%	1.997%
60	8.453	2209	2212	2213	rBV	151	77	0.01%	0.001%
61	8.472	2213	2218	2225	rVB2	365	530	0.04%	0.005%
62	8.555	2242	2244	2248	rVB2	177	82	0.01%	0.001%
63	8.633	2256	2268	2304	rBV	439821	747021	58.26%	7.498%
64	8.816	2322	2325	2328	rBV2	162	109	0.01%	0.001%
65	8.932	2359	2361	2366	rVB2	140	98	0.01%	0.001%
66	9.221	2449	2451	2456	rVB	221	107	0.01%	0.001%
67	9.250	2456	2460	2463	rBV	166	158	0.01%	0.002%
68	9.420	2500	2513	2544	rBV	555179	925747	72.19%	9.292%
69	9.568	2554	2559	2561	rBV3	514	526	0.04%	0.005%
70	9.697	2591	2599	2608	rVB3	1270	1974	0.15%	0.020%
71	10.118	2723	2730	2737	rVB4	961	1230	0.10%	0.012%
72	10.433	2825	2828	2829	rBV	156	101	0.01%	0.001%
73	10.639	2887	2892	2896	rBV2	922	1048	0.08%	0.011%
74	10.674	2896	2903	2912	rVB2	2798	3852	0.30%	0.039%
75	10.758	2916	2929	2947	rBV	416031	664543	51.82%	6.670%
76	10.870	2958	2964	2966	rBV	350	432	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110121\
 Data File : VU045483.D
 Acq On : 01 Nov 2021 12:22
 Operator : SY/MD
 Sample : VU1101WBL05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK038

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
 Title : VOC Analysis

77	11.005	3004	3006	3008	rBV3	187	102	0.01%	0.001%
78	11.044	3016	3018	3024	rBV	108	106	0.01%	0.001%
79	11.092	3029	3033	3036	rVV2	306	278	0.02%	0.003%
80	11.211	3067	3070	3072	rBV2	192	146	0.01%	0.001%
81	11.388	3120	3125	3126	rBV	269	226	0.02%	0.002%
82	11.462	3141	3148	3160	rVB5	2366	3881	0.30%	0.039%
83	11.562	3175	3179	3180	rBV	236	156	0.01%	0.002%
84	11.700	3215	3222	3228	rBV3	1298	1628	0.13%	0.016%
85	11.748	3232	3237	3245	rVB2	990	1185	0.09%	0.012%
86	11.813	3245	3257	3272	rBV	599579	931896	72.67%	9.353%
87	11.941	3295	3297	3302	rBV4	507	593	0.05%	0.006%
88	11.973	3303	3307	3319	rVB5	1962	2692	0.21%	0.027%
89	12.054	3330	3332	3334	rBV2	202	104	0.01%	0.001%
90	12.195	3360	3376	3394	rBV	574131	918834	71.65%	9.222%
91	12.333	3415	3419	3426	rBV3	366	366	0.03%	0.004%
92	12.391	3435	3437	3438	rBV3	318	122	0.01%	0.001%
93	12.629	3508	3511	3516	rBV2	318	372	0.03%	0.004%
94	12.767	3550	3554	3557	rBV2	473	475	0.04%	0.005%
95	13.147	3669	3672	3673	rBV	294	159	0.01%	0.002%
96	13.224	3691	3696	3703	rVB3	408	536	0.04%	0.005%
97	13.838	3883	3887	3889	rBV3	1096	848	0.07%	0.009%
98	14.086	3959	3964	3965	rBV	1070	829	0.06%	0.008%
99	14.330	4035	4040	4041	rBV3	1121	850	0.07%	0.009%
100	14.398	4056	4061	4064	rBV3	300	328	0.03%	0.003%




Sum of corrected areas: 9963154

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110121\
Data File : VU045483.D
Acq On : 01 Nov 2021 12:22
Operator : SY/MD
Sample : VU1101WBL05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK038

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

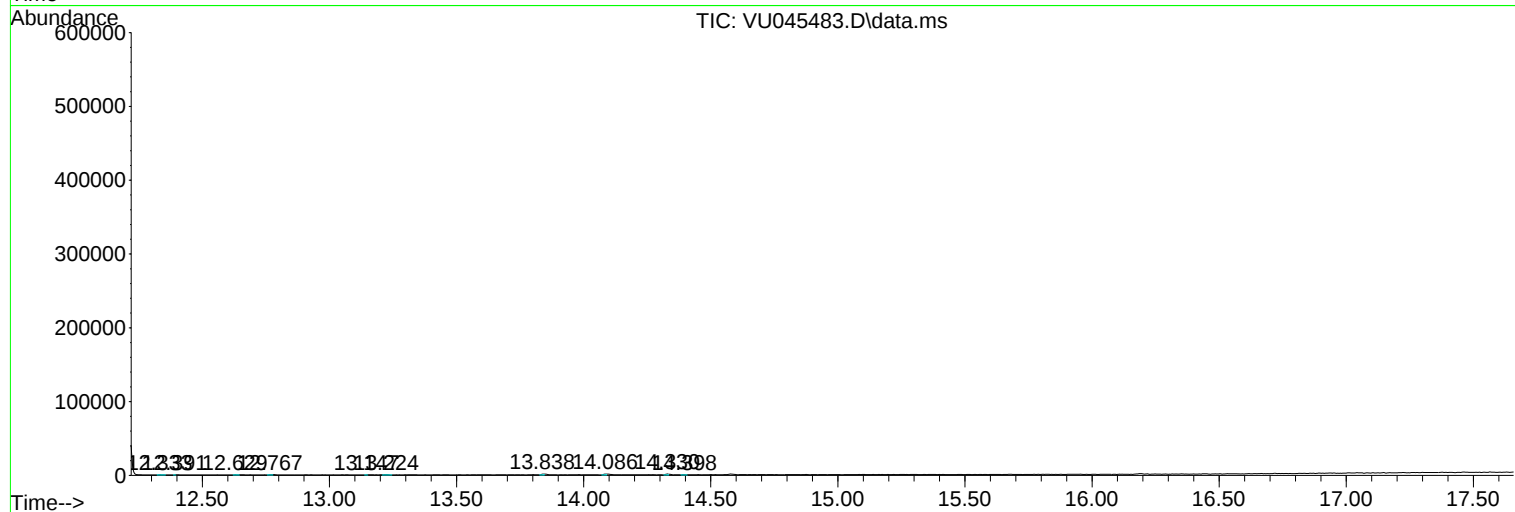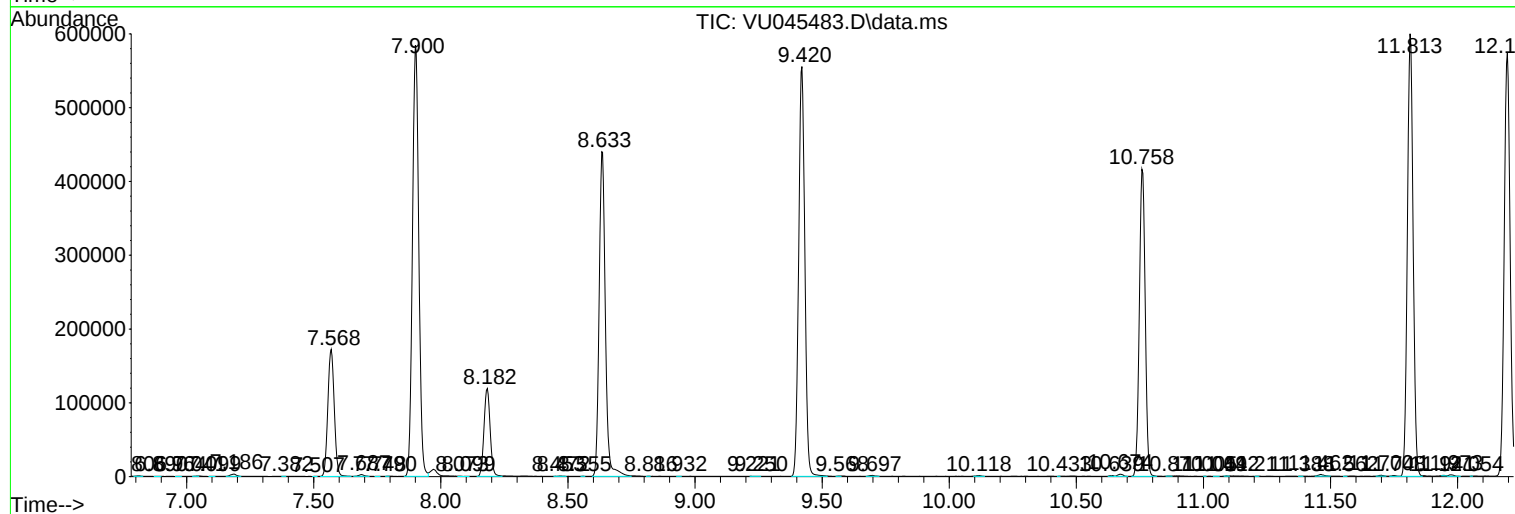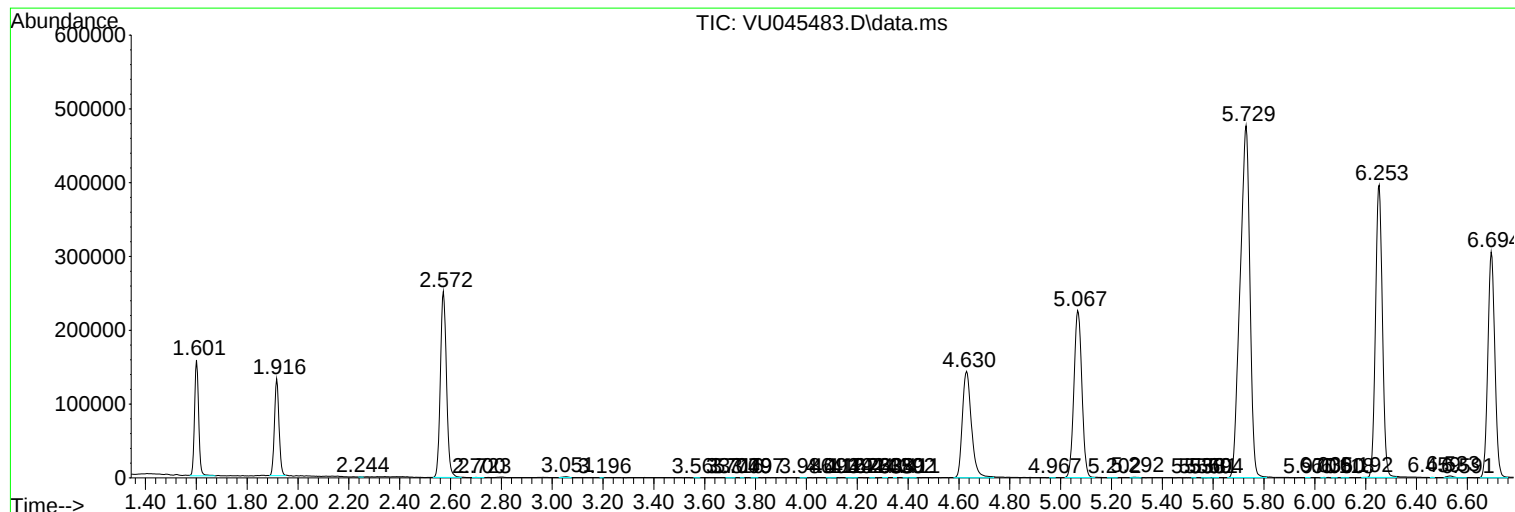

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110121\
Data File : VU045483.D
Acq On : 01 Nov 2021 12:22
Operator : SY/MD
Sample : VU1101WBL05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK038

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110121\
Data File : VU045483.D
Acq On : 01 Nov 2021 12:22
Operator : SY/MD
Sample : VU1101WBL05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK038

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc