


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110121\
Data File : VU045479.D
Acq On : 01 Nov 2021 09:54
Operator : SY/MD
Sample : BFB017
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB017

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM102821WMA.M
Title : VOC Analysis
Last Update : Tue Nov 02 02:33:37 2021

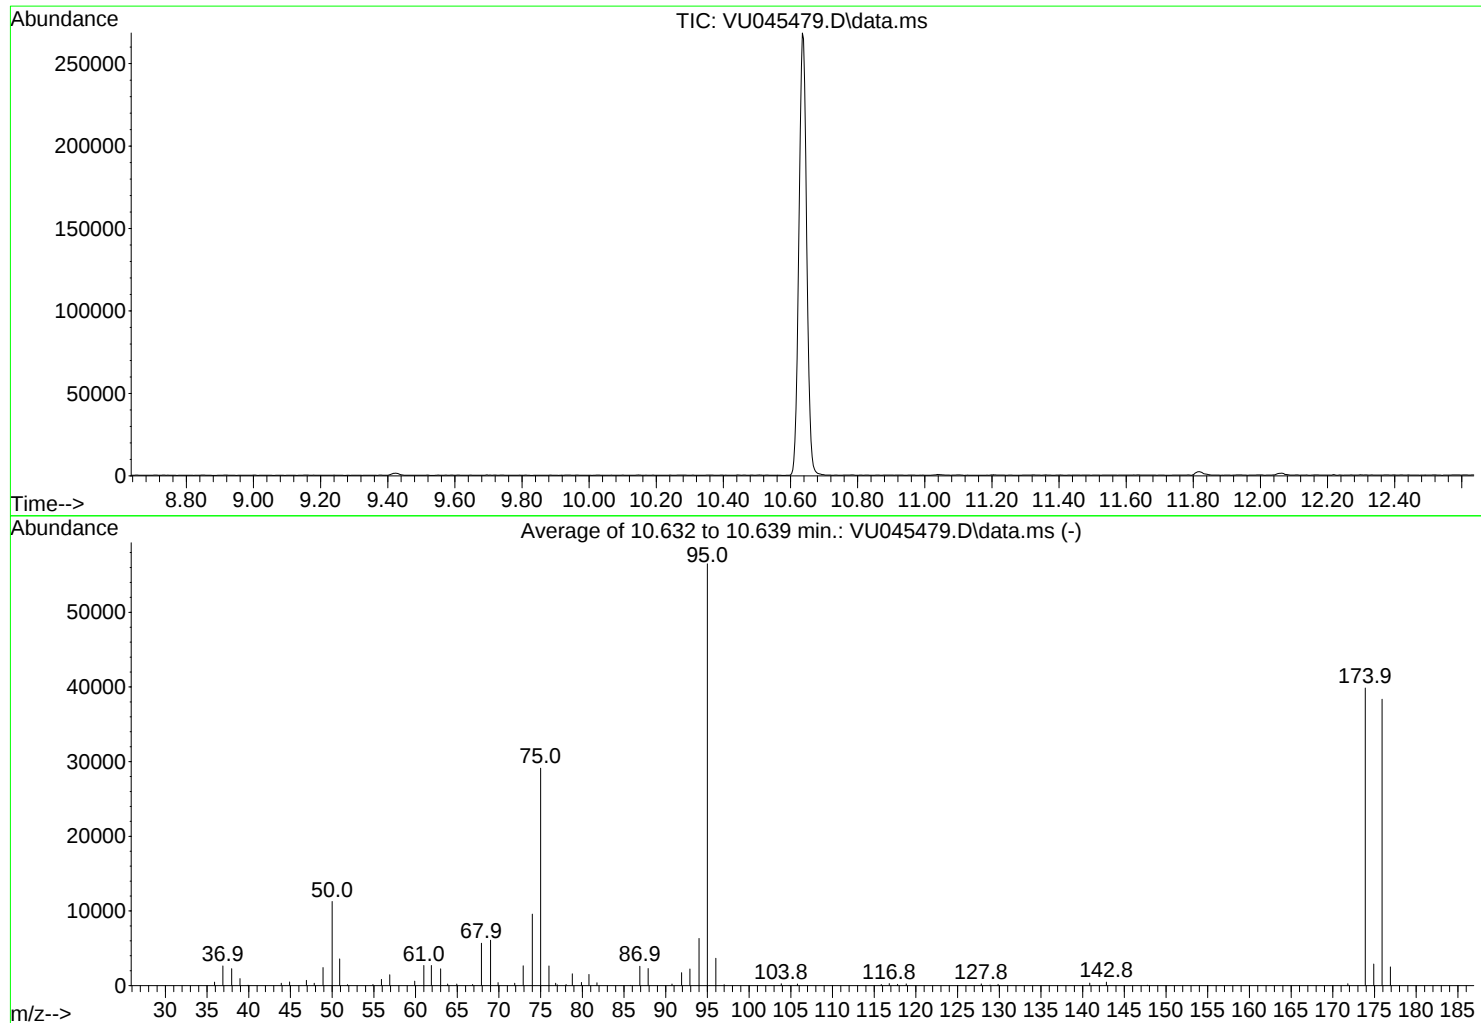

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.0	11276	PASS
75	95	30	80	51.6	29123	PASS
95	95	100	100	100.0	56491	PASS
96	95	5	9	6.5	3671	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.6	39859	PASS
175	174	5	9	7.3	2899	PASS
176	174	95	101	96.3	38368	PASS
177	176	5	9	6.5	2507	PASS

Scan 2878 (10.594 min): VU045479.D\data.ms
BFB017

m/z	Abundance
39.90	143.0
43.90	230.0

Instrument :
MSVOA_U
ClientSampleId :
BFB017

m/z	Abundance
35.90	448.0
36.90	2591.0
37.90	2316.0
38.90	851.0
39.90	219.0
43.90	589.0
44.90	475.0
46.90	674.0
47.90	358.0
48.90	2354.0
50.00	11080.0
50.90	3611.0
51.90	124.0
54.90	177.0
55.90	768.0
56.90	1418.0
59.90	535.0
61.00	2657.0
61.90	2519.0
63.00	2182.0
63.80	247.0
64.90	238.0
66.80	165.0
67.90	5452.0
69.00	5976.0
69.90	363.0
71.90	314.0
72.90	2459.0
74.00	9114.0
75.00	28008.0
76.00	2462.0
76.80	318.0
78.80	1560.0
79.90	403.0
80.80	1428.0
81.80	386.0
86.90	2498.0
87.90	2301.0
90.90	223.0
91.90	1690.0
92.90	2102.0
94.00	6036.0
95.00	53840.0
96.00	3558.0
97.00	121.0
103.90	237.0
105.80	225.0
115.80	140.0
116.80	285.0
117.80	170.0
118.80	238.0
127.90	211.0
129.90	145.0
140.90	317.0
142.80	460.0
171.80	229.0
173.90	37120.0
174.90	2827.0
175.90	36104.0
176.90	2382.0

Instrument :
MSVOA_U
ClientSampleId :
BFB017

m/z	Abundance
35.90	473.0
36.90	2706.0
38.00	2319.0
38.90	929.0
39.90	216.0
43.90	544.0
44.90	511.0
46.90	714.0
47.90	316.0
48.90	2492.0
50.00	11624.0
50.90	3686.0
51.80	138.0
54.90	154.0
55.90	857.0
56.90	1480.0
59.90	628.0
61.00	2763.0
61.90	2766.0
63.00	2312.0
63.80	229.0
64.90	213.0
66.80	149.0
67.90	5877.0
69.00	6247.0
69.90	412.0
71.90	332.0
72.90	2742.0
74.00	9849.0
75.00	30056.0
76.00	2695.0
76.80	355.0
78.10	213.0
78.80	1687.0
79.90	424.0
80.80	1541.0
81.70	412.0
85.80	102.0
86.90	2678.0
87.90	2388.0
90.70	205.0
91.90	1817.0
92.90	2296.0
94.00	6486.0
95.00	58240.0
96.00	3767.0
97.00	141.0
103.90	248.0
104.80	113.0
105.80	229.0
115.90	152.0
116.80	294.0
117.80	167.0
118.80	239.0
127.90	242.0
128.90	123.0
129.80	169.0
140.80	359.0
142.90	491.0
147.70	109.0
171.80	283.0
173.90	41104.0
174.90	2995.0
175.90	39464.0
176.90	2580.0

Instrument :
MSVOA_U
ClientSampleId :
BFB017

m/z	Abundance
35.90	484.0
36.90	2623.0
38.00	2201.0
39.00	1026.0
39.90	216.0
43.90	523.0
44.90	500.0
46.90	717.0
47.80	261.0
48.90	2400.0
50.00	11123.0
50.90	3470.0
51.80	134.0
54.90	145.0
55.90	856.0
56.90	1468.0
59.90	621.0
61.00	2677.0
61.90	2810.0
63.00	2276.0
63.90	198.0
65.00	202.0
66.90	132.0
67.90	5715.0
69.00	6023.0
69.90	441.0
71.90	322.0
72.90	2756.0
74.00	9758.0
75.00	29304.0
76.00	2745.0
76.80	327.0
77.00	333.0
78.00	243.0
78.80	1542.0
79.90	433.0
80.80	1500.0
81.80	371.0
86.90	2595.0
87.90	2227.0
90.70	198.0
91.90	1724.0
92.90	2269.0
94.00	6421.0
95.00	57392.0
96.00	3689.0
97.00	145.0
103.80	260.0
105.80	191.0
115.80	146.0
116.80	287.0
117.80	159.0
118.90	245.0
127.80	239.0
128.90	110.0
129.80	174.0
140.80	373.0
142.90	495.0
147.80	114.0
171.80	285.0
173.90	41352.0
174.90	2876.0
175.90	39536.0
176.90	2558.0

Instrument :
MSVOA_U
ClientSampleId :
BFB017