

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110123\
 Data File : VU056040.D
 Acq On : 01 Nov 2023 15:29
 Operator : MD/SY
 Sample : 05053-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056040.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	111	rVB	168530	196551	15.87%	1.941%
2	1.914	185	194	210	rBV	126641	176502	14.25%	1.743%
3	2.566	382	397	420	rBV	285147	469298	37.90%	4.634%
4	3.045	533	546	566	rBV2	23255	46239	3.73%	0.457%
5	4.634	1025	1040	1085	rBV	117796	410600	33.16%	4.054%
6	5.061	1155	1173	1202	rBV	240356	579624	46.80%	5.723%
7	5.724	1356	1379	1408	rBV3	479700	1238410	100.00%	12.227%
8	6.245	1528	1541	1572	rBV	401471	795025	64.20%	7.850%
9	6.688	1662	1679	1704	rBV	280572	560515	45.26%	5.534%
10	7.106	1798	1809	1822	rVB3	11441	21772	1.76%	0.215%
11	7.563	1939	1951	1977	rBV	139181	258816	20.90%	2.555%
12	7.894	2040	2054	2088	rBV	566479	1049208	84.72%	10.359%
13	8.177	2132	2142	2160	rBV	80061	144578	11.67%	1.427%
14	8.470	2222	2233	2243	rBV2	15853	28812	2.33%	0.284%
15	8.634	2272	2284	2322	rBV3	501665	1125524	90.88%	11.113%
16	9.415	2514	2527	2550	rBV	557617	980530	79.18%	9.681%
17	10.753	2928	2943	2966	rBV	196764	328241	26.51%	3.241%
18	10.891	2975	2986	3002	rVB	35486	59696	4.82%	0.589%
19	11.810	3260	3272	3296	rBV	509860	851316	68.74%	8.405%
20	12.190	3377	3390	3408	rBV2	473764	806865	65.15%	7.967%




Sum of corrected areas: 10128122

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110123\
Data File : VU056040.D
Acq On : 01 Nov 2023 15:29
Operator : MD/SY
Sample : 05053-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

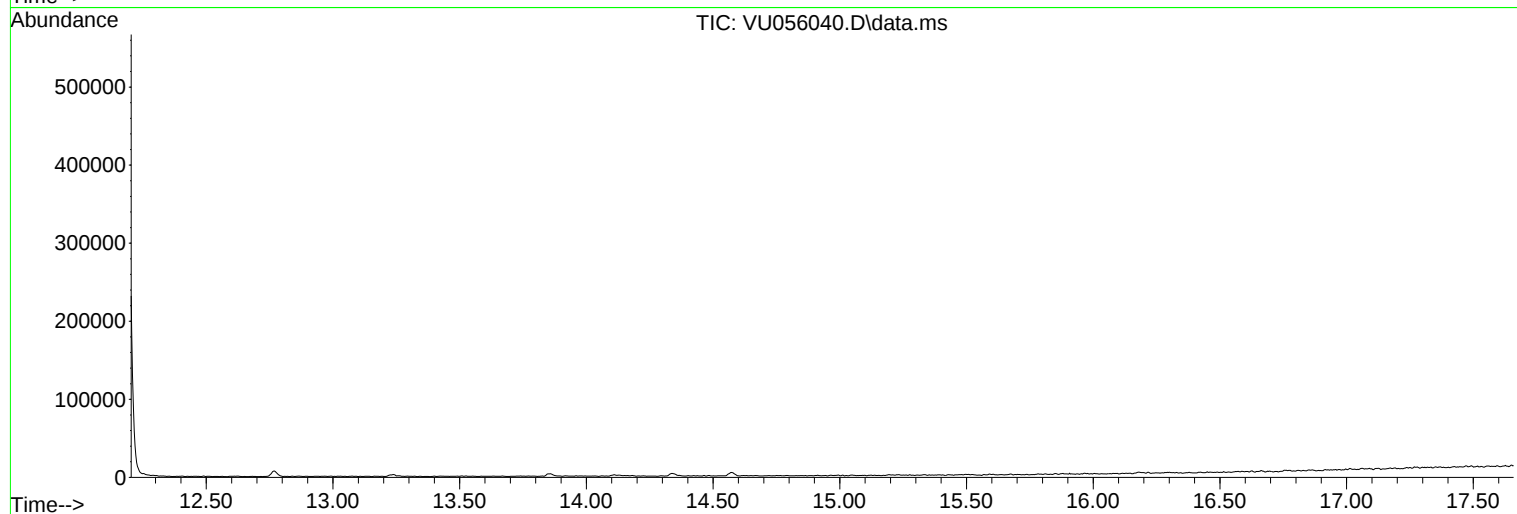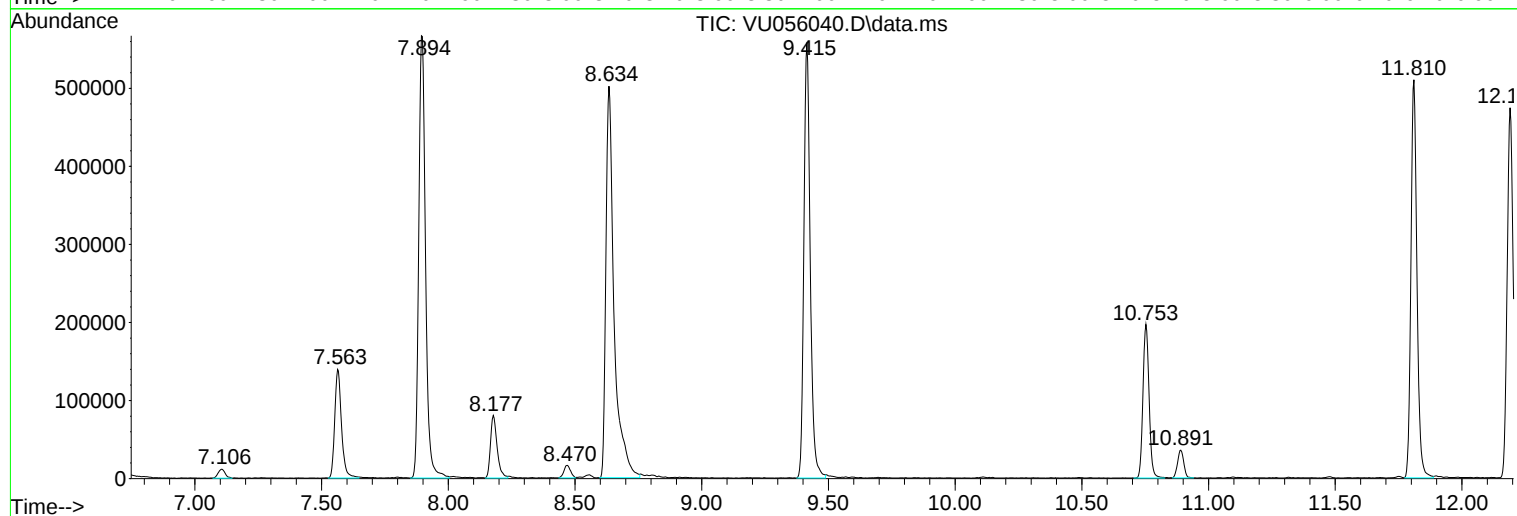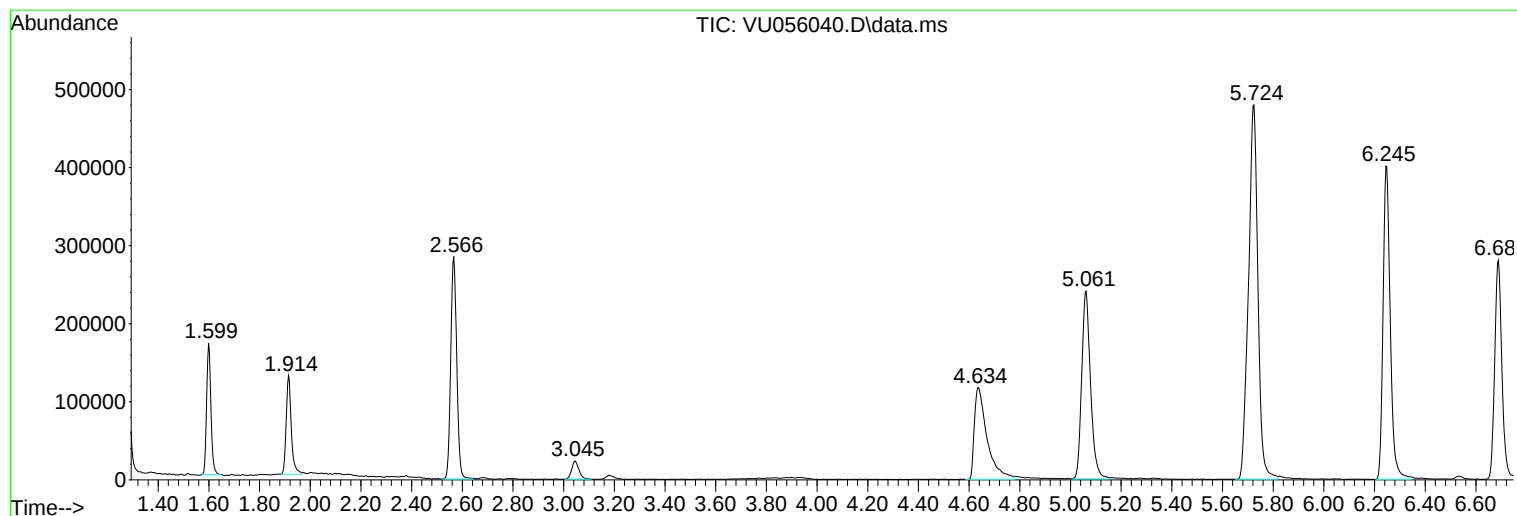

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110123\
Data File : VU056040.D
Acq On : 01 Nov 2023 15:29
Operator : MD/SY
Sample : 05053-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110123\
Data File : VU056040.D
Acq On : 01 Nov 2023 15:29
Operator : MD/SY
Sample : 05053-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc