

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110123\
 Data File : VU056042.D
 Acq On : 01 Nov 2023 16:17
 Operator : MD/SY
 Sample : 05052-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AL9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU056042.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	112	rVB	95850	112020	7.52%	1.151%
2	1.914	186	194	211	rVB	86610	120799	8.11%	1.241%
3	2.566	384	397	414	rBV	176496	288874	19.38%	2.968%
4	3.045	534	546	564	rVB	22764	45506	3.05%	0.467%
5	3.181	574	588	601	rBV2	12347	27940	1.87%	0.287%
6	4.631	1024	1039	1079	rBV	135654	423282	28.40%	4.348%
7	5.081	1156	1179	1218	rBV3	520391	1490307	100.00%	15.310%
8	5.724	1359	1379	1407	rBV2	367930	992537	66.60%	10.196%
9	6.248	1527	1542	1570	rBV	375831	747893	50.18%	7.683%
10	6.688	1664	1679	1701	rBV	240234	479208	32.15%	4.923%
11	7.563	1940	1951	1969	rBV	102483	192818	12.94%	1.981%
12	7.897	2042	2055	2093	rBV	409212	762904	51.19%	7.837%
13	8.180	2131	2143	2164	rBV	62980	115797	7.77%	1.190%
14	8.470	2222	2233	2249	rVV3	14781	27372	1.84%	0.281%
15	8.634	2272	2284	2330	rBV2	487008	1096851	73.60%	11.268%
16	9.415	2514	2527	2553	rBV	528073	936445	62.84%	9.620%
17	10.753	2931	2943	2963	rBV	184538	301341	20.22%	3.096%
18	10.891	2973	2986	3001	rVB2	46071	78164	5.24%	0.803%
19	11.810	3258	3272	3298	rBV	492221	828882	55.62%	8.515%
20	12.190	3378	3390	3419	rBV	395042	665303	44.64%	6.835%




Sum of corrected areas: 9734243

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110123\
Data File : VU056042.D
Acq On : 01 Nov 2023 16:17
Operator : MD/SY
Sample : 05052-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COAL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

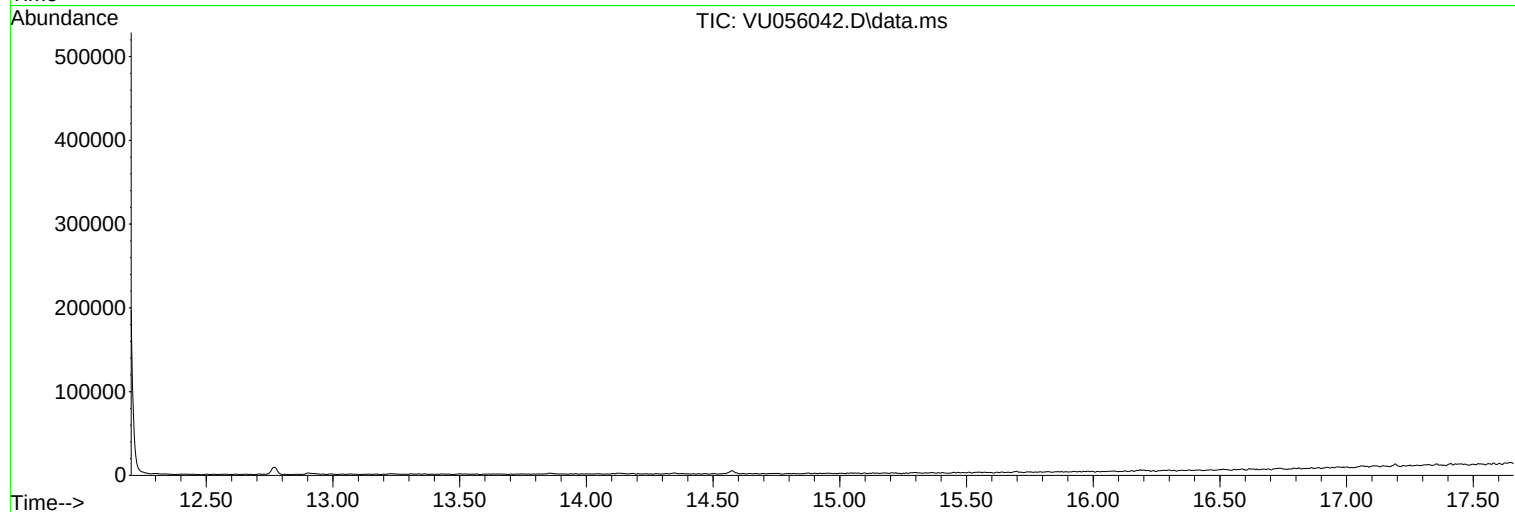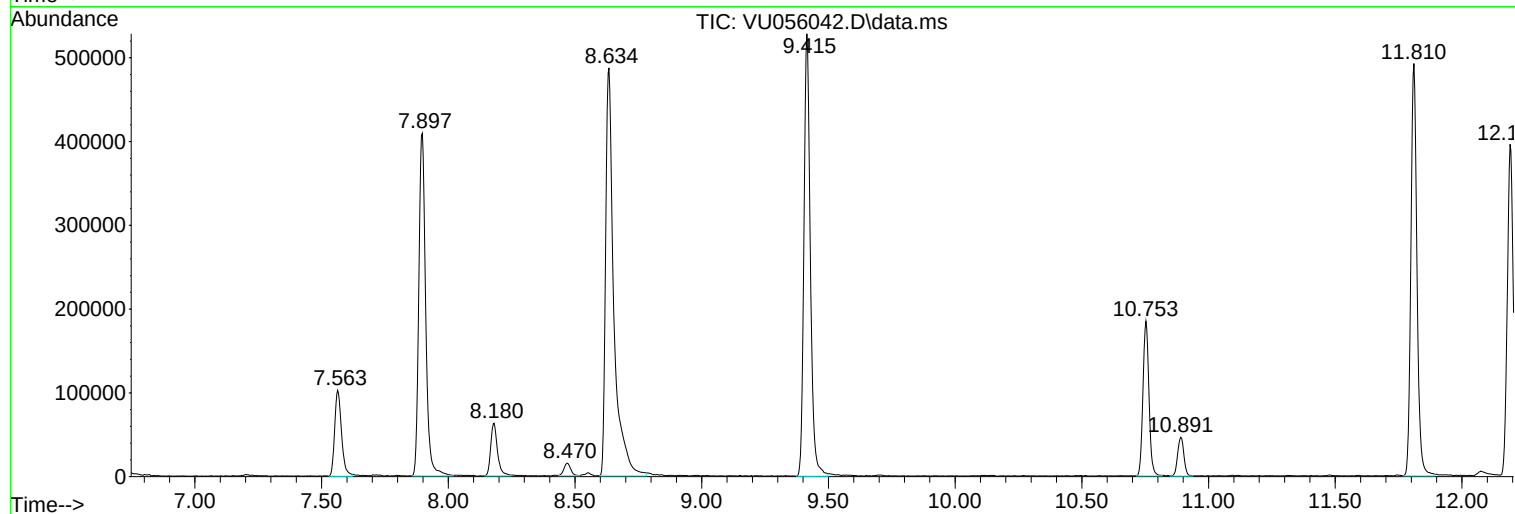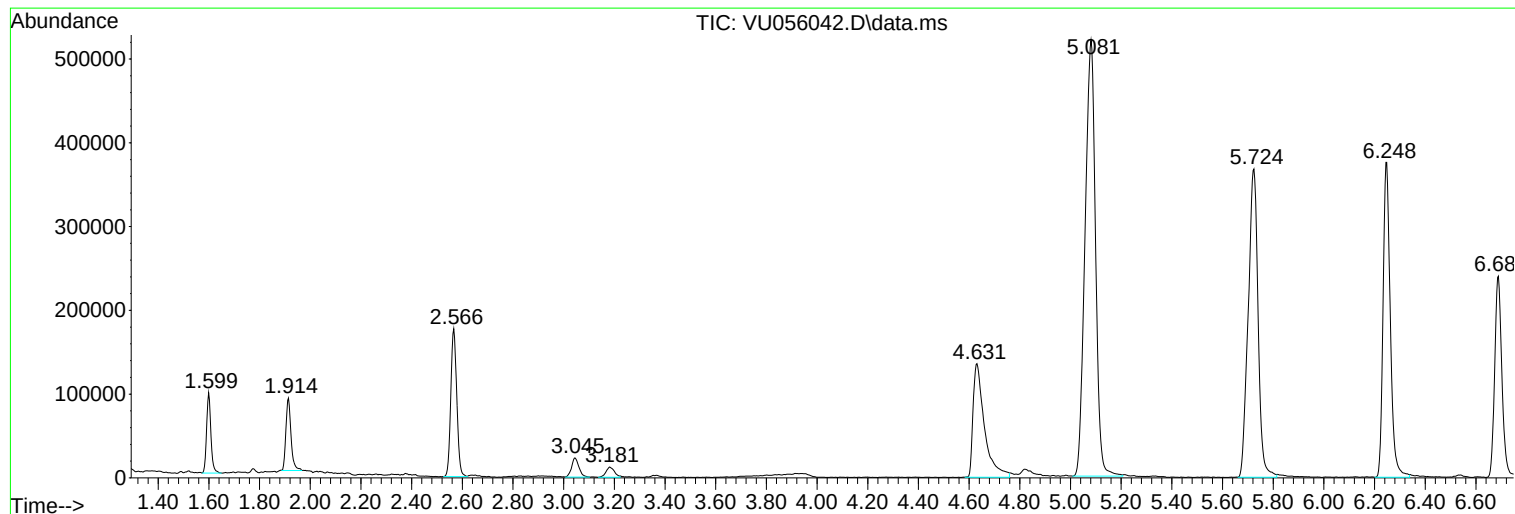

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110123\
Data File : VU056042.D
Acq On : 01 Nov 2023 16:17
Operator : MD/SY
Sample : 05052-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110123\
Data File : VU056042.D
Acq On : 01 Nov 2023 16:17
Operator : MD/SY
Sample : 05052-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc