


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110123\
Data File : VU056031.D
Acq On : 01 Nov 2023 09:02
Operator : MD/SY
Sample : BFB063
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB063

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Nov 02 02:08:05 2023

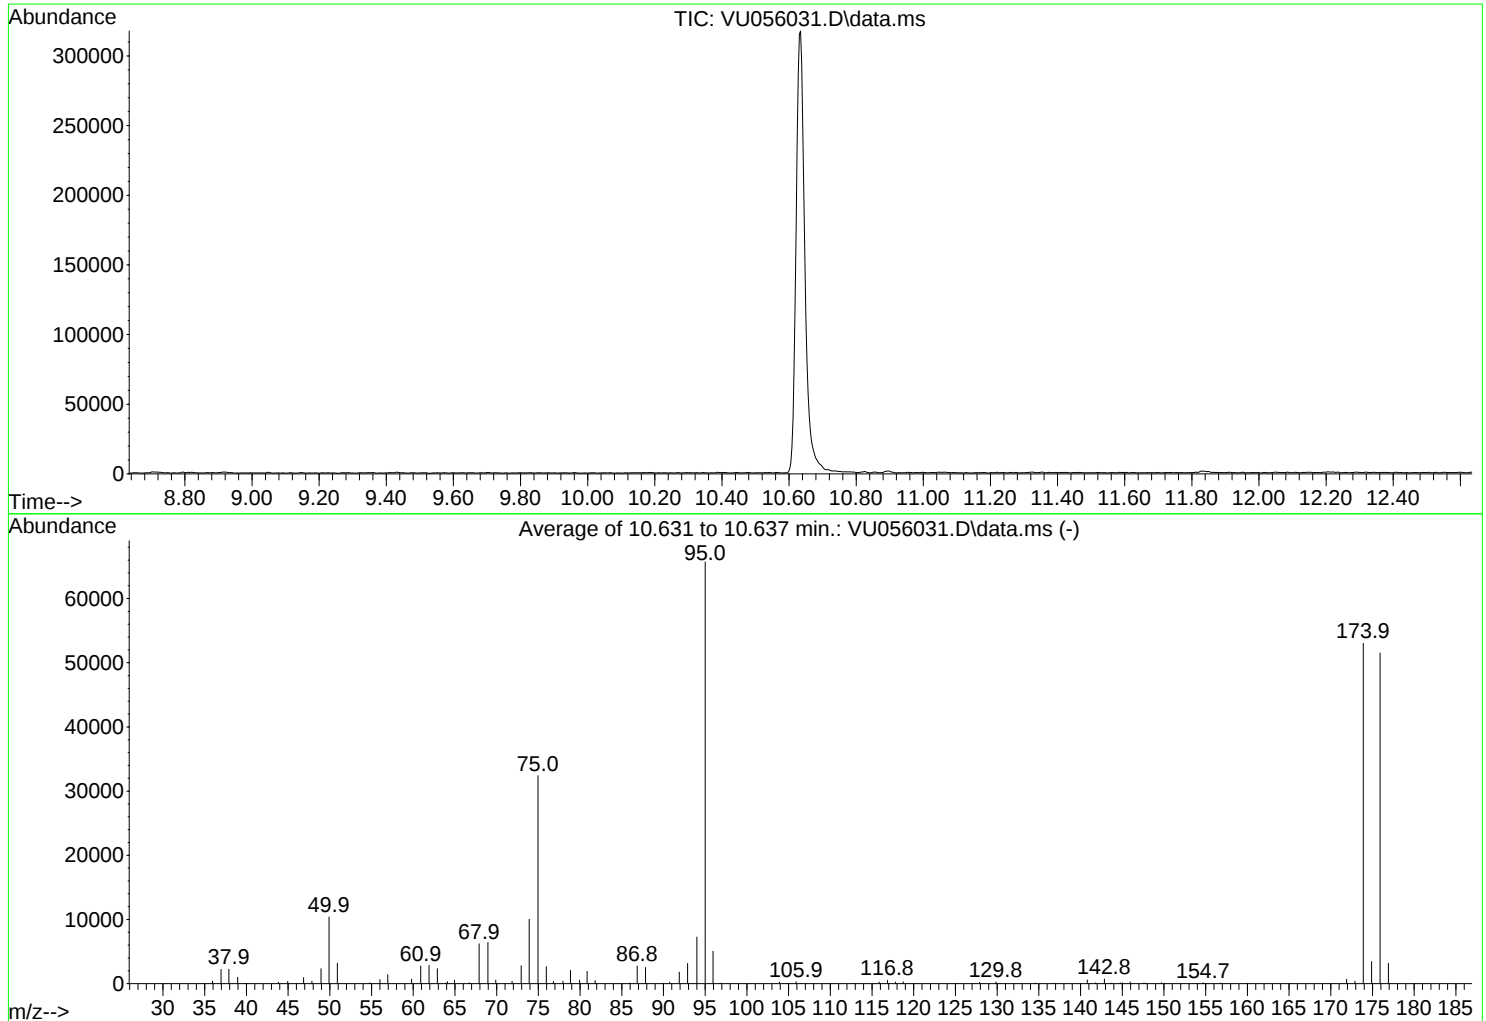

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.8	10368	PASS
75	95	30	80	49.3	32413	PASS
95	95	100	100	100.0	65725	PASS
96	95	5	9	7.7	5038	PASS
173	174	0.00	2	0.7	370	PASS
174	95	50	120	80.7	53043	PASS
175	174	5	9	6.5	3452	PASS
176	174	95	101	97.1	51523	PASS
177	176	5	9	6.2	3172	PASS

m/z	Abundance
39.80	251.0
43.80	503.0

Instrument :
MSVOA_U
ClientSampleId :
BFB063

m/z	Abundance
36.00	429.0
37.00	2217.0
37.90	2372.0
38.90	1029.0
40.00	310.0
43.90	714.0
45.00	280.0
46.90	917.0
47.90	473.0
49.00	2552.0
49.90	10923.0
50.90	3355.0
54.80	182.0
56.00	669.0
56.90	1481.0
59.80	703.0
60.90	3024.0
61.90	2926.0
62.90	2361.0
63.90	345.0
65.00	507.0
66.70	154.0
67.90	6395.0
69.00	6653.0
69.90	548.0
71.80	383.0
72.90	2800.0
73.90	10421.0
74.90	33576.0
75.90	2783.0
76.80	401.0
77.90	302.0
78.80	2108.0
79.90	548.0
80.90	2184.0
81.80	514.0
86.00	105.0
86.80	2700.0
87.80	2529.0
90.80	202.0
91.90	1783.0
92.90	3109.0
94.00	7391.0
95.00	67280.0
95.90	5149.0
96.80	142.0
103.90	278.0
105.90	315.0
115.80	242.0
116.80	508.0
117.80	313.0
118.70	302.0
127.90	206.0
129.90	229.0
136.70	108.0
140.80	607.0
141.80	130.0
142.80	766.0
143.70	103.0
144.80	228.0
145.90	282.0
147.60	139.0
149.70	113.0
154.70	205.0
171.90	620.0
173.90	53832.0
174.90	3526.0
175.90	51696.0
176.90	3119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB063

m/z	Abundance
36.00	398.0
36.90	2320.0
37.90	2328.0
39.00	1015.0
40.00	262.0
43.90	739.0
44.90	330.0
46.90	1037.0
47.80	383.0
48.90	2374.0
49.90	10681.0
50.90	3255.0
54.80	123.0
56.00	631.0
56.90	1471.0
59.80	729.0
60.90	2844.0
61.90	2970.0
62.90	2459.0
64.10	425.0
64.90	531.0
66.70	170.0
67.90	6464.0
68.90	6561.0
69.90	581.0
71.80	373.0
73.00	2829.0
73.90	10253.0
74.90	33096.0
75.90	2691.0
76.80	331.0
77.90	383.0
78.90	2138.0
80.00	602.0
80.80	1936.0
81.80	486.0
85.90	111.0
86.90	2817.0
87.80	2524.0
90.70	229.0
91.90	1842.0
92.90	3254.0
94.00	7332.0
95.00	67432.0
96.00	5210.0
96.80	103.0
103.90	242.0
105.90	306.0
112.80	103.0
115.80	276.0
116.80	559.0
117.80	257.0
118.70	255.0
127.90	210.0
129.90	294.0
134.60	110.0
136.70	119.0
140.80	565.0
141.80	152.0
142.90	717.0
143.70	101.0
145.00	208.0
146.00	307.0
147.60	174.0
149.70	149.0
154.70	169.0
156.80	162.0
171.90	698.0
172.90	576.0
173.90	54416.0
174.90	3618.0
175.90	52840.0
176.90	3254.0

Instrument :
MSVOA_U
ClientSampleId :
BFB063

m/z	Abundance
35.80	379.0
36.90	2123.0
37.90	2068.0
39.00	940.0
39.90	220.0
43.90	710.0
44.90	439.0
46.80	877.0
47.80	291.0
48.90	2040.0
49.90	9499.0
50.90	2973.0
54.80	111.0
56.00	594.0
57.00	1273.0
59.80	659.0
60.90	2396.0
61.90	2665.0
62.90	2219.0
64.10	459.0
64.90	535.0
66.70	134.0
67.90	5741.0
68.90	6055.0
69.90	542.0
71.90	346.0
73.00	2735.0
73.90	9421.0
75.00	30568.0
76.00	2423.0
76.80	334.0
78.00	426.0
78.90	1956.0
80.00	514.0
80.90	1647.0
81.80	433.0
85.90	114.0
86.90	2694.0
87.90	2513.0
90.70	238.0
91.90	1806.0
92.90	3049.0
94.00	7017.0
95.00	62464.0
96.00	4756.0
103.90	213.0
104.90	115.0
105.90	258.0
115.90	245.0
116.90	521.0
117.80	176.0
118.80	286.0
127.90	223.0
129.80	277.0
134.60	170.0
140.80	573.0
141.80	118.0
142.90	673.0
144.70	149.0
145.10	177.0
146.00	225.0
147.80	229.0
149.70	169.0
154.80	100.0
156.80	169.0
171.90	738.0
172.90	534.0
173.90	50880.0
174.90	3212.0
175.90	50032.0
176.90	3143.0

Instrument :
MSVOA_U
ClientSampleId :
BFB063