



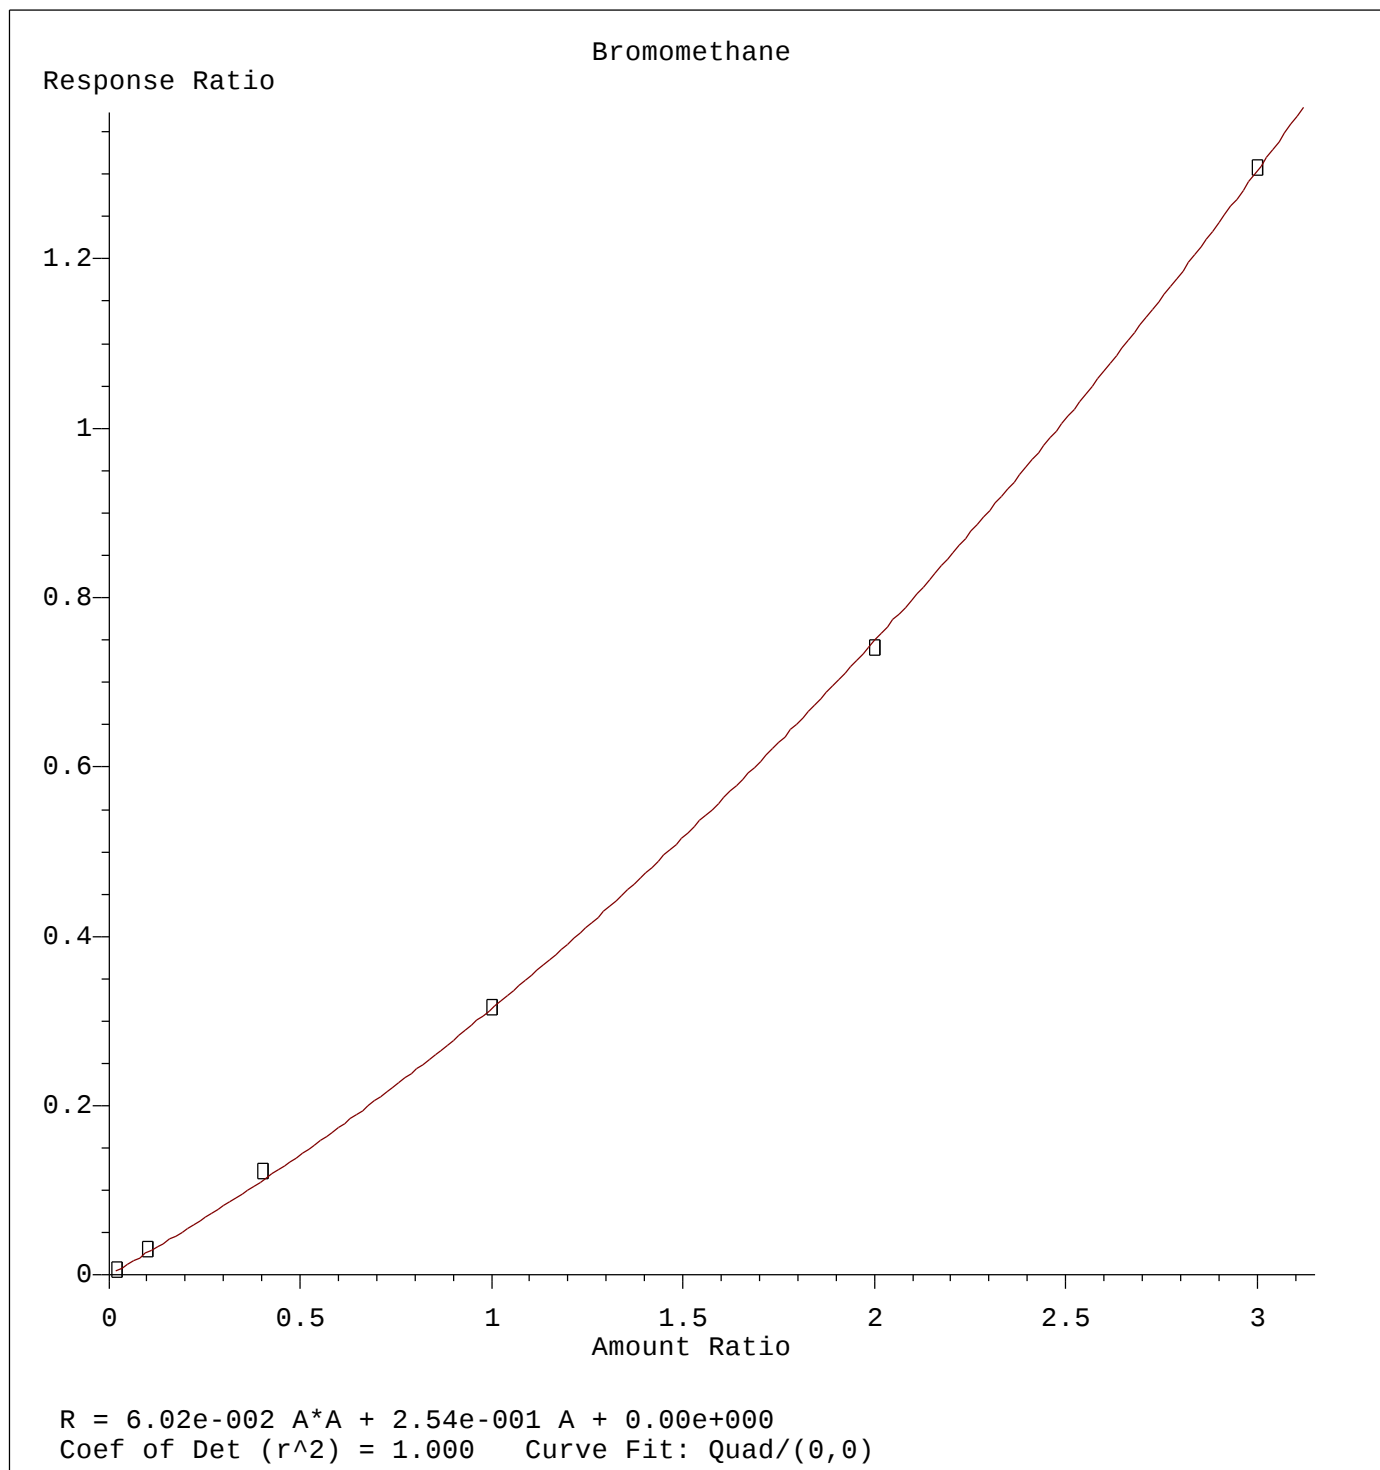

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U110218W.M
Calibration Table Last Updated: Fri Nov 02 02:28:20 2018

Naphthalene

Response Ratio

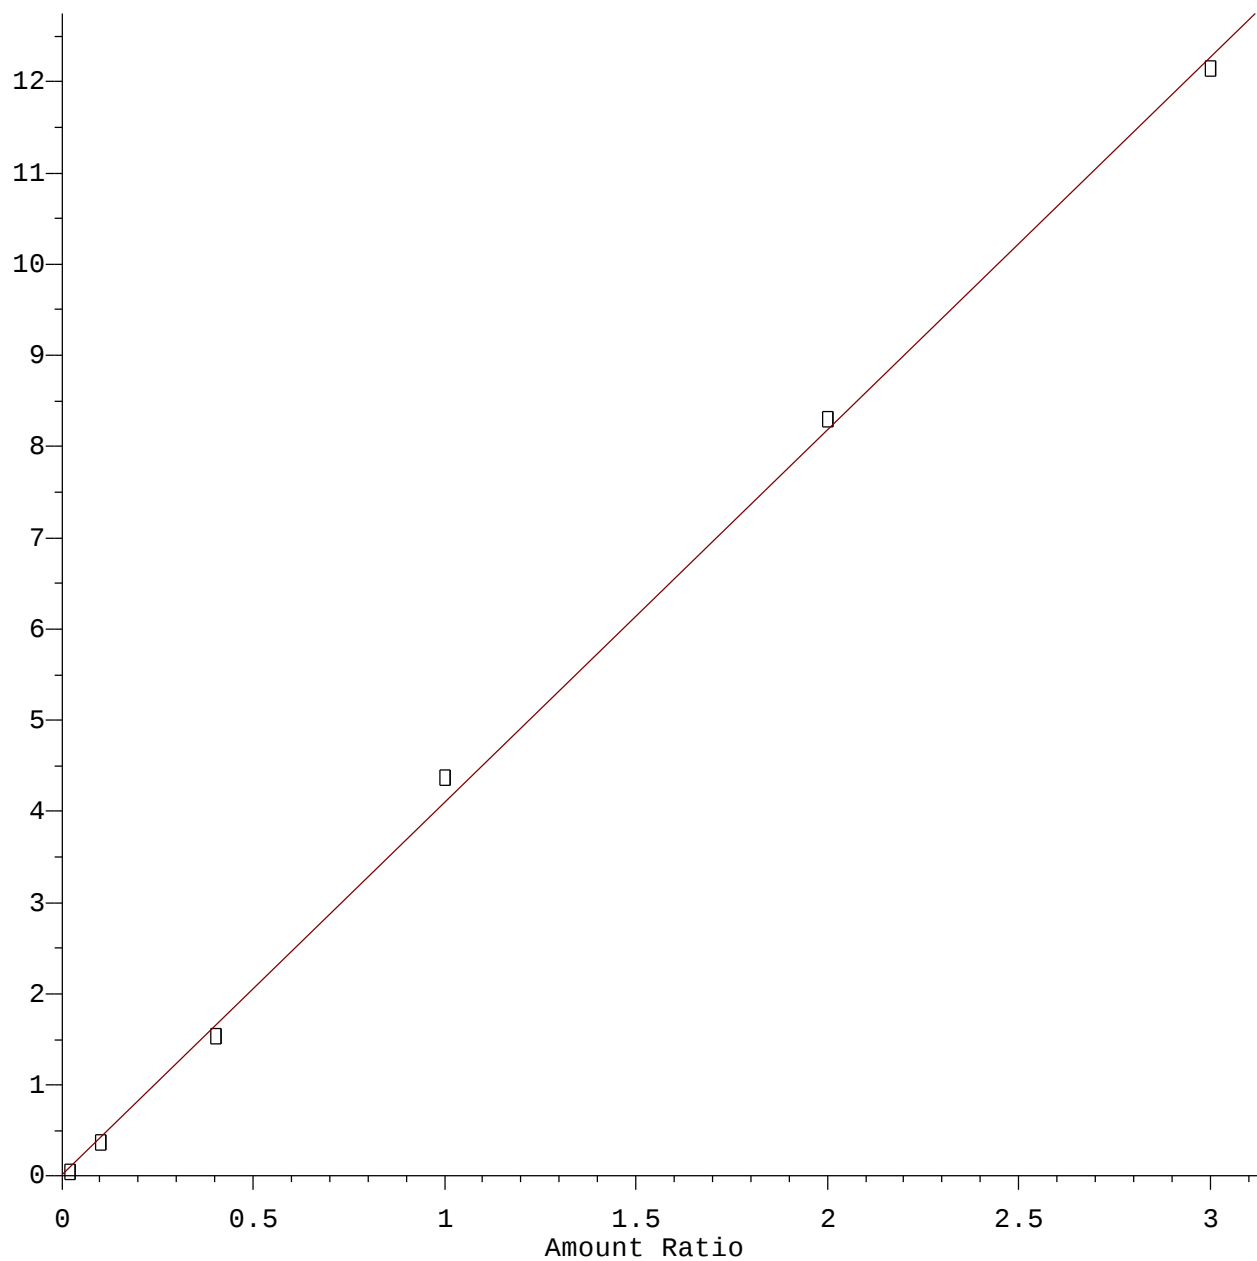


Resp Ratio = 4.09×10^0 * Amt + 1.49×10^{-2}
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U110218W.M
Calibration Table Last Updated: Fri Nov 02 02:28:20 2018

1,2,4-Trichlorobenzene

Response Ratio

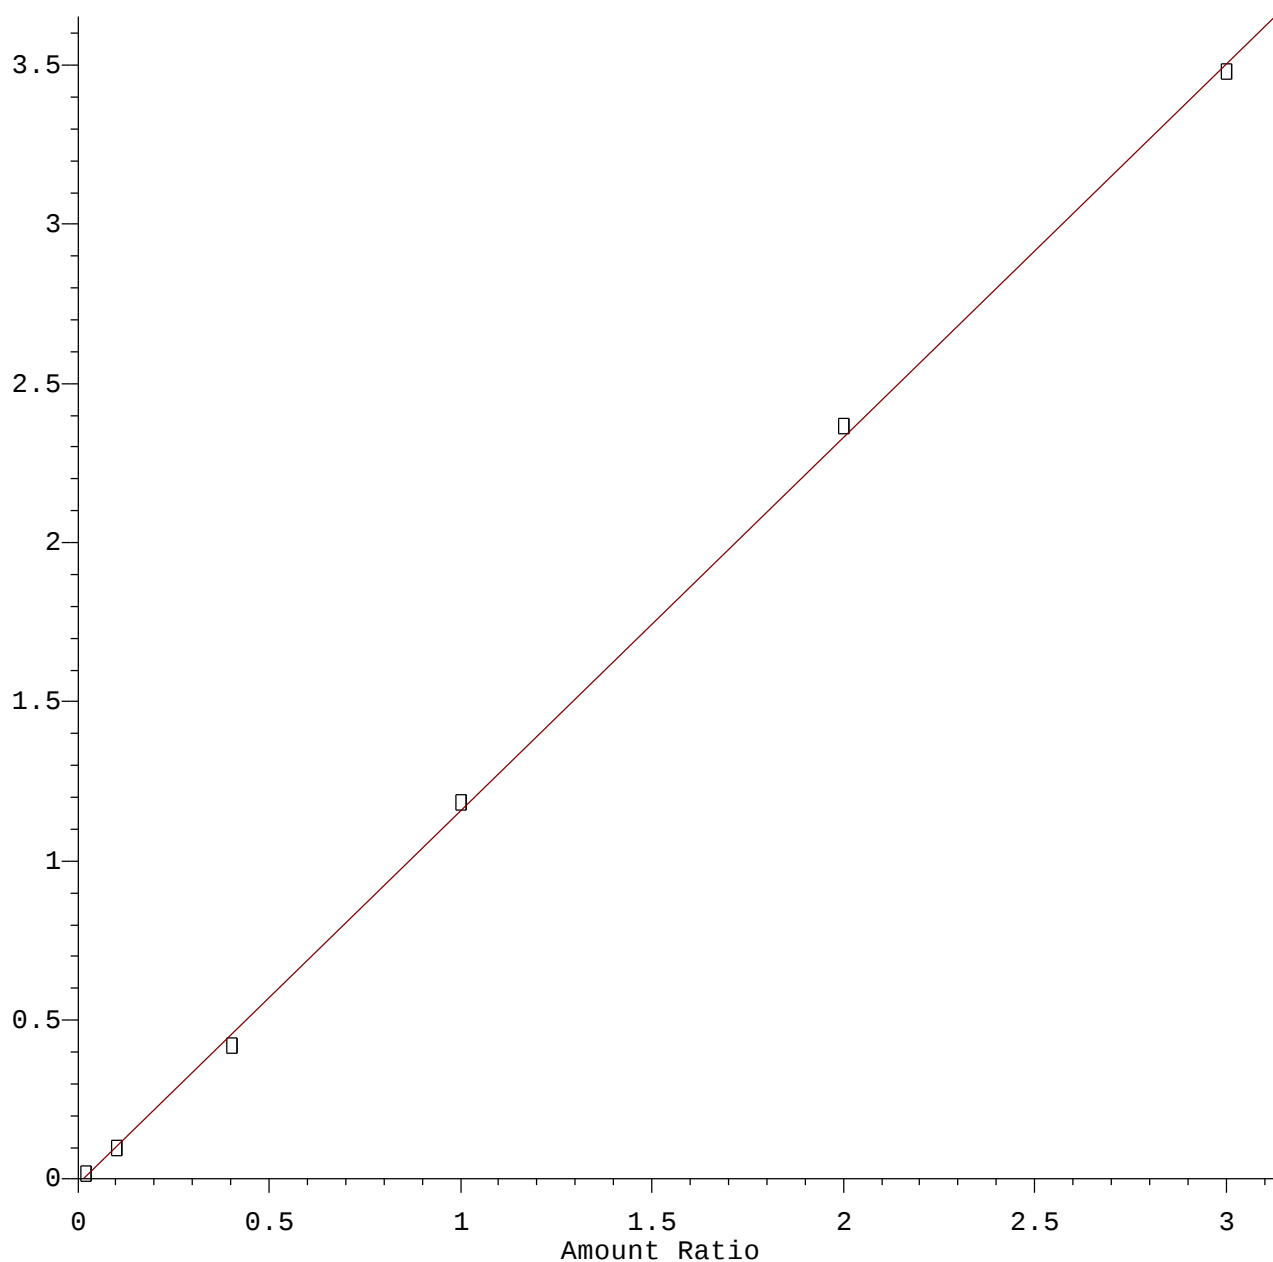


Resp Ratio = 1.17e+000 * Amt - 1.61e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U110218W.M
Calibration Table Last Updated: Fri Nov 02 02:28:20 2018

trans-1,4-Dichloro-2-butene

Response Ratio

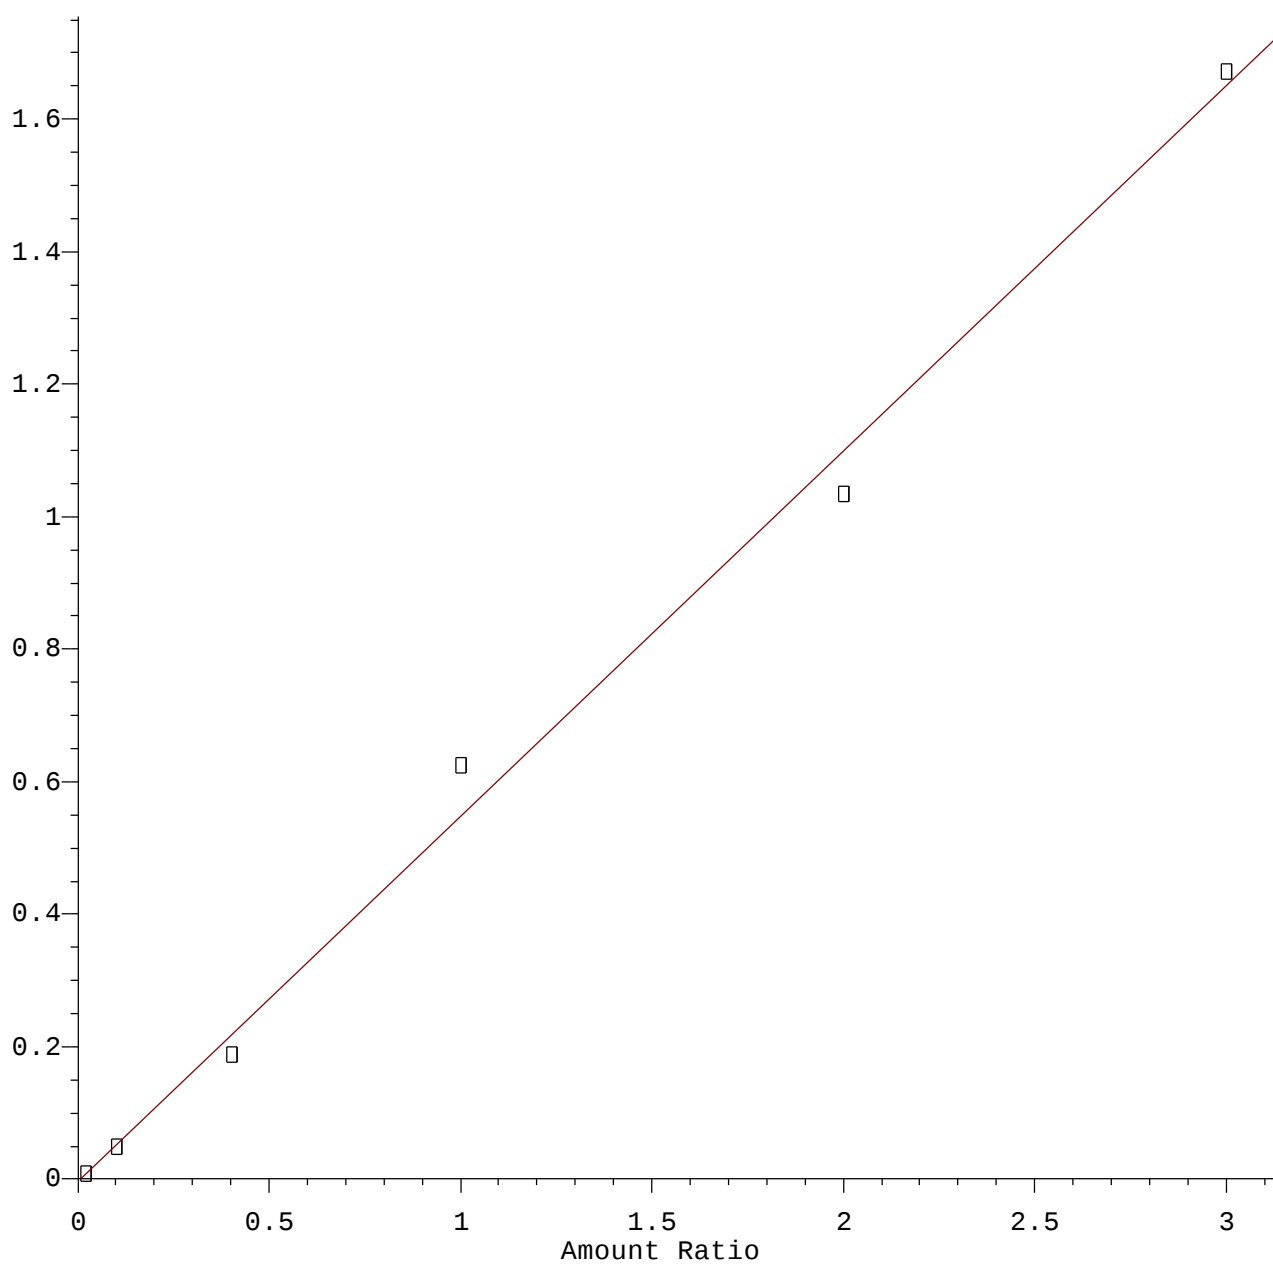


Resp Ratio = $5.51 \times 10^{-1} \times \text{Amt} - 2.90 \times 10^{-3}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U110218W.M
Calibration Table Last Updated: Fri Nov 02 02:28:20 2018


t-1,3-Dichloropropene

Response Ratio

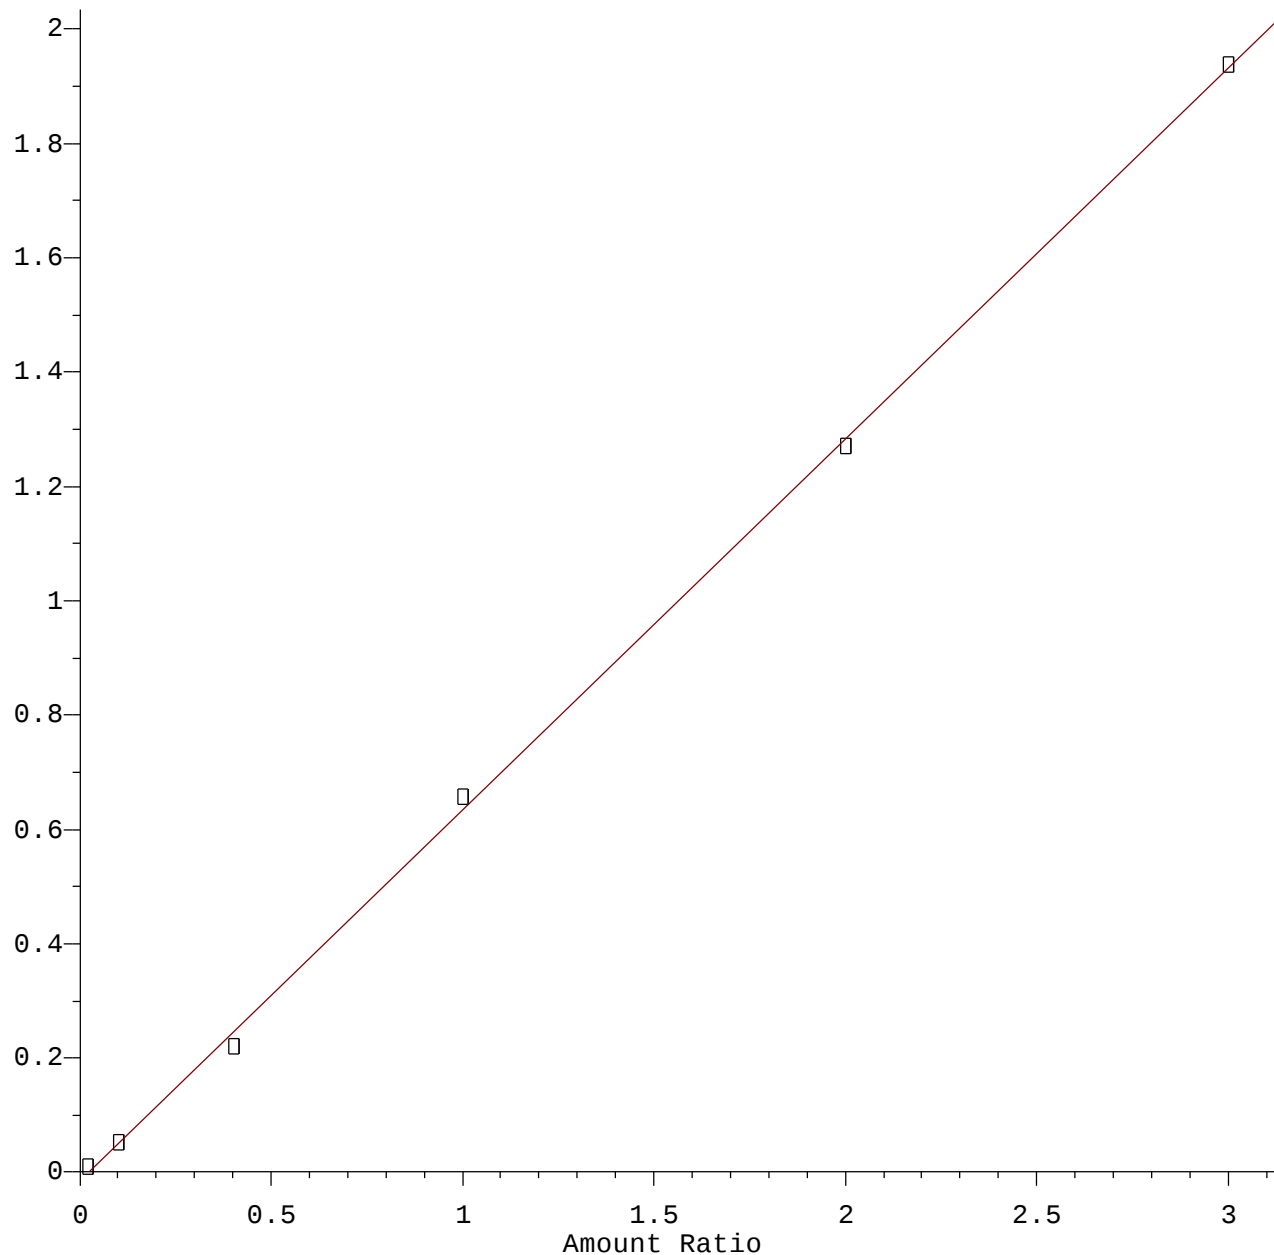

Resp Ratio = 6.49e-001 * Amt - 1.45e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U110218W.M
Calibration Table Last Updated: Fri Nov 02 02:28:20 2018

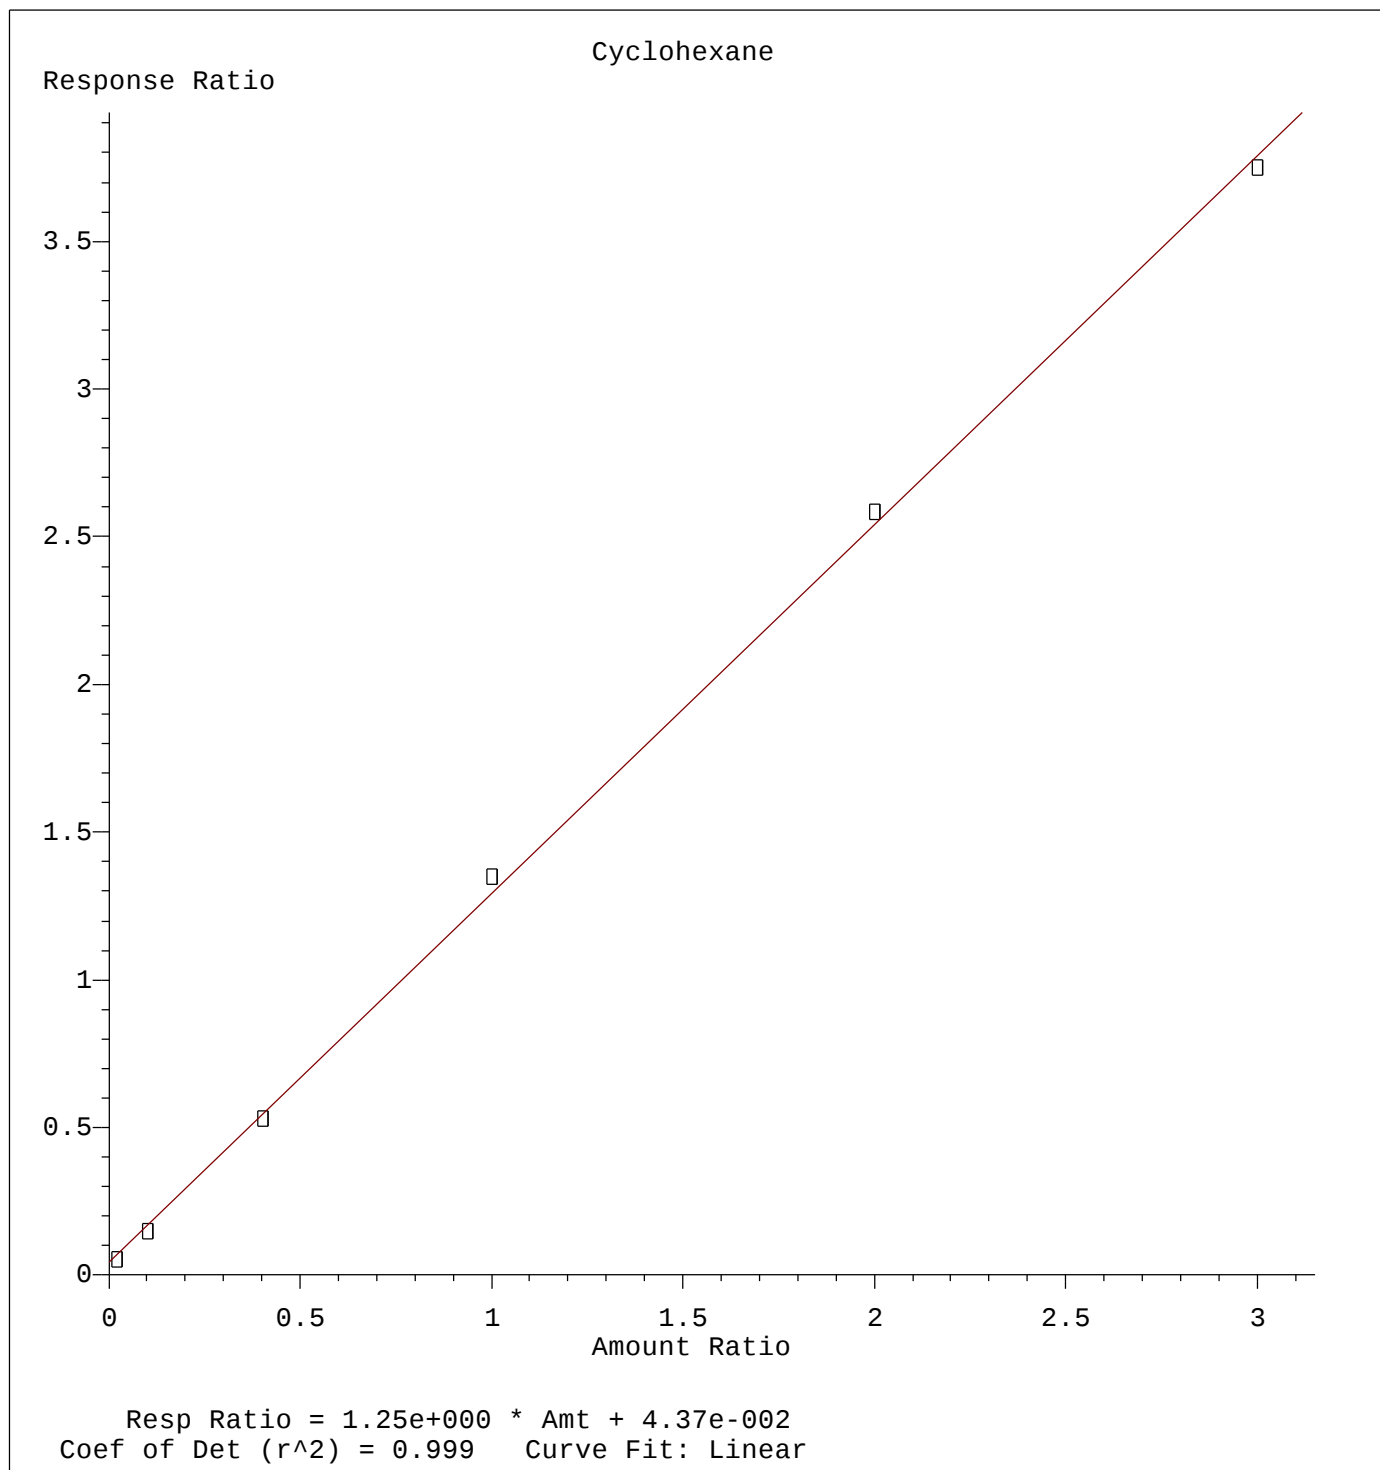

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U110218W.M
Calibration Table Last Updated: Fri Nov 02 02:28:20 2018


Acrolein

Response Ratio

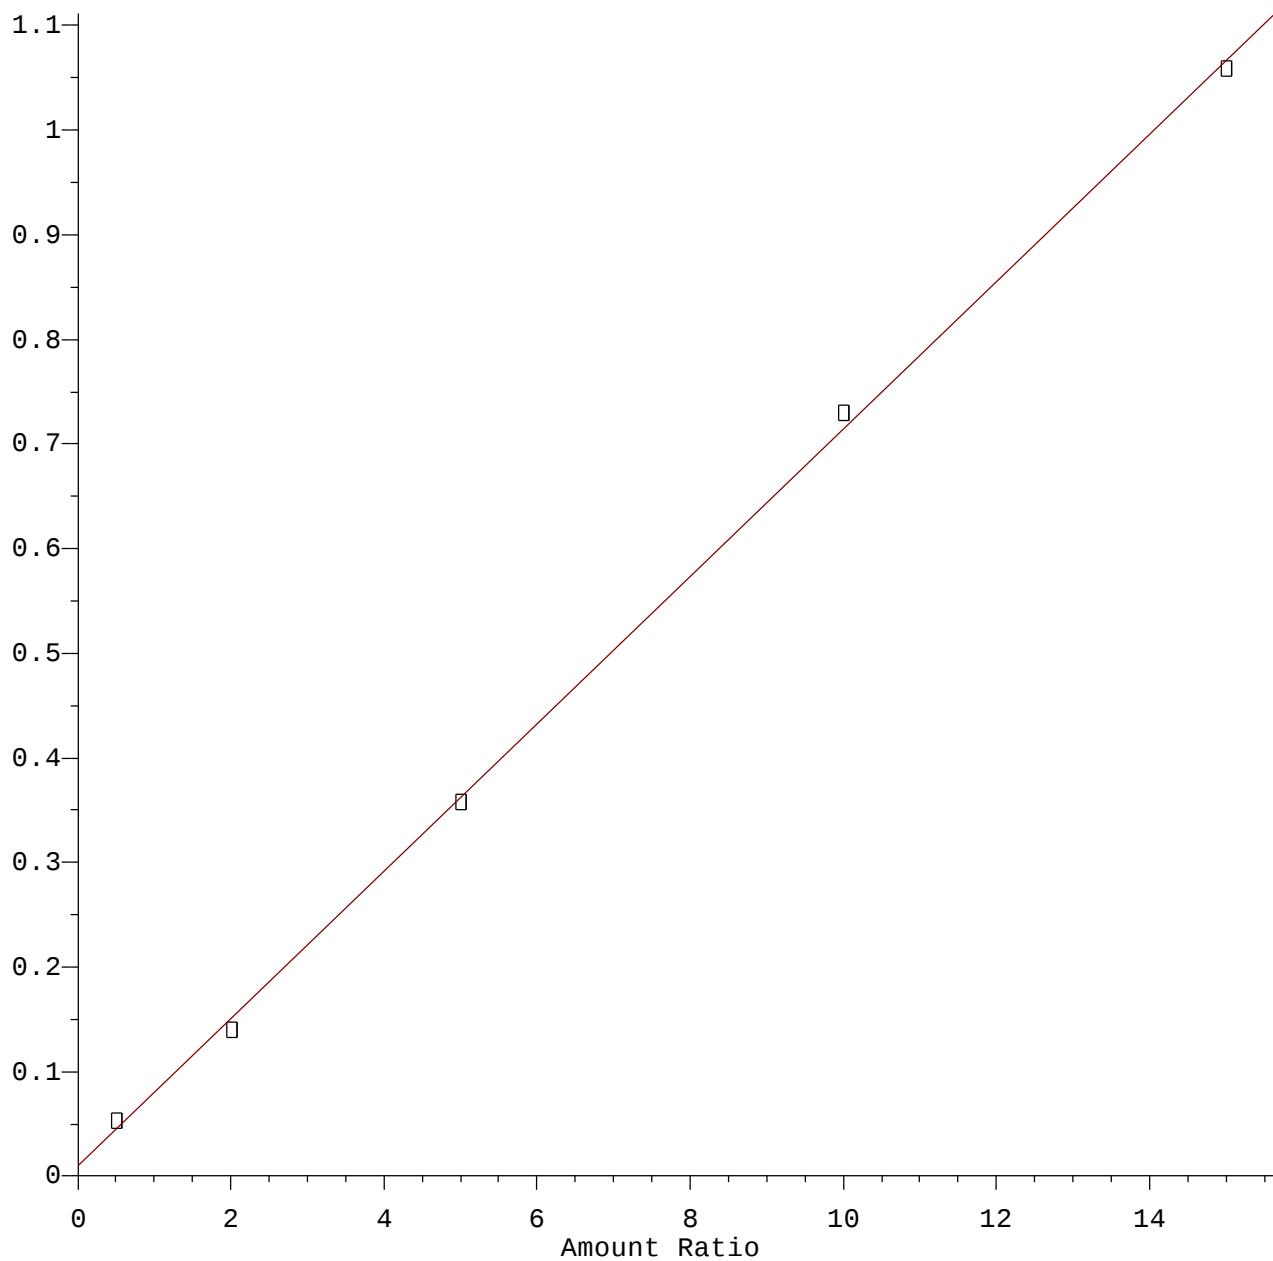

Resp Ratio = 7.04e-002 * Amt + 9.84e-003
Coef of Det (r²) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U110218W.M
Calibration Table Last Updated: Fri Nov 02 02:28:20 2018

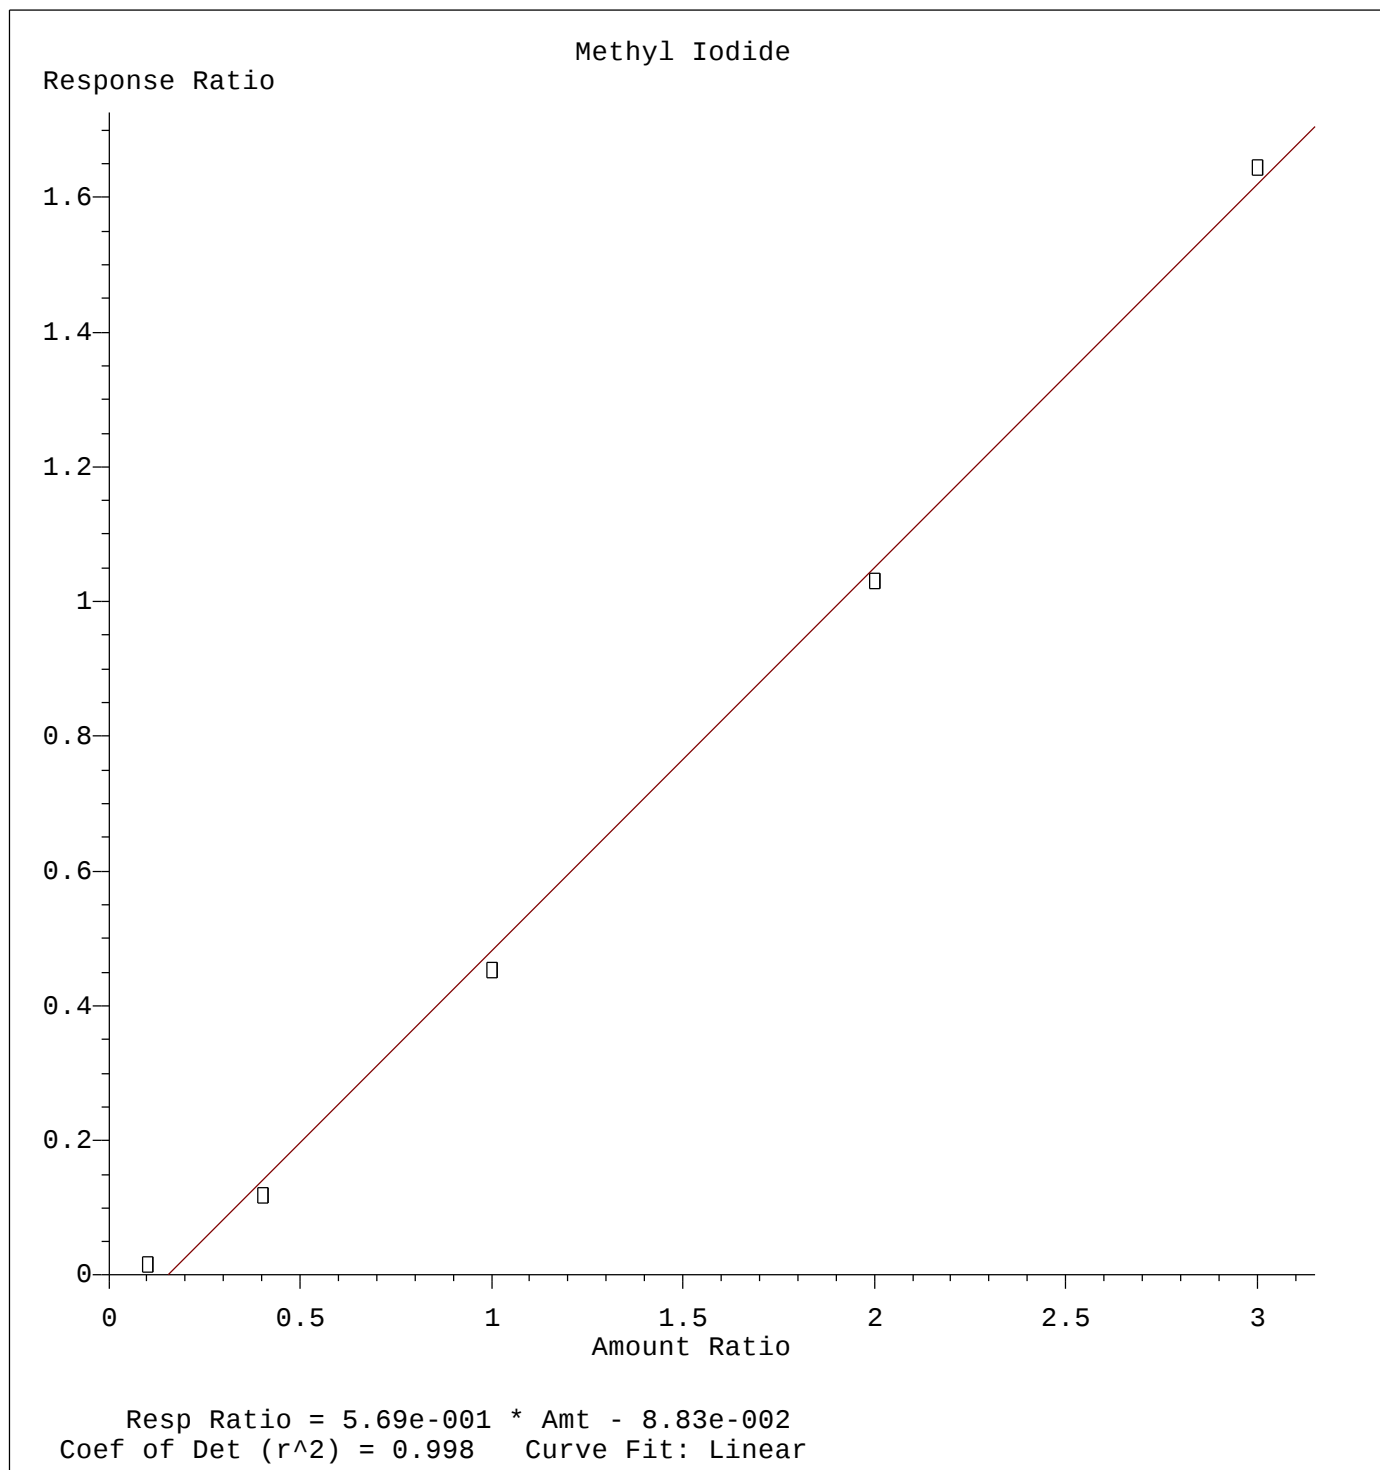

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U110218W.M
Calibration Table Last Updated: Fri Nov 02 02:28:20 2018