

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU110220\
 Data File : VU041057.D
 Acq On : 02 Nov 2020 18:05
 Operator : SY/MD
 Sample : L4584-01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFSE9

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.527	51	58	67	rBV	15293	16760	5.60%	0.894%
2	1.607	75	83	103	rVB	30228	33908	11.34%	1.808%
3	1.925	173	182	192	rBV	22271	28476	9.52%	1.518%
4	2.469	342	351	363	rVB2	10037	15754	5.27%	0.840%
5	2.581	373	386	400	rBV	46103	75732	25.32%	4.038%
6	2.658	400	410	430	rVB3	1862	4923	1.65%	0.263%
7	4.655	1015	1031	1062	rBV	42663	123857	41.41%	6.605%
8	5.083	1150	1164	1182	rBB2	40550	87968	29.41%	4.691%
9	5.742	1347	1369	1390	rBV3	79622	208551	69.72%	11.121%
10	6.173	1491	1503	1513	rBV2	3961	7553	2.53%	0.403%
11	6.263	1518	1531	1548	rVV	66355	121959	40.77%	6.504%
12	6.703	1656	1668	1684	rBV3	51609	98122	32.80%	5.232%
13	7.575	1928	1939	1951	rBV	25535	42847	14.32%	2.285%
14	7.722	1974	1985	1996	rVB4	6276	11289	3.77%	0.602%
15	7.906	2028	2042	2056	rBV	91135	152143	50.87%	8.113%
16	8.185	2119	2129	2146	rBV3	16965	28685	9.59%	1.530%
17	8.639	2257	2270	2300	rBV	168744	299108	100.00%	15.950%
18	9.015	2377	2387	2395	rBV3	5862	8678	2.90%	0.463%
19	9.420	2501	2513	2529	rBV	97226	158361	52.94%	8.445%
20	10.754	2915	2928	2943	rVB	42982	68642	22.95%	3.660%
21	10.890	2962	2970	2978	rBV5	2807	4224	1.41%	0.225%
22	11.806	3240	3255	3272	rVB	88814	139757	46.72%	7.453%
23	12.188	3363	3374	3386	rVB	87182	137981	46.13%	7.358%


Sum of corrected areas: 1875278

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU110220\
Data File : VU041057.D
Acq On : 02 Nov 2020 18:05
Operator : SY/MD
Sample : L4584-01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFSE9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

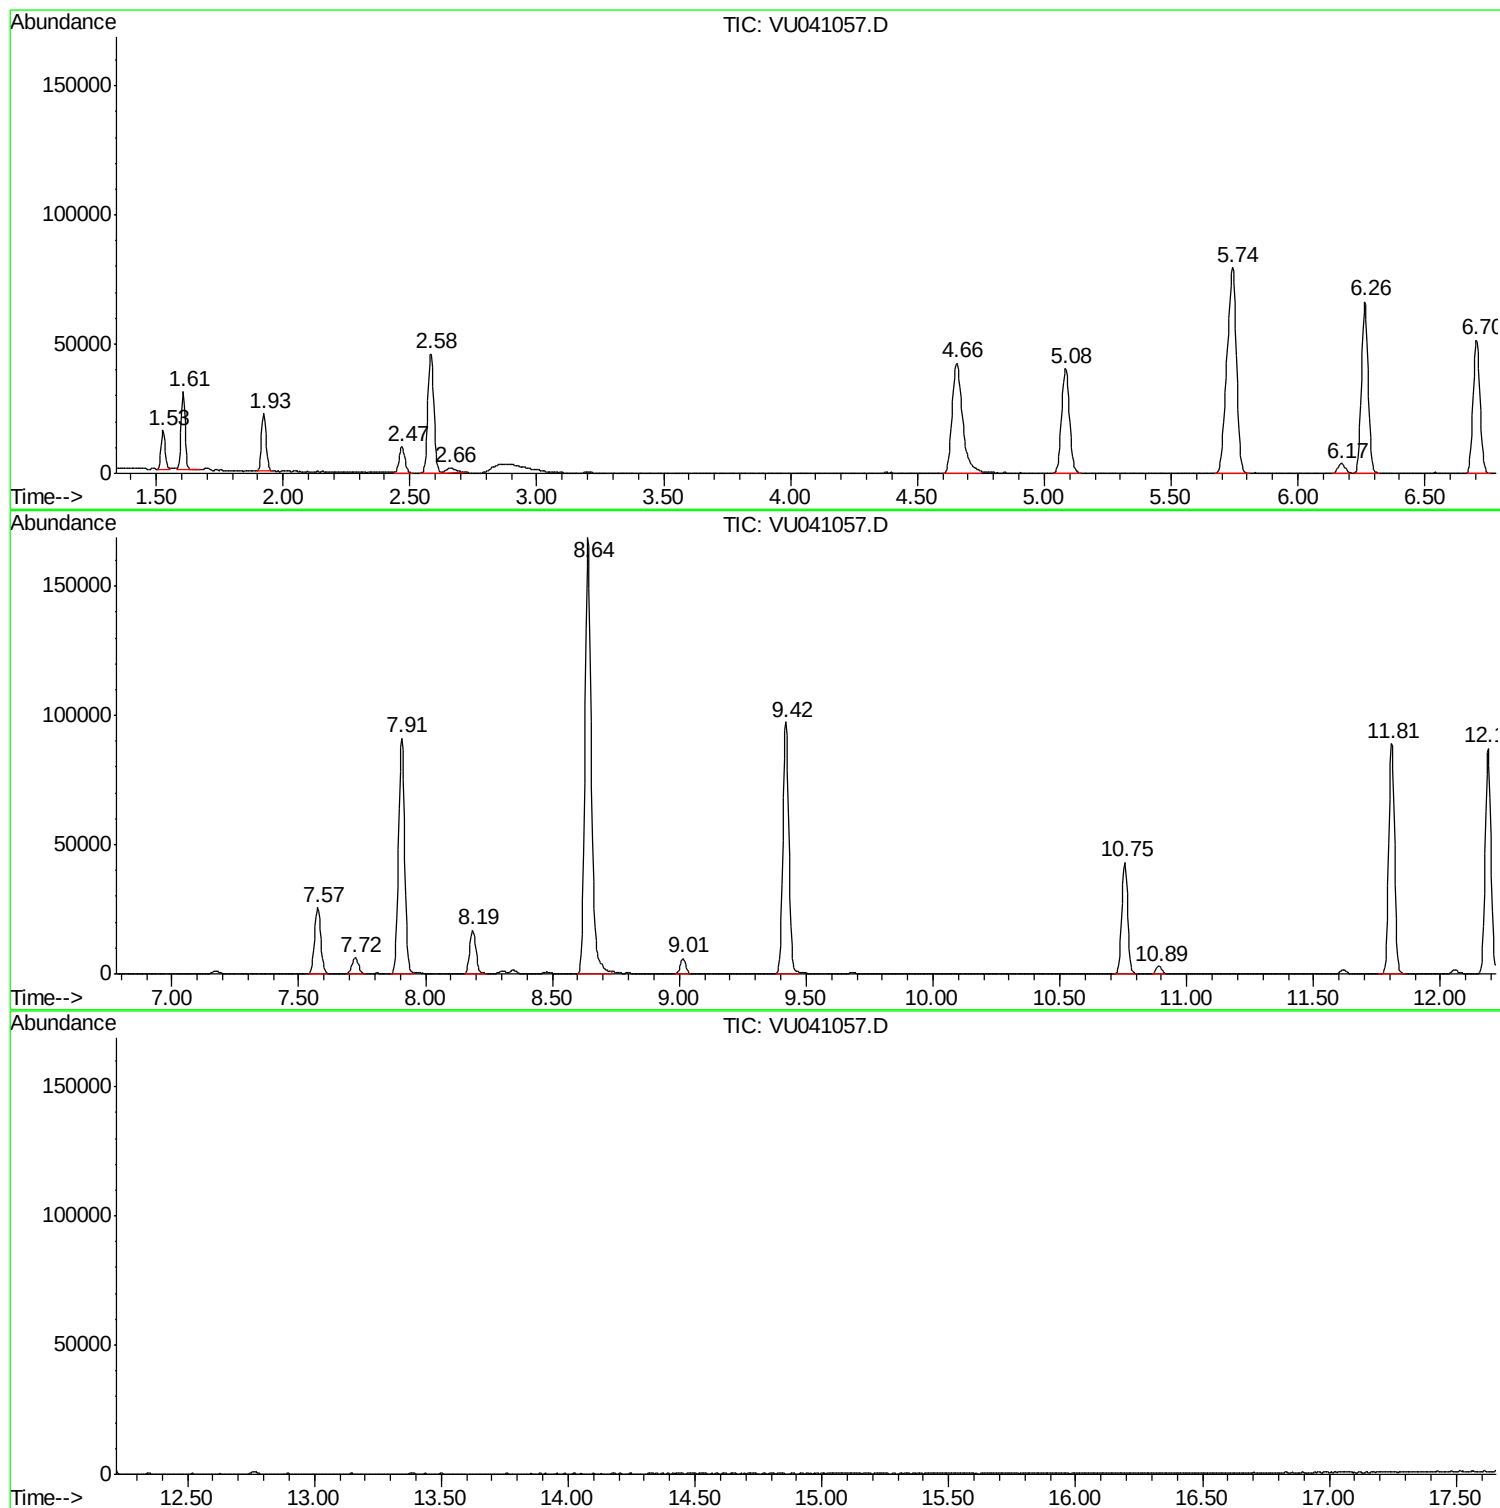

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU110220\
Data File : VU041057.D
Acq On : 02 Nov 2020 18:05
Operator : SY/MD
Sample : L4584-01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
BFSE9










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.47	0.65 ug/L	15754	1,4-Difluorobenzene	6.26

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Propane, 2-chloro-	78	C3H7Cl	000075-29-6	83
2		Propane, 2-chloro-	78	C3H7Cl	000075-29-6	59
3		Propane, 2-chloro-	78	C3H7Cl	000075-29-6	9
4		Propane, 2-nitro-	89	C3H7NO2	000079-46-9	4
5		Propane, 2-nitro-	89	C3H7NO2	000079-46-9	4

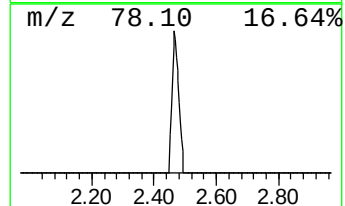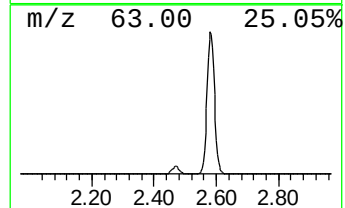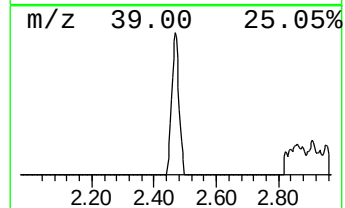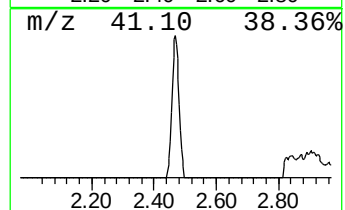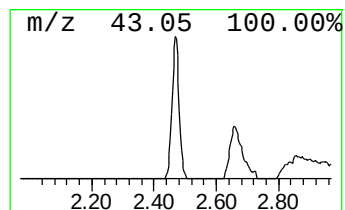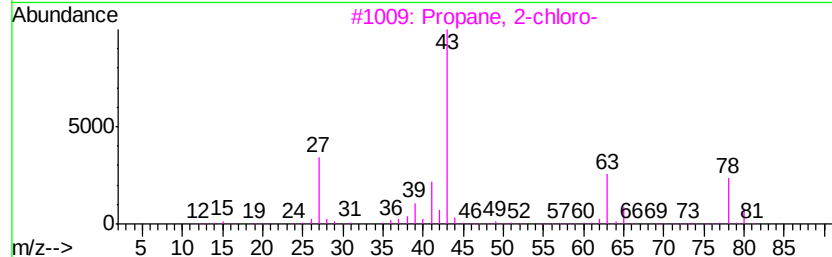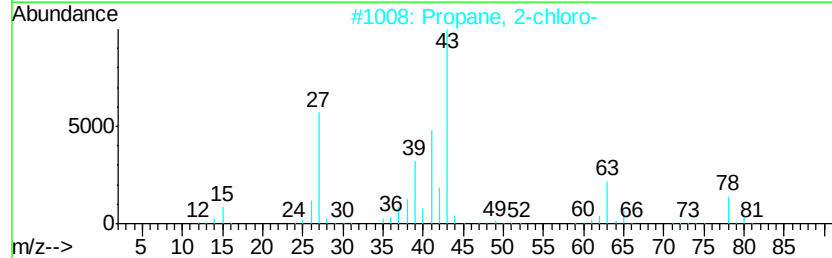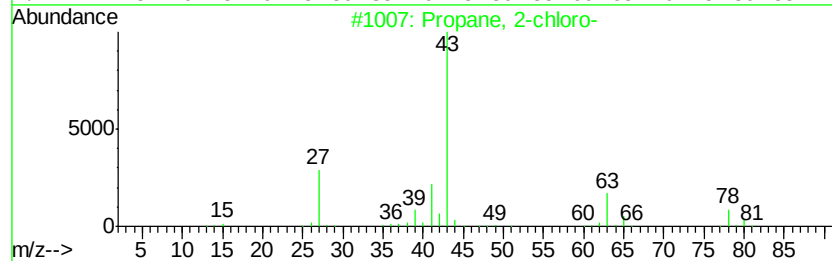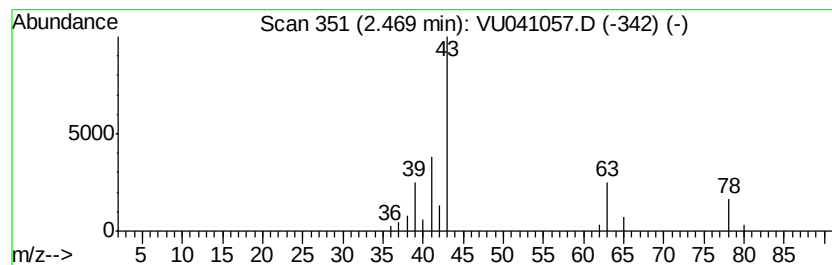

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU110220\
Data File : VU041057.D
Acq On : 02 Nov 2020 18:05
Operator : SY/MD
Sample : L4584-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFSE9

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.47	0.7	ug/L	15754	1	6.26	121959	5.0