

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110221\
 Data File : VU045514.D
 Acq On : 02 Nov 2021 15:12
 Operator : SY/MD
 Sample : M4431-04RE
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BP-VPB-RW9-GW-383-385RE

Quant Time: Nov 02 16:18:29 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U102821W.M
 Quant Title : SW846 8260
 QLast Update : Fri Oct 29 11:09:42 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.379	168	185504	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.253	114	330846	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.420	117	365198	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.816	152	170830	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.707	65	148443	49.152	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	98.300%
35) Dibromofluoromethane	5.292	113	116685	55.467	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	110.940%
50) Toluene-d8	7.899	98	485659	58.873	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	117.740%#
62) 4-Bromofluorobenzene	10.636	95	179918	57.235	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	114.480%
Target Compounds						
16) Acetone	2.646	43	4377	3.192	ug/l	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110221\
Data File : VU045514.D
Acq On : 02 Nov 2021 15:12
Operator : SY/MD
Sample : M4431-04RE
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW9-GW-383-385RE

Quant Time: Nov 02 16:18:29 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U102821W.M
Quant Title : SW846 8260
QLast Update : Fri Oct 29 11:09:42 2021
Response via : Initial Calibration




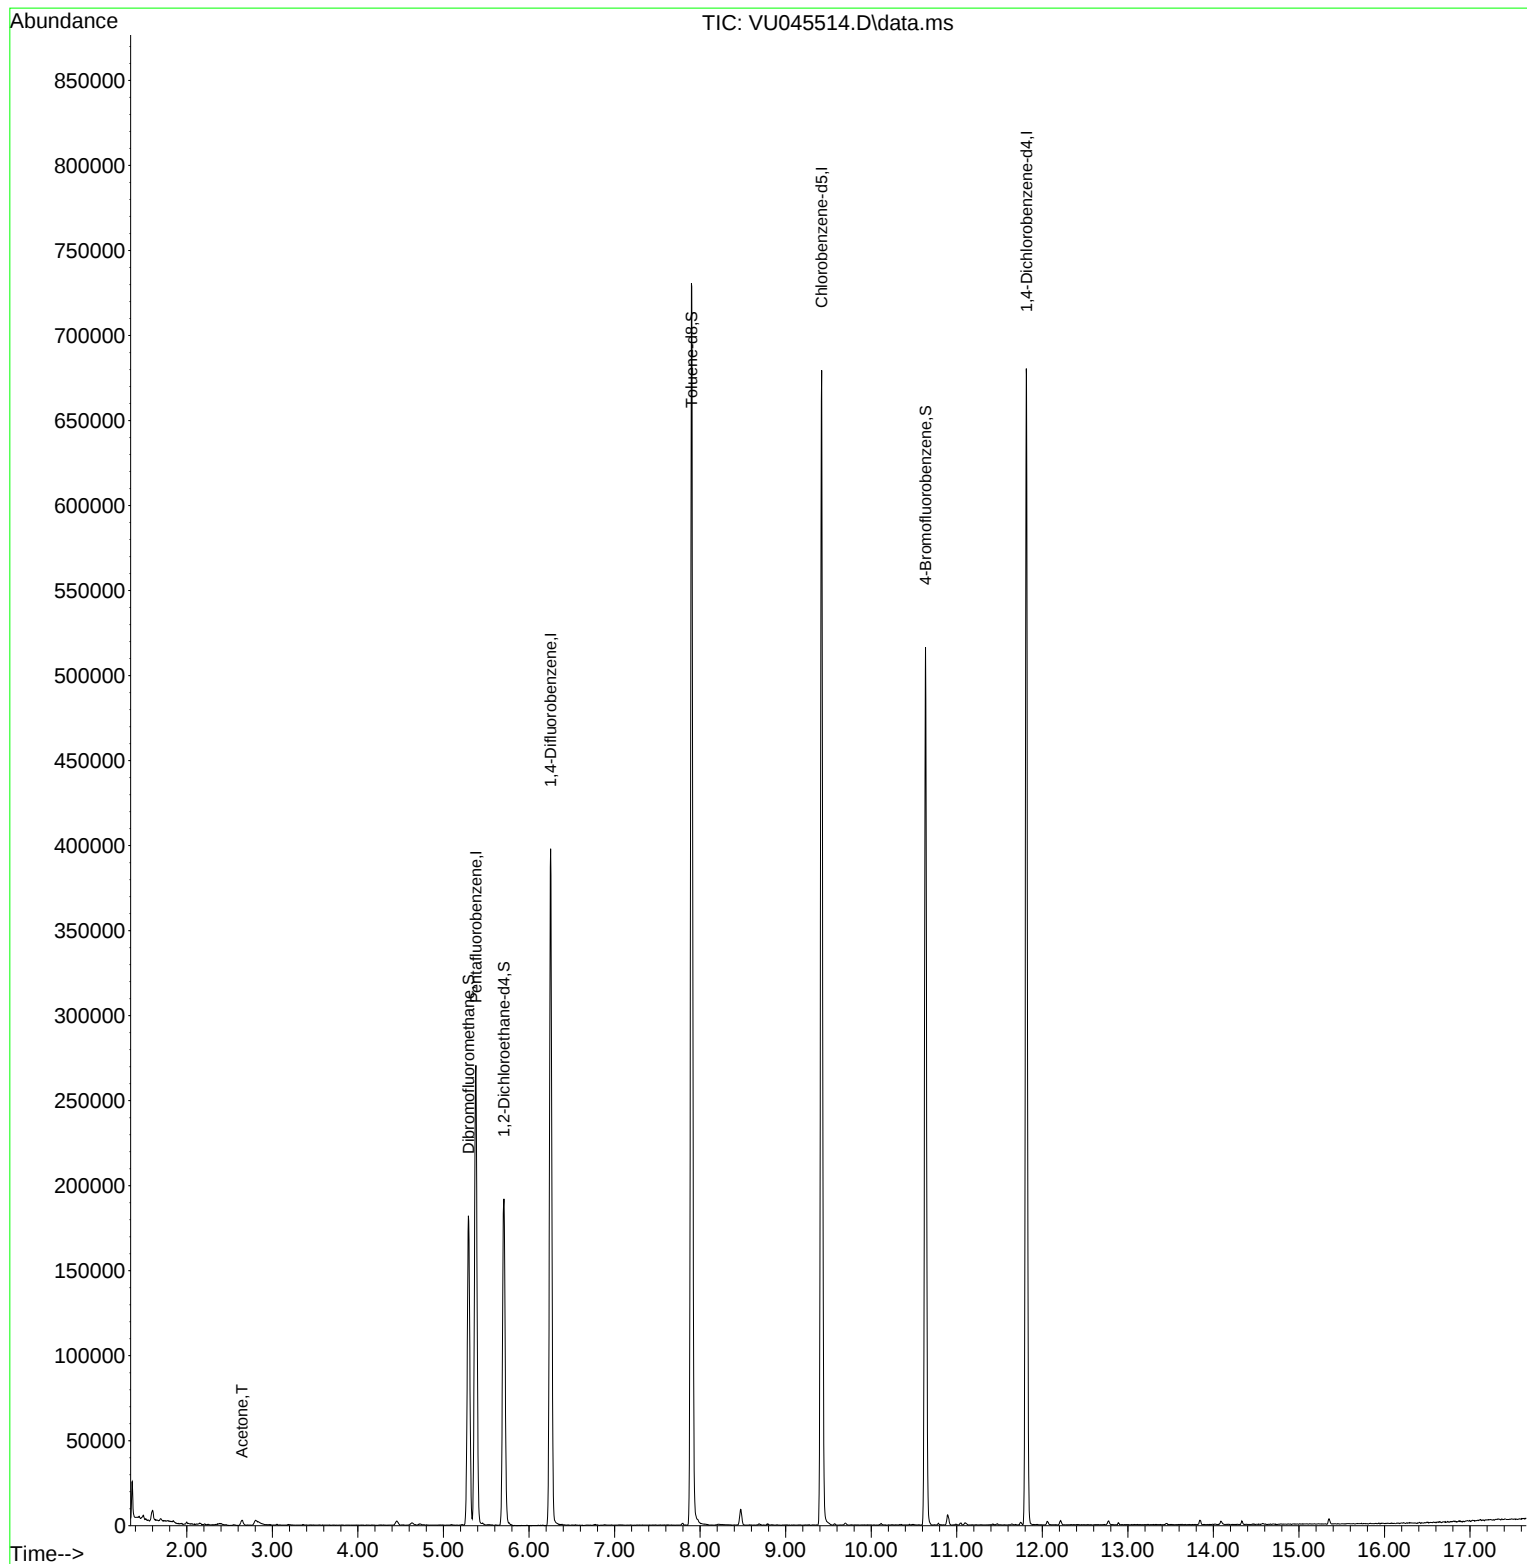


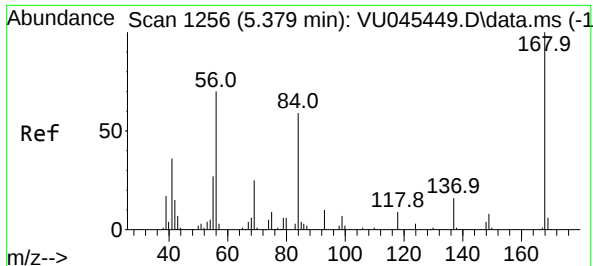

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.379 min Scan# 11
Delta R.T. -0.000 min
Lab File: VU045514.D
Acq: 02 Nov 2021 15:12




Instrument :
MSVOA_U
ClientSampleId :
BP-VPB-RW9-GW-383-385RE


Tgt Ion:168 Resp: 185504
Ion Ratio Lower Upper
168 100
99 61.7 51.0 76.6

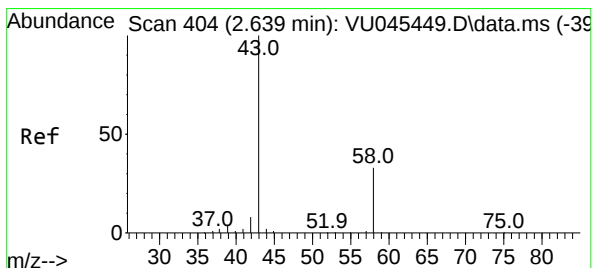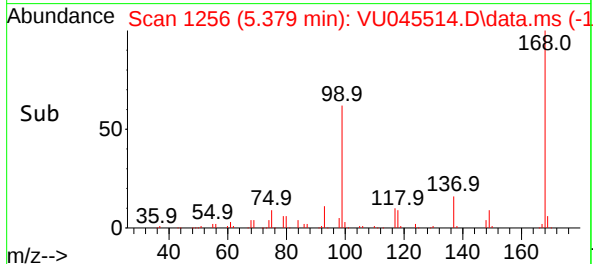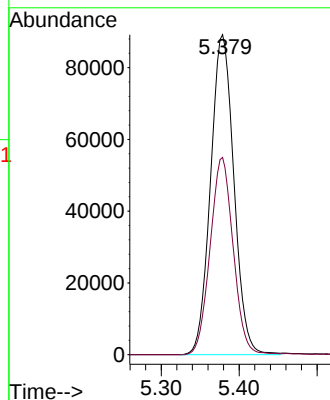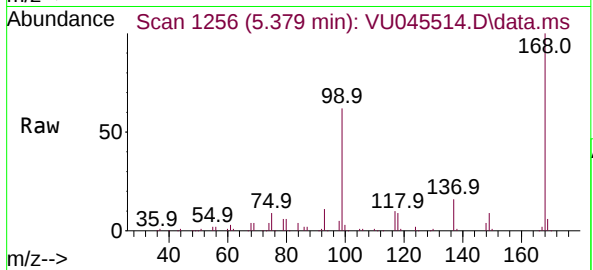

#16
Acetone
Concen: 3.192 ug/l
RT: 2.646 min Scan# 406
Delta R.T. 0.007 min
Lab File: VU045514.D
Acq: 02 Nov 2021 15:12

Tgt Ion: 43 Resp: 4377
Ion Ratio Lower Upper
43 100
58 38.9 26.2 39.2

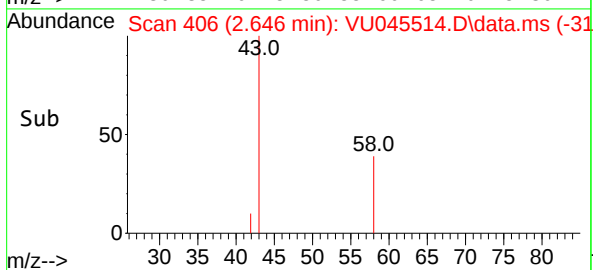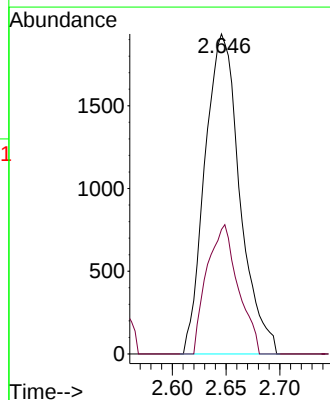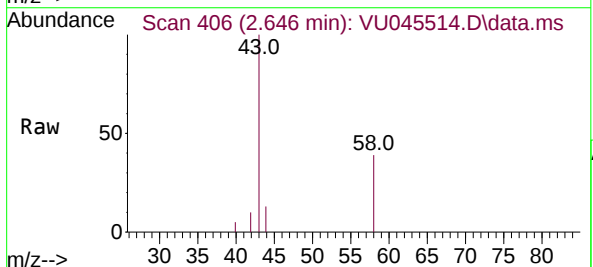

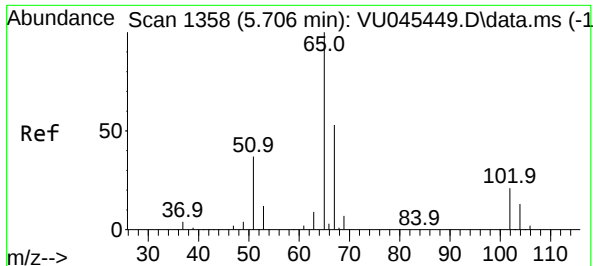

#33

1,2-Dichloroethane-d4

Concen: 49.152 ug/l

RT: 5.707 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU045514.D

Acq: 02 Nov 2021 15:12

Instrument :

MSVOA_U

ClientSampleId :





BP-VPB-RW9-GW-383-385RE

Tgt Ion: 65 Resp: 148443

Ion Ratio Lower Upper

65 100

67 52.8 0.0 105.8

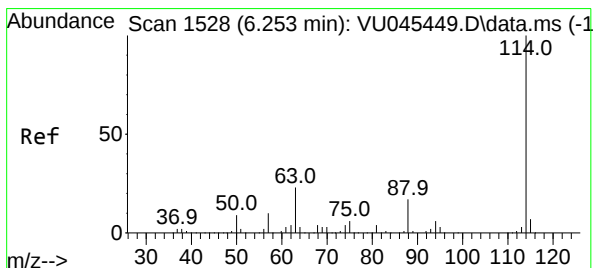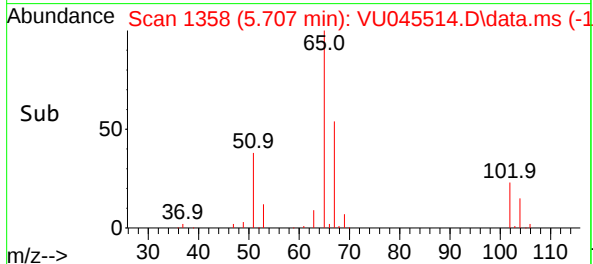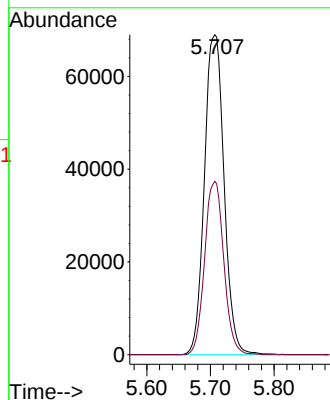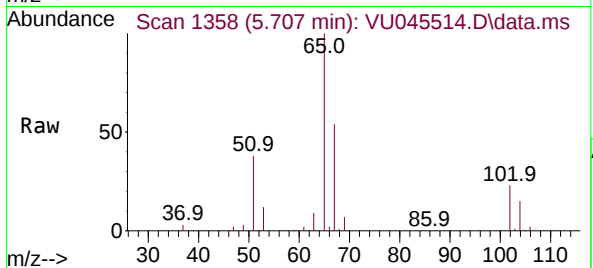

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.253 min Scan# 1528

Delta R.T. 0.000 min

Lab File: VU045514.D

Acq: 02 Nov 2021 15:12




Tgt Ion: 114 Resp: 330846


Ion Ratio Lower Upper

114 100

63 20.7 0.0 45.6

88 16.3 0.0 33.8

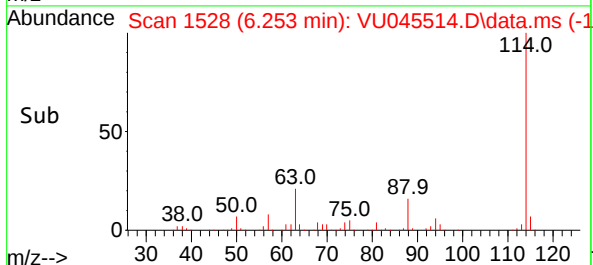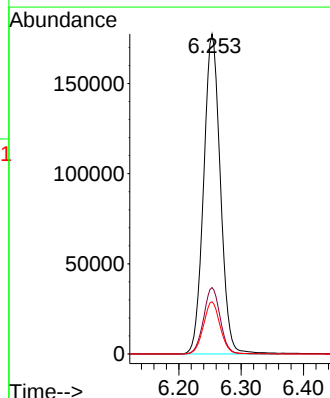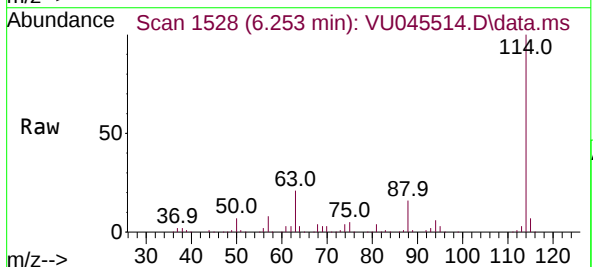

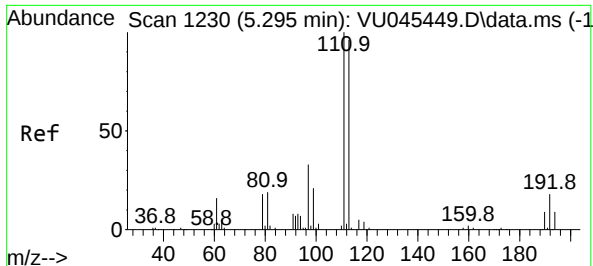

#35

Dibromofluoromethane

Concen: 55.467 ug/l

RT: 5.292 min Scan# 11

Delta R.T. -0.003 min

Lab File: VU045514.D

Acq: 02 Nov 2021 15:12

Instrument :

MSVOA_U

ClientSampleId :

BP-VPB-RW9-GW-383-385RE





Tgt Ion:113 Resp: 116685

Ion Ratio Lower Upper

113 100

111 103.5 82.8 124.2

192 18.5 14.8 22.2

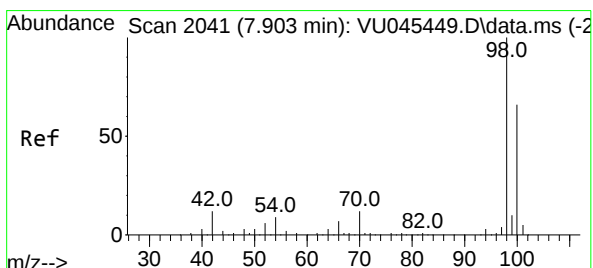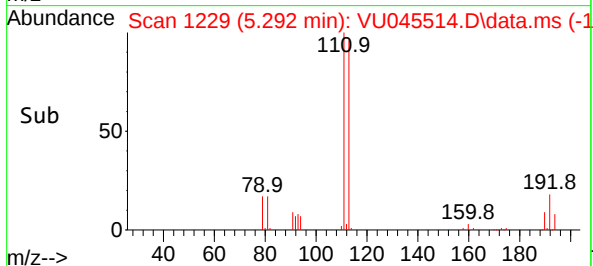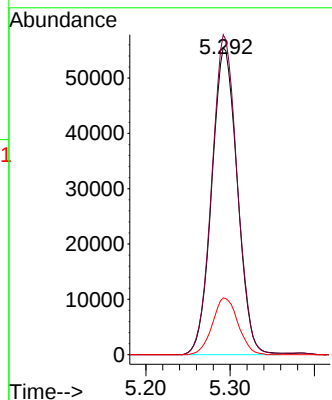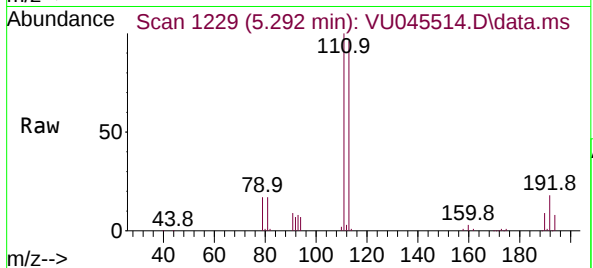

#50

Toluene-d8

Concen: 58.873 ug/l

RT: 7.899 min Scan# 2040

Delta R.T. -0.003 min

Lab File: VU045514.D




Acq: 02 Nov 2021 15:12


Tgt Ion: 98 Resp: 485659

Ion Ratio Lower Upper

98 100

100 65.8 52.5 78.7


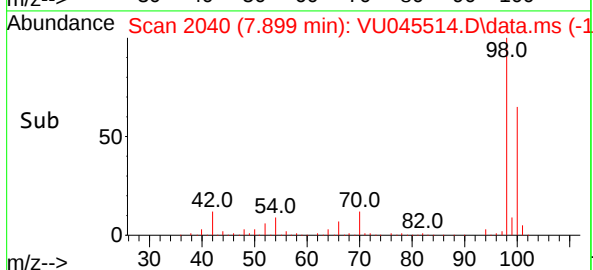
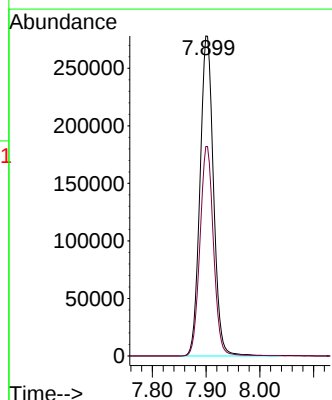
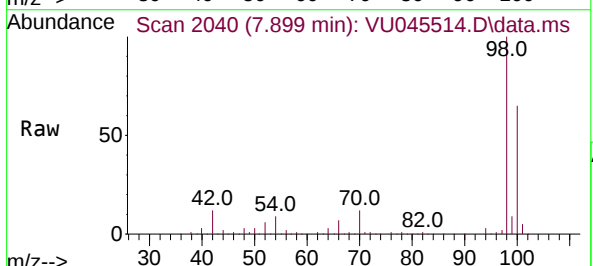


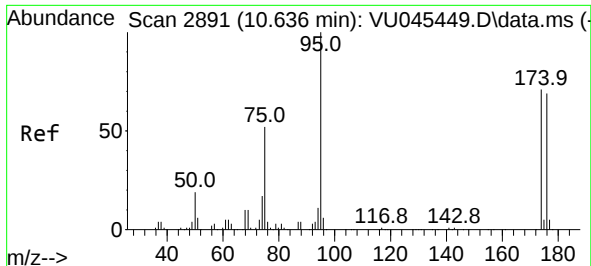

#62
4-Bromofluorobenzene
Concen: 57.235 ug/l
RT: 10.636 min Scan# 2891
Delta R.T. 0.000 min
Lab File: VU045514.D
Acq: 02 Nov 2021 15:12




Instrument : MSVOA_U
ClientSampleId : BP-VPB-RW9-GW-383-385RE


Tgt Ion: 95 Resp: 179918
Ion Ratio Lower Upper
95 100
174 70.9 0.0 141.8
176 68.6 0.0 138.2

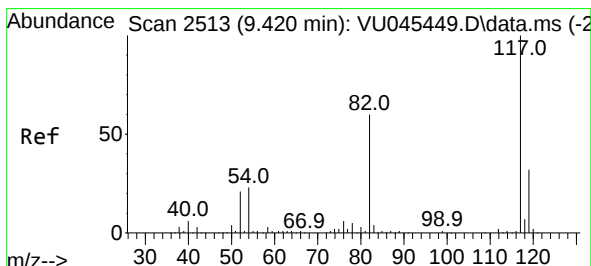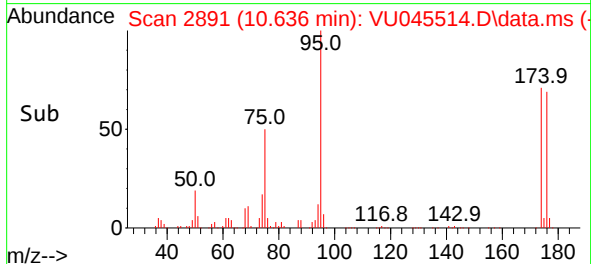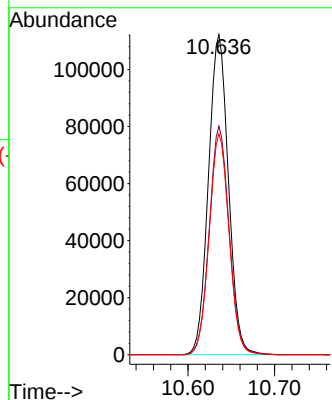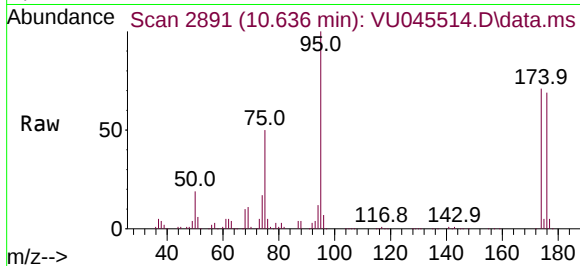

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.420 min Scan# 2513
Delta R.T. 0.000 min
Lab File: VU045514.D
Acq: 02 Nov 2021 15:12

Tgt Ion: 117 Resp: 365198
Ion Ratio Lower Upper
117 100
82 59.8 47.8 71.8
119 31.8 25.8 38.8

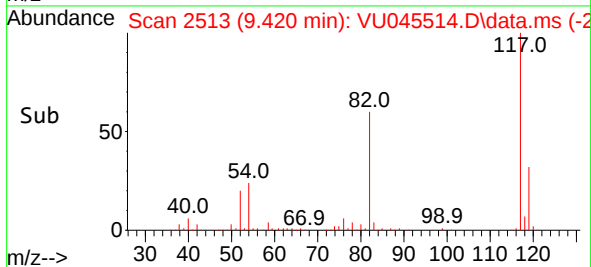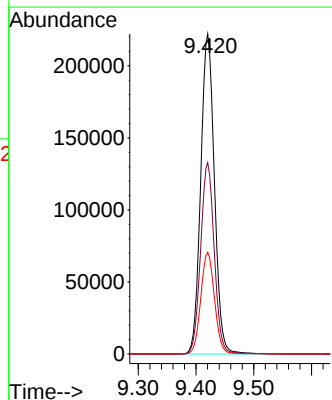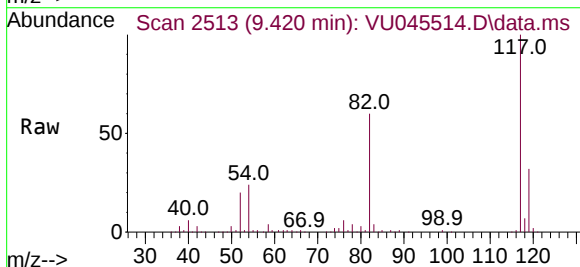

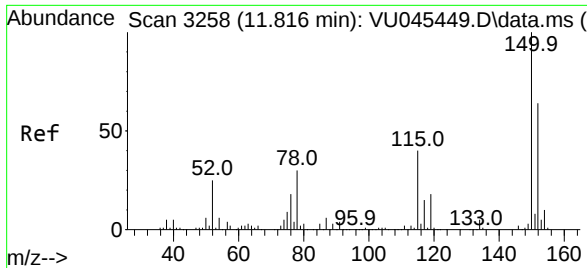

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 11.816 min Scan# 31

Delta R.T. 0.000 min

Lab File: VU045514.D


Acq: 02 Nov 2021 15:12

Instrument :

MSVOA_U

ClientSampleId :

BP-VPB-RW9-GW-383-385RE

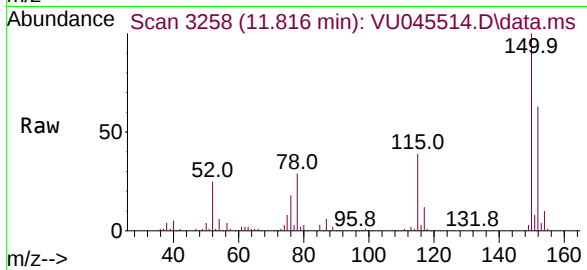

Tgt Ion:152 Resp: 170830

Ion Ratio Lower Upper

152 100

115 62.5 42.7 128.1

150 158.6 0.0 346.8

