

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU110221\  
Data File : VU045501.D  
Acq On : 01 Nov 2021 20:49  
Operator : SY/MD  
Sample : M4431-08  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BP-VPB-RW9-GW-443-445

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U102821W.M

Title : SW846 8260

Signal : TIC: VU045501.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.295       | 1214          | 1230        | 1243         | rBV      | 189664         | 398151        | 30.63%          | 5.798%        |
| 2         | 5.379       | 1243          | 1256        | 1280         | rVB      | 287886         | 593172        | 45.63%          | 8.637%        |
| 3         | 5.707       | 1342          | 1358        | 1381         | rBV      | 224464         | 452179        | 34.79%          | 6.584%        |
| 4         | 6.253       | 1512          | 1528        | 1550         | rBV      | 482541         | 909783        | 69.99%          | 13.248%       |
| 5         | 7.903       | 2026          | 2041        | 2077         | rBV      | 750375         | 1299859       | 100.00%         | 18.928%       |
| 6         | 9.420       | 2500          | 2513        | 2551         | rBV      | 705717         | 1161168       | 89.33%          | 16.908%       |
| 7         | 10.636      | 2878          | 2891        | 2913         | rBV      | 548159         | 870642        | 66.98%          | 12.678%       |
| 8         | 11.816      | 3244          | 3258        | 3277         | rBV      | 752598         | 1182598       | 90.98%          | 17.220%       |




Sum of corrected areas: 6867552

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU110221\  
Data File : VU045501.D  
Acq On : 01 Nov 2021 20:49  
Operator : SY/MD  
Sample : M4431-08  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BP-VPB-RW9-GW-443-445

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U102821W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

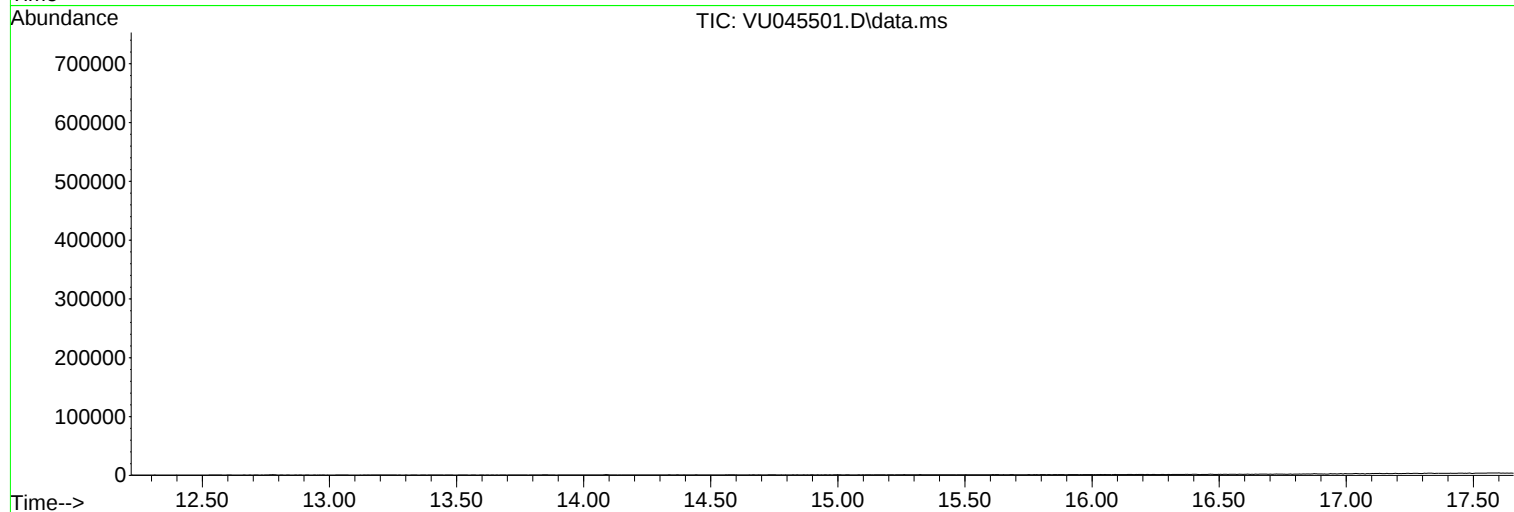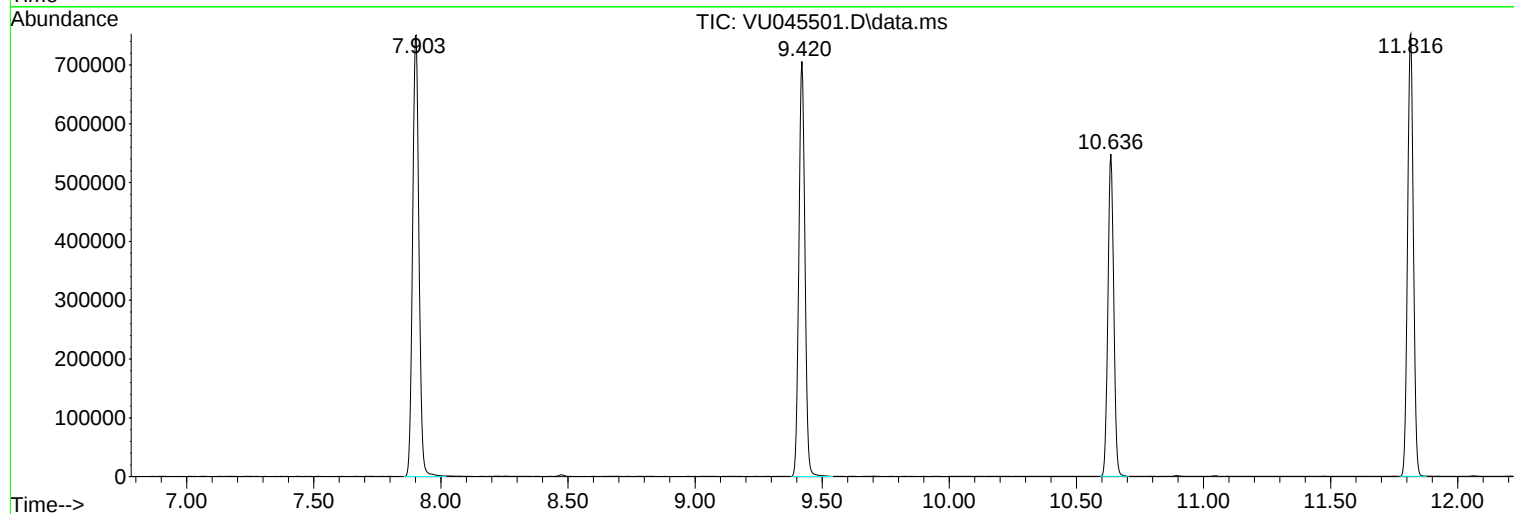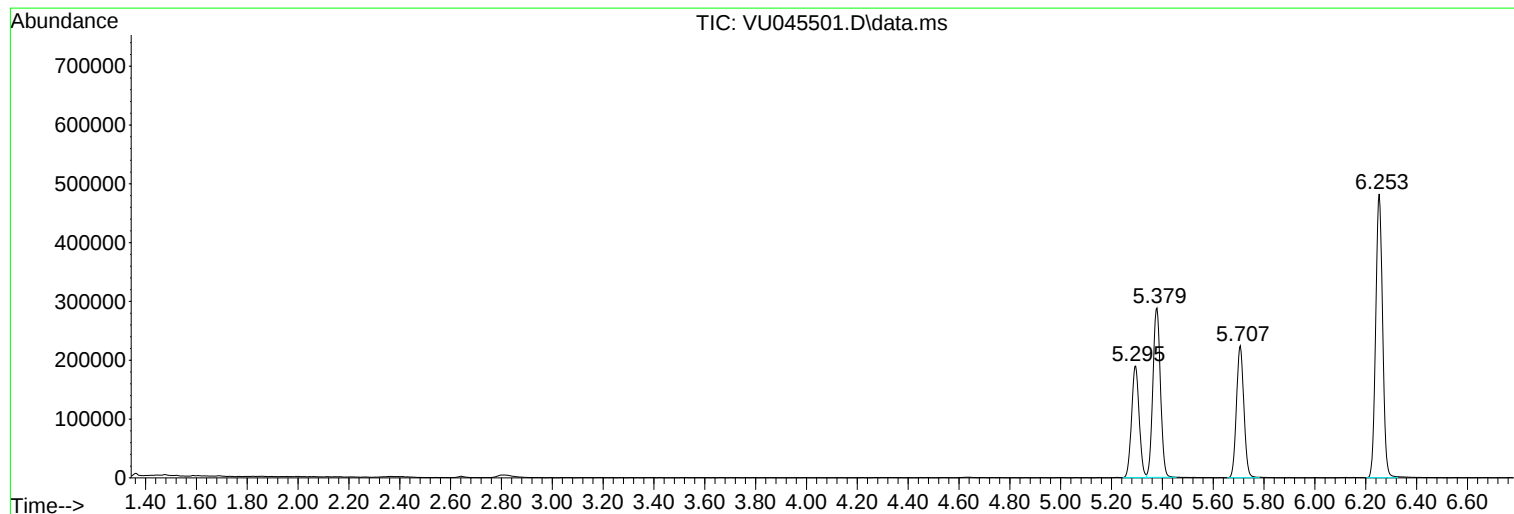

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU110221\  
Data File : VU045501.D  
Acq On : 01 Nov 2021 20:49  
Operator : SY/MD  
Sample : M4431-08  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BP-VPB-RW9-GW-443-445

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U102821W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU110221\  
Data File : VU045501.D  
Acq On : 01 Nov 2021 20:49  
Operator : SY/MD  
Sample : M4431-08  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BP-VPB-RW9-GW-443-445

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U102821W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|