


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110221\
 Data File : VU045488.D
 Acq On : 01 Nov 2021 14:56
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U102821W.M
 Title : SW846 8260
 Last Update : Fri Oct 29 11:09:42 2021

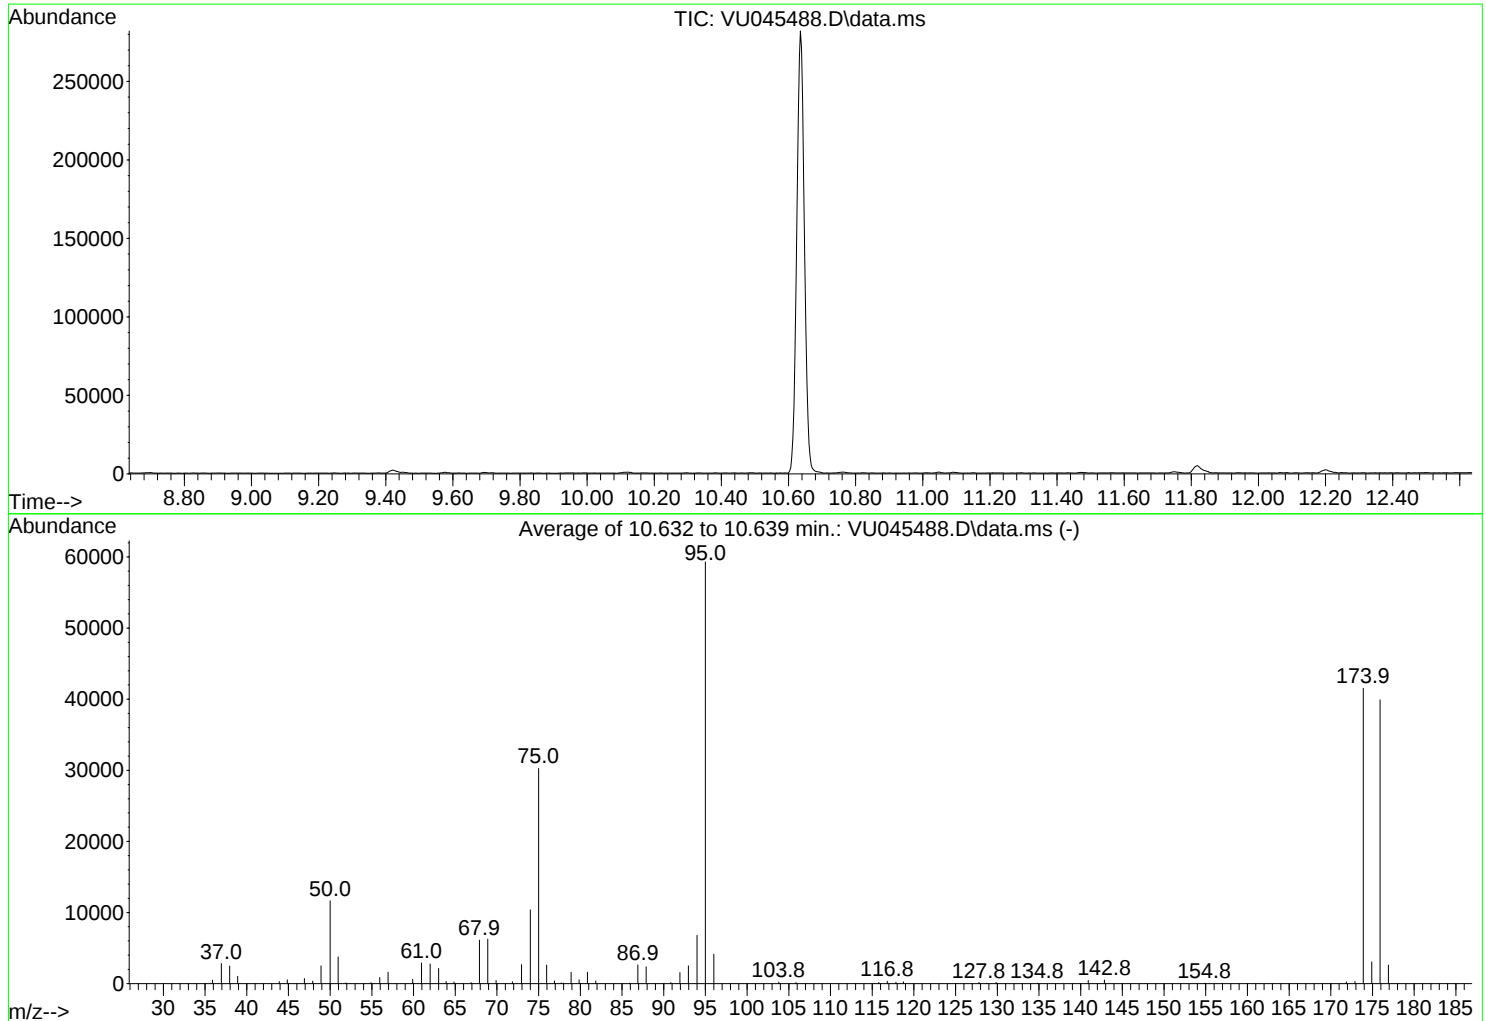

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	11651	PASS
75	95	30	60	51.0	30264	PASS
95	95	100	100	100.0	59317	PASS
96	95	5	9	7.0	4151	PASS
173	174	0.00	2	0.7	292	PASS
174	95	50	100	70.0	41544	PASS
175	174	5	9	7.4	3054	PASS
176	174	95	101	96.1	39912	PASS
177	176	5	9	6.6	2615	PASS