
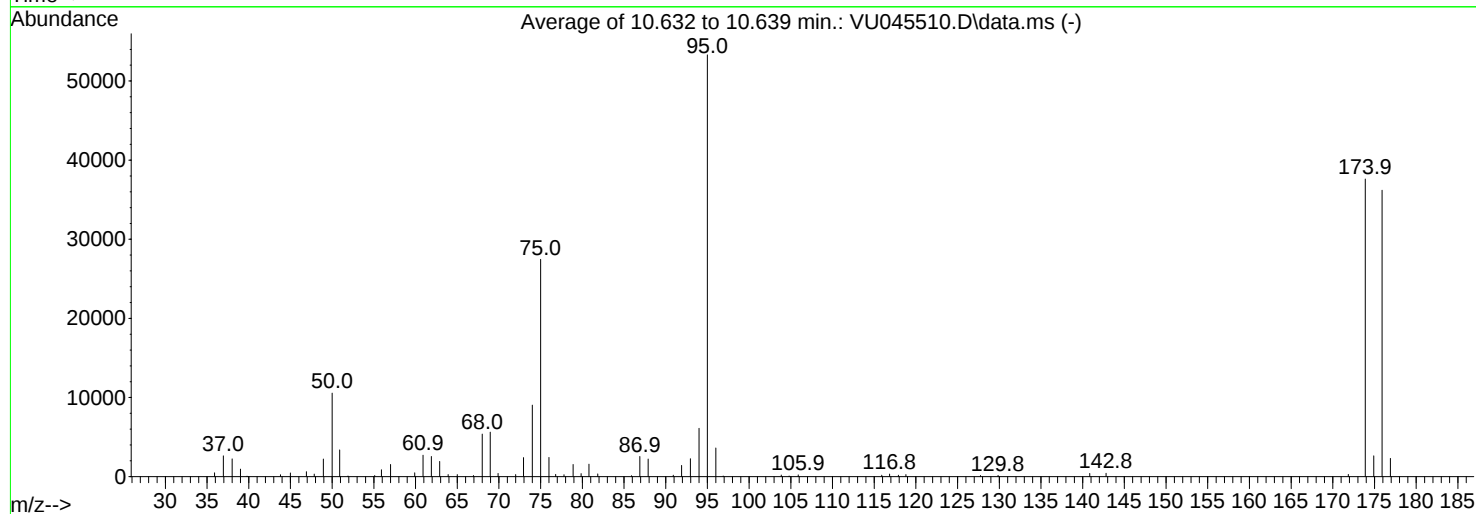


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110221\
Data File : VU045510.D
Acq On : 02 Nov 2021 09:27
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U102821W.M
Title : SW846 8260
Last Update : Fri Oct 29 11:09:42 2021

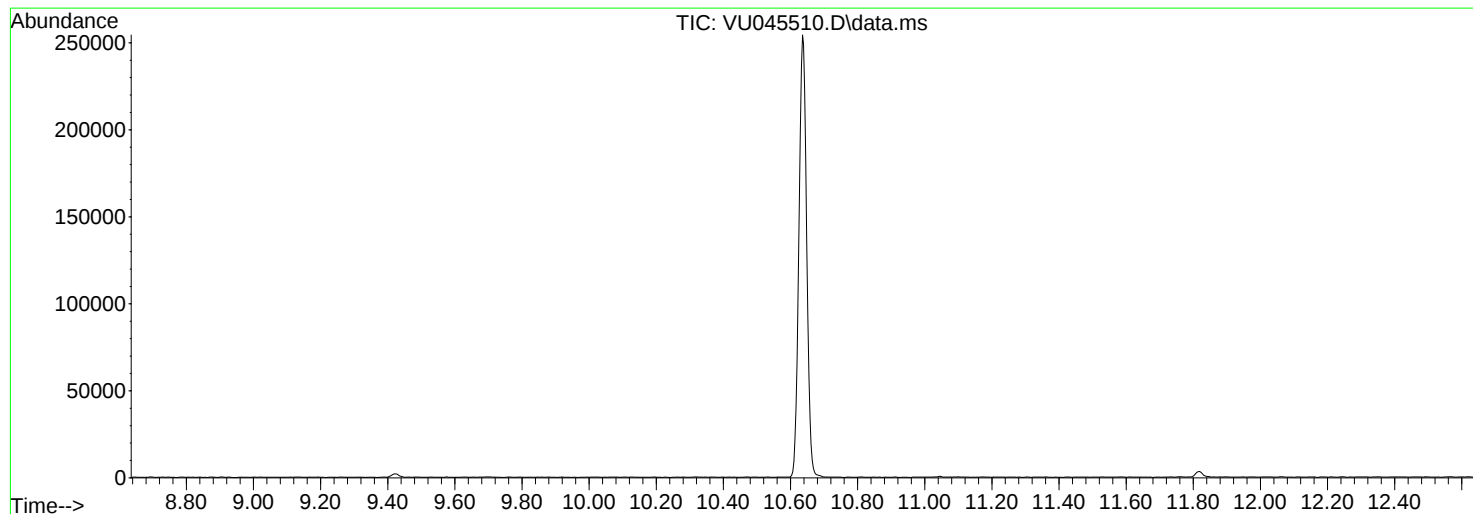

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.8	10560	PASS
75	95	30	60	51.5	27459	PASS
95	95	100	100	100.0	53307	PASS
96	95	5	9	6.8	3627	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.6	37613	PASS
175	174	5	9	7.0	2626	PASS
176	174	95	101	96.2	36192	PASS
177	176	5	9	6.4	2310	PASS