

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110223\
 Data File : VU056057.D
 Acq On : 02 Nov 2023 11:45
 Operator : MD/SY
 Sample : 05112-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056057.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.602	88	97	112	rVB	155735	193215	16.31%	2.059%
2	1.917	185	195	217	rBV	119013	175886	14.85%	1.875%
3	2.567	384	397	420	rBV	277351	460301	38.86%	4.906%
4	3.046	535	546	560	rBV2	14814	30701	2.59%	0.327%
5	3.181	573	588	604	rBV	44394	105028	8.87%	1.119%
6	4.647	1023	1044	1090	rBV2	99396	423495	35.75%	4.514%
7	5.062	1156	1173	1201	rBV	227934	532828	44.98%	5.679%
8	5.724	1357	1379	1399	rBV2	457417	1184542	100.00%	12.626%
9	6.248	1526	1542	1565	rBV	381867	764520	64.54%	8.149%
10	6.689	1665	1679	1704	rBV	268971	545203	46.03%	5.811%
11	7.107	1796	1809	1821	rBV5	7143	12725	1.07%	0.136%
12	7.563	1939	1951	1968	rBV3	124374	236853	20.00%	2.525%
13	7.898	2042	2055	2088	rBV	512055	971318	82.00%	10.353%
14	8.181	2131	2143	2162	rBV2	71448	132578	11.19%	1.413%
15	8.640	2272	2286	2322	rBV3	424923	1030773	87.02%	10.987%
16	9.415	2514	2527	2566	rBV	510638	915147	77.26%	9.754%
17	10.756	2932	2944	2962	rBV2	181902	302736	25.56%	3.227%
18	11.811	3260	3272	3304	rBV	410864	704443	59.47%	7.509%
19	12.190	3376	3390	3413	rBV	384324	659506	55.68%	7.030%




Sum of corrected areas: 9381798

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110223\
Data File : VU056057.D
Acq On : 02 Nov 2023 11:45
Operator : MD/SY
Sample : 05112-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

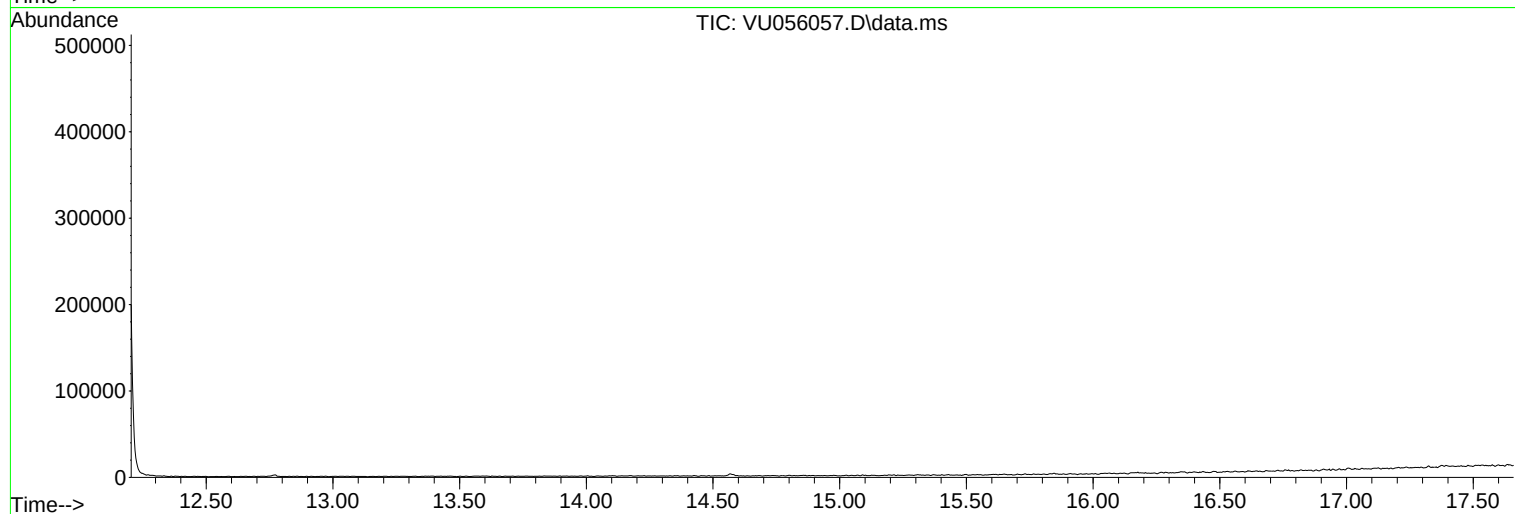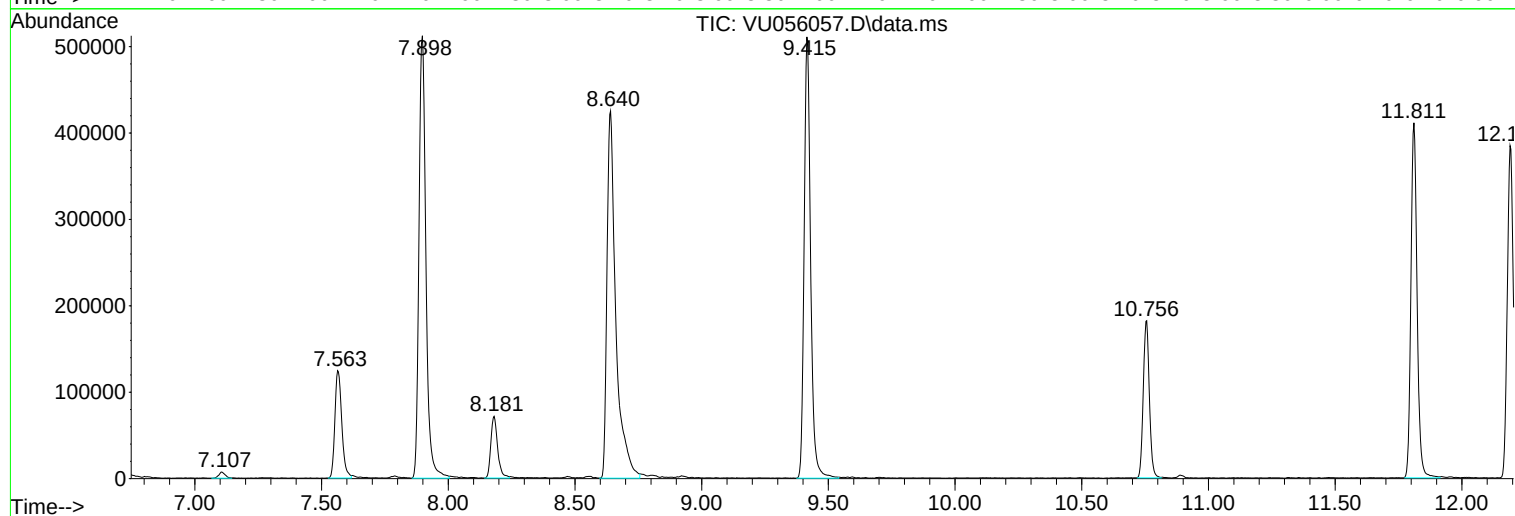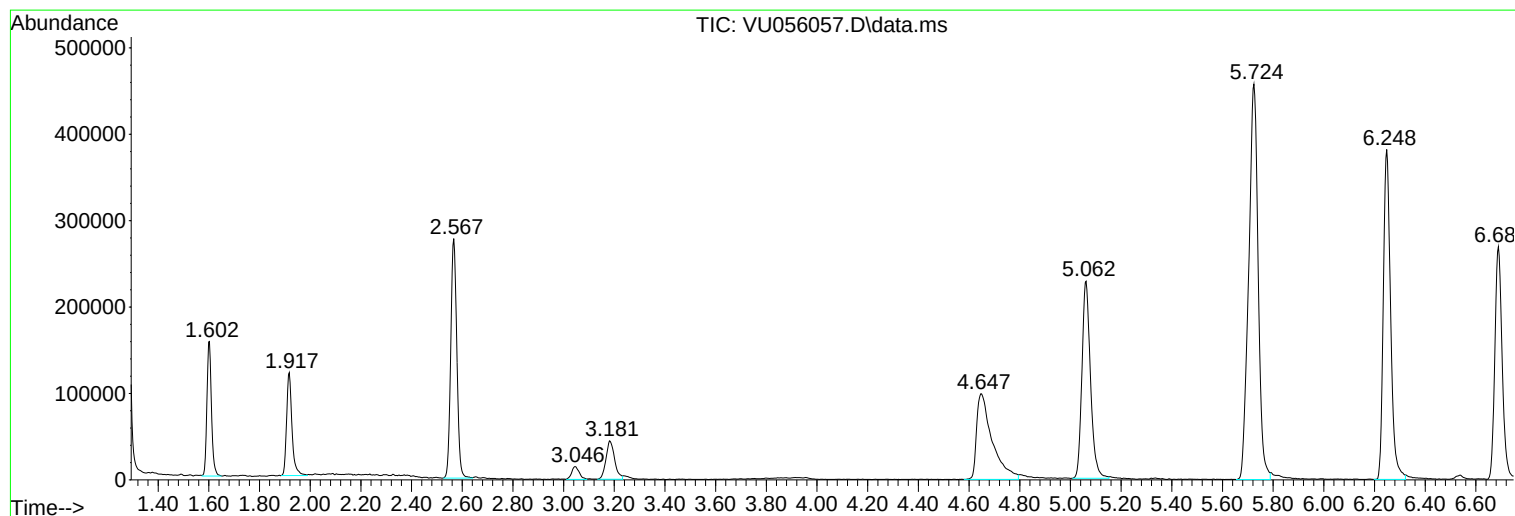

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110223\
Data File : VU056057.D
Acq On : 02 Nov 2023 11:45
Operator : MD/SY
Sample : 05112-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110223\
Data File : VU056057.D
Acq On : 02 Nov 2023 11:45
Operator : MD/SY
Sample : 05112-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc