

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110223\
 Data File : VU056071.D
 Acq On : 02 Nov 2023 17:19
 Operator : MD/SY
 Sample : VIBLK154
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK154

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU056071.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.358	15	21	32	rBV2	10842	12422	1.20%	0.135%
2	1.599	87	96	114	rVB	130435	156126	15.03%	1.693%
3	1.914	185	194	212	rBV	103050	146947	14.15%	1.593%
4	2.567	381	397	415	rBV	218888	363800	35.03%	3.944%
5	3.046	534	546	563	rVB	19750	37807	3.64%	0.410%
6	3.184	576	589	610	rBV	13328	30358	2.92%	0.329%
7	4.634	1026	1040	1076	rBV2	120972	386769	37.24%	4.193%
8	5.062	1155	1173	1209	rBV	201630	507909	48.90%	5.506%
9	5.724	1356	1379	1409	rBV2	398719	1038563	100.00%	11.259%
10	6.245	1528	1541	1577	rBV	389120	781194	75.22%	8.469%
11	6.689	1664	1679	1706	rBV	243276	487728	46.96%	5.287%
12	7.563	1935	1951	1976	rBV	116390	218967	21.08%	2.374%
13	7.894	2042	2054	2071	rBV	457159	835809	80.48%	9.061%
14	8.177	2132	2142	2161	rBV2	67925	124027	11.94%	1.345%
15	8.470	2221	2233	2246	rBV2	14954	28837	2.78%	0.313%
16	8.634	2272	2284	2324	rBV3	453825	1029908	99.17%	11.165%
17	9.415	2513	2527	2548	rBV	547608	976263	94.00%	10.584%
18	9.695	2606	2614	2625	rBV5	6021	11344	1.09%	0.123%
19	10.753	2931	2943	2962	rBV2	171022	292314	28.15%	3.169%
20	10.891	2974	2986	3000	rBV	40099	68016	6.55%	0.737%
21	11.807	3259	3271	3293	rBV	527463	880133	84.75%	9.541%
22	12.071	3344	3353	3374	rBV6	10807	30063	2.89%	0.326%
23	12.190	3377	3390	3407	rBV	426761	711152	68.47%	7.709%
24	12.769	3559	3570	3582	rVB2	8872	14336	1.38%	0.155%
25	12.897	3599	3610	3620	rBV5	7633	14743	1.42%	0.160%
26	14.573	4120	4131	4145	rBV	7135	13073	1.26%	0.142%
27	16.116	4602	4611	4621	rVB3	17947	25763	2.48%	0.279%




Sum of corrected areas: 9224371

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110223\
Data File : VU056071.D
Acq On : 02 Nov 2023 17:19
Operator : MD/SY
Sample : VIBLK154
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK154

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

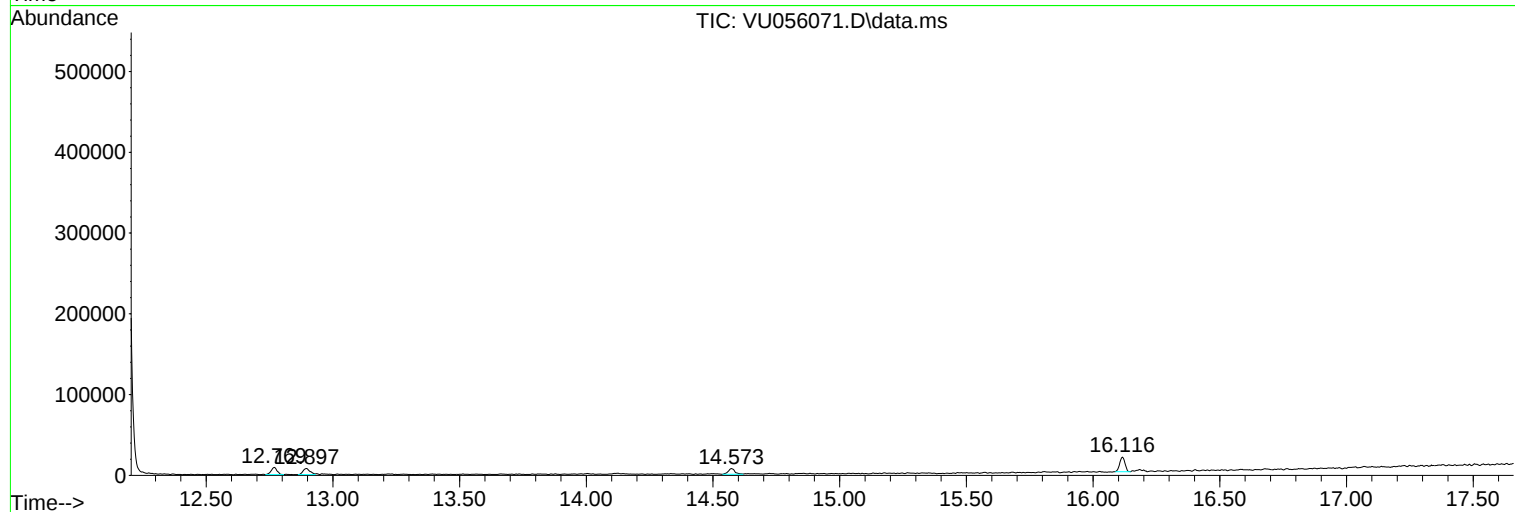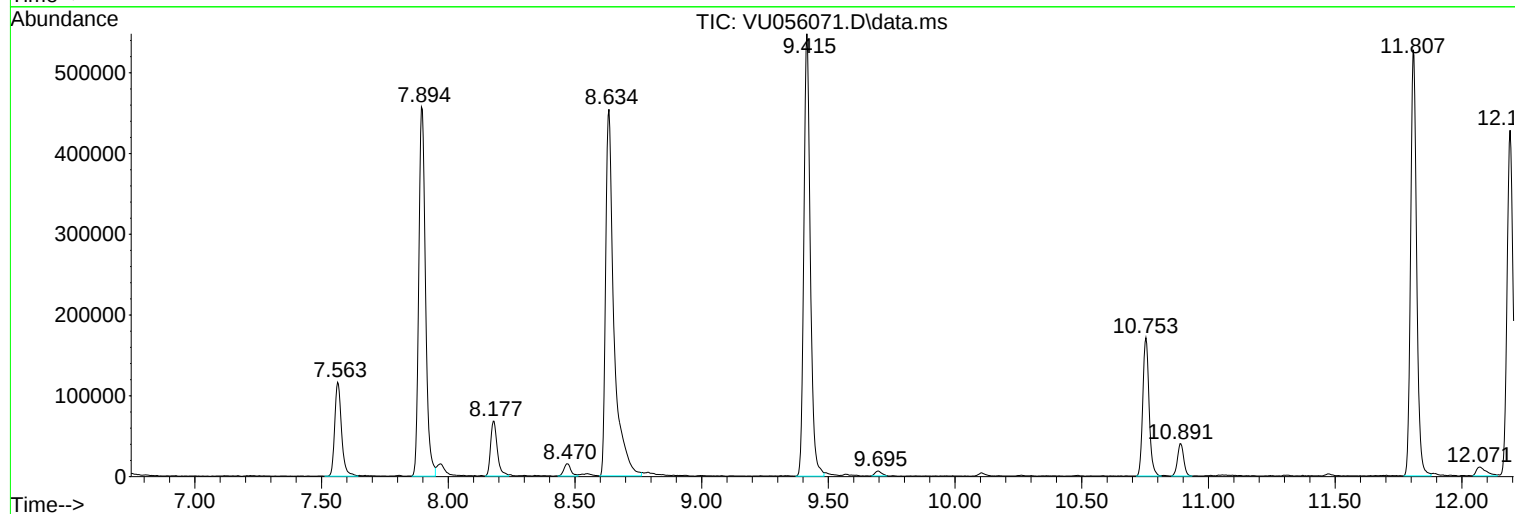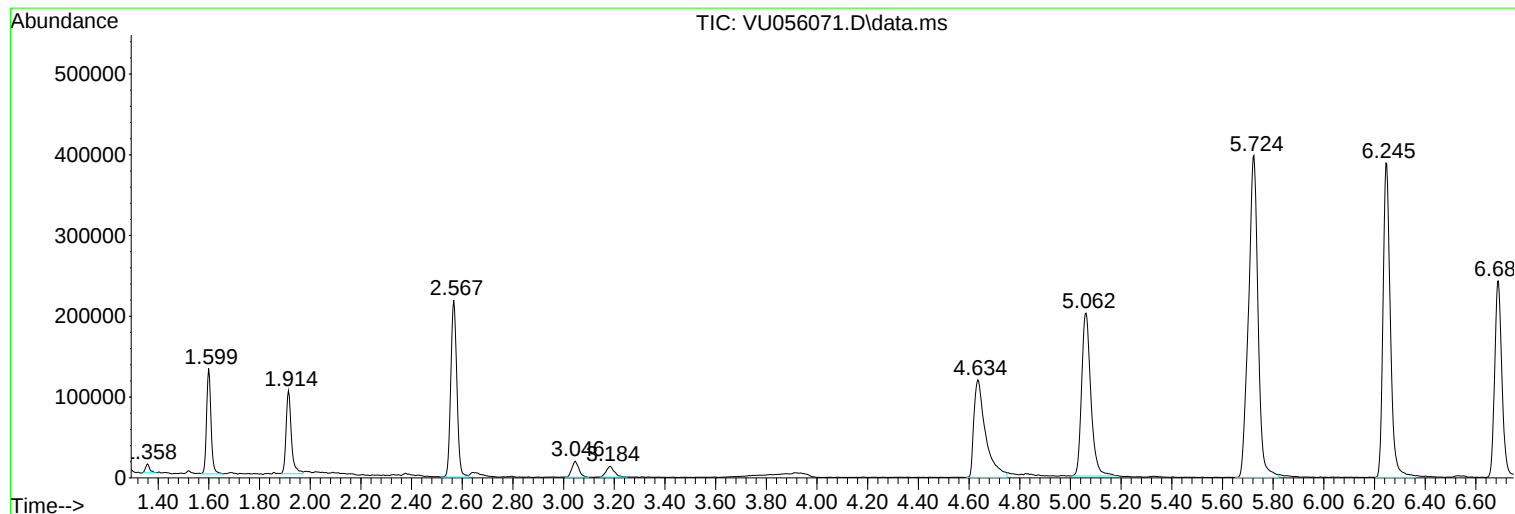

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110223\
Data File : VU056071.D
Acq On : 02 Nov 2023 17:19
Operator : MD/SY
Sample : VIBLK154
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK154

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110223\
Data File : VU056071.D
Acq On : 02 Nov 2023 17:19
Operator : MD/SY
Sample : VIBLK154
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK154

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------