


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110223\
Data File : VU056054.D
Acq On : 02 Nov 2023 08:32
Operator : MD/SY
Sample : BFB064
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB064

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Nov 03 00:21:27 2023

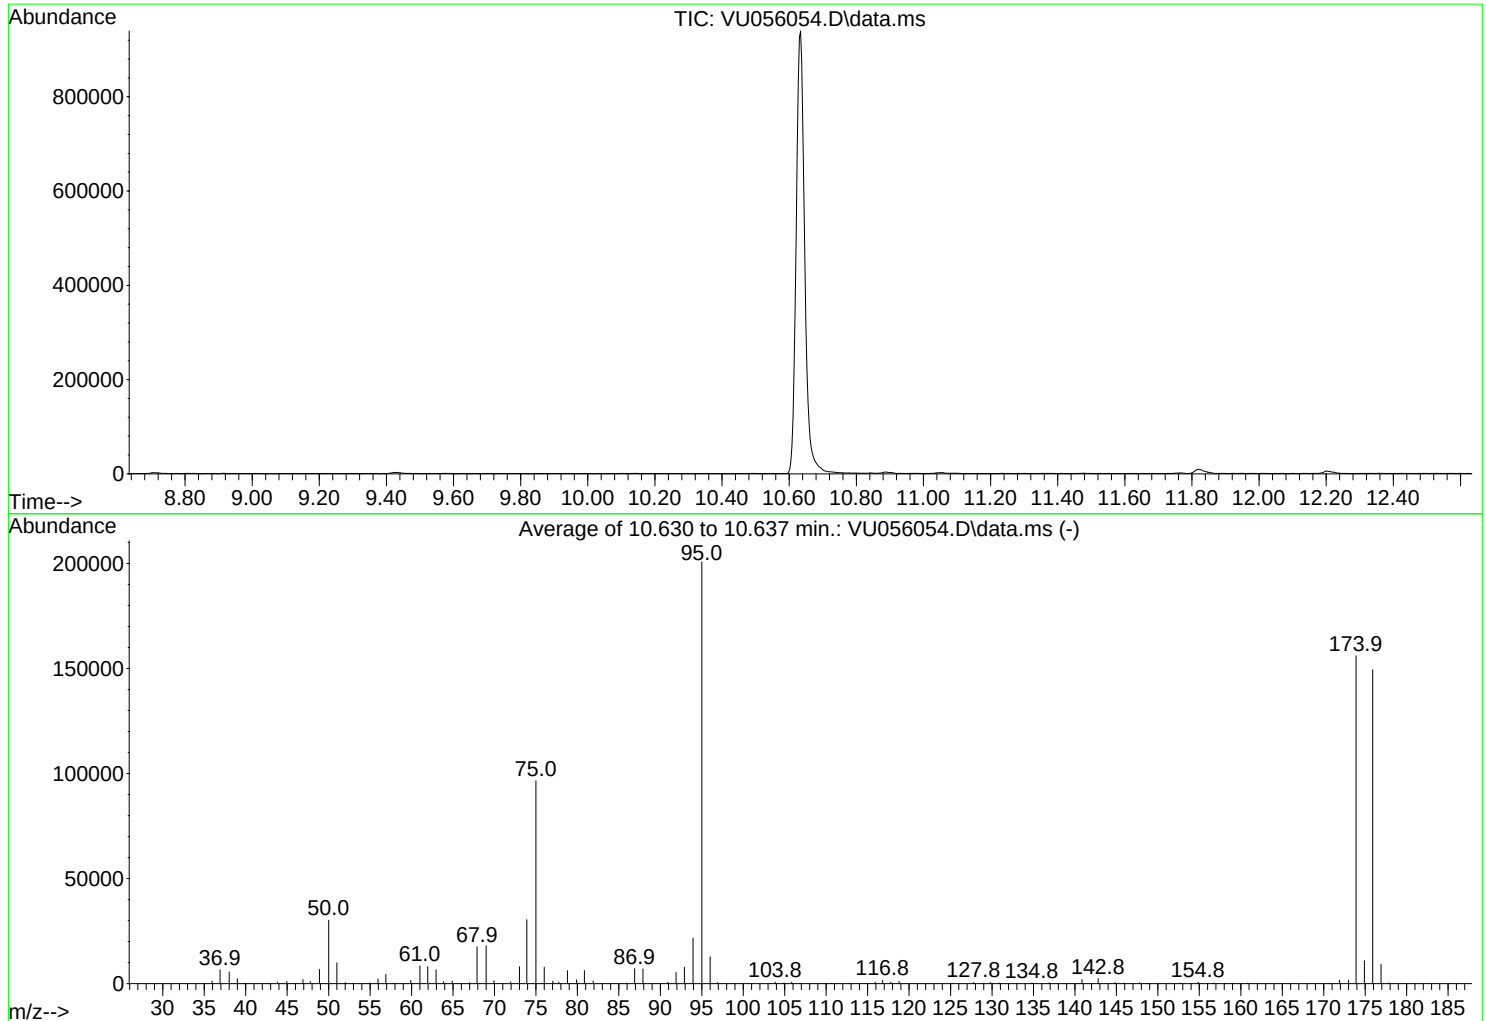

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.0	30141	PASS
75	95	30	80	48.1	96592	PASS
95	95	100	100	100.0	200768	PASS
96	95	5	9	6.4	12811	PASS
173	174	0.00	2	1.1	1657	PASS
174	95	50	120	77.7	156075	PASS
175	174	5	9	7.0	10957	PASS
176	174	95	101	95.7	149440	PASS
177	176	5	9	6.2	9330	PASS

m/z	Abundance
39.80	283.0
43.80	481.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064

m/z	Abundance
35.90	1374.0
36.90	6599.0
38.00	5287.0
39.00	2457.0
39.80	280.0
42.70	107.0
43.90	1290.0
45.00	1173.0
46.10	192.0
46.90	1814.0
47.80	977.0
48.90	7028.0
50.00	31760.0
51.00	9989.0
52.00	560.0
52.90	225.0
54.90	417.0
55.90	2294.0
56.90	4592.0
57.90	182.0
59.90	1526.0
61.00	8947.0
61.90	8250.0
62.90	6529.0
63.80	965.0
64.90	1337.0
66.00	190.0
67.00	360.0
67.90	18520.0
69.00	18688.0
70.00	1596.0
72.00	935.0
73.00	8082.0
73.90	31424.0
75.00	99024.0
76.00	8323.0
77.10	1419.0
77.80	806.0
78.80	6328.0
79.90	1874.0
80.90	6529.0
81.90	1455.0
83.00	179.0
86.90	7489.0
87.90	7436.0
90.90	739.0
91.90	5234.0
92.90	8032.0
93.90	22160.0
95.00	203264.0
96.00	13032.0
96.90	592.0
103.90	899.0
104.90	320.0
105.80	886.0
106.80	202.0
109.90	124.0
110.60	137.0
112.60	149.0
114.70	190.0
115.90	714.0
116.80	1653.0
117.80	721.0
118.80	1070.0
127.80	563.0
129.00	298.0
129.70	605.0
130.80	331.0
134.80	377.0
136.90	412.0
140.00	128.0
140.80	1869.0
142.00	121.0
142.80	2405.0
144.80	589.0
145.90	334.0
146.70	135.0
147.80	406.0
148.70	125.0
149.90	160.0
152.80	201.0
154.90	624.0
156.00	169.0
156.80	313.0
158.90	247.0
160.80	202.0
171.90	1756.0
173.00	1800.0
173.90	155456.0
174.90	10654.0
175.90	148992.0
176.90	9400.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064

177.80

418.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064

m/z	Abundance
36.00	1347.0
36.90	6717.0
38.00	5744.0
39.00	2460.0
39.80	302.0
43.90	1278.0
44.90	1046.0
46.10	186.0
46.90	1958.0
47.80	1006.0
48.90	7069.0
50.00	30760.0
51.00	10172.0
52.00	575.0
53.00	209.0
55.00	336.0
56.00	2319.0
56.90	4595.0
57.90	211.0
59.90	1615.0
61.00	8669.0
61.90	8331.0
62.90	6596.0
63.80	910.0
64.90	1275.0
66.00	158.0
67.00	481.0
67.90	17984.0
69.00	18584.0
69.90	1473.0
72.00	889.0
73.00	8369.0
73.90	31168.0
75.00	99568.0
76.00	7955.0
77.00	1246.0
77.70	822.0
78.80	6448.0
79.90	1900.0
80.90	6461.0
81.90	1329.0
82.90	136.0
85.90	302.0
86.90	7267.0
87.90	7136.0
90.90	729.0
91.90	5549.0
92.90	7909.0
93.90	22296.0
95.00	206336.0
96.00	13174.0
96.90	522.0
103.90	828.0
104.90	327.0
105.90	738.0
106.80	234.0
109.90	145.0
110.60	185.0
112.70	175.0
114.70	194.0
115.90	736.0
116.80	1642.0
117.80	777.0
118.80	1089.0
127.80	679.0
129.00	277.0
129.80	646.0
130.80	343.0
134.80	345.0
136.90	415.0
140.00	172.0
140.90	1971.0
142.00	177.0
142.80	2393.0
144.90	538.0
145.90	364.0
146.70	147.0
147.80	430.0
150.00	183.0
152.70	241.0
153.90	116.0
154.90	691.0
156.00	163.0
156.70	322.0
158.00	105.0
159.00	252.0
160.80	193.0
171.90	1729.0
173.00	1671.0
173.90	160832.0
174.90	11326.0
175.90	153728.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064

176.909585.0

177.80396.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064

m/z	Abundance
36.00	1099.0
36.90	6371.0
38.00	5685.0
39.00	2296.0
39.80	344.0
43.90	1152.0
44.90	1015.0
45.90	177.0
46.90	1935.0
47.80	959.0
48.90	6259.0
50.00	27904.0
51.00	9502.0
52.00	493.0
52.80	174.0
53.00	170.0
55.00	282.0
56.00	2223.0
56.90	4199.0
57.80	216.0
59.90	1662.0
61.00	7751.0
62.00	7764.0
63.00	6466.0
63.90	847.0
64.90	1212.0
66.00	122.0
67.00	535.0
67.90	16305.0
69.00	16960.0
69.90	1342.0
71.90	795.0
73.00	7682.0
73.90	28704.0
75.00	91184.0
76.00	7319.0
77.00	1058.0
77.80	785.0
78.80	5744.0
79.90	1750.0
80.80	5711.0
81.90	1131.0
85.90	368.0
86.90	6708.0
87.90	6210.0
90.90	594.0
91.90	5335.0
92.90	7529.0
94.00	20776.0
95.00	192704.0
96.00	12228.0
97.00	353.0
103.80	676.0
104.90	279.0
105.90	618.0
106.90	182.0
109.90	110.0
110.70	195.0
112.80	228.0
114.70	201.0
115.90	659.0
116.80	1460.0
117.80	832.0
118.80	1057.0
127.80	701.0
128.70	221.0
129.90	645.0
130.90	307.0
134.80	262.0
136.90	409.0
139.90	148.0
140.90	2035.0
142.00	245.0
142.80	2309.0
144.90	526.0
145.90	356.0
146.70	140.0
147.80	447.0
149.90	198.0
152.70	213.0
153.90	126.0
154.80	654.0
156.70	253.0
159.00	243.0
160.80	209.0
170.70	105.0
171.90	1575.0
173.00	1501.0
173.90	151936.0
174.90	10892.0
175.90	145600.0
176.90	9005.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064

177.90

342.0

Instrument :
MSVOA_U
ClientSampleId :
BFB064