


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU110320\
 Data File : VU041064.D
 Acq On : 03 Nov 2020 08:55
 Operator : SY/MD
 Sample : BFB04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB04

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Nov 04 00:51:13 2020

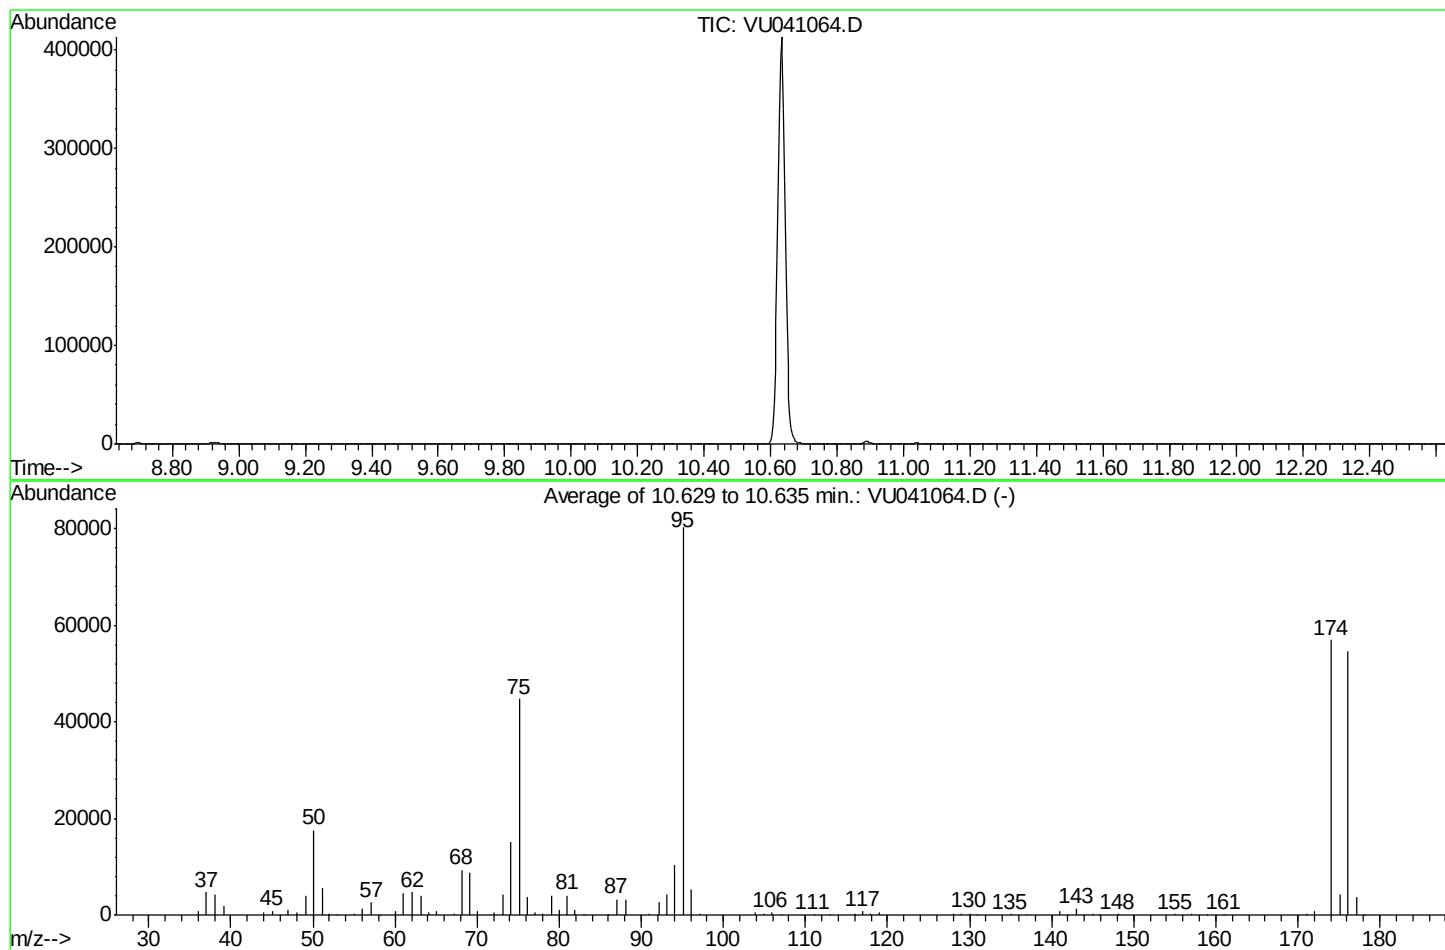

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	17568	PASS
75	95	30	80	55.7	44666	PASS
95	95	100	100	100.0	80240	PASS
96	95	5	9	6.8	5432	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.0	56952	PASS
175	174	5	9	7.7	4372	PASS
176	174	95	101	96.0	54658	PASS
177	176	5	9	6.7	3648	PASS

m/z	Abundance
36.10	852.0
37.00	4657.0
38.10	4285.0
39.10	1778.0
44.00	640.0
45.00	834.0
46.00	168.0
47.00	1045.0
48.00	592.0
49.10	3980.0
50.10	17392.0
51.10	5563.0
52.00	257.0
52.90	122.0
55.00	252.0
56.10	1377.0
57.10	2653.0
60.00	880.0
61.10	4616.0
62.10	4652.0
63.10	3887.0
64.10	661.0
65.00	675.0
67.10	235.0
68.10	9260.0
69.10	8774.0
70.10	697.0
72.00	691.0
73.10	4039.0
74.10	15226.0
75.10	44296.0
76.10	3829.0
77.00	489.0
78.10	369.0
79.00	4130.0
80.00	955.0
81.00	4013.0
82.00	1003.0
87.00	3291.0
88.00	3115.0
91.00	373.0
92.10	2539.0
93.10	3892.0
94.10	10005.0
95.10	79104.0
96.10	5475.0
97.10	159.0
103.90	455.0
104.90	133.0
105.90	506.0
111.00	136.0
116.00	348.0
117.00	646.0
117.90	304.0
119.00	575.0
128.00	288.0
129.10	185.0
130.00	316.0
130.90	101.0
135.00	147.0
136.90	122.0
141.00	819.0
142.00	112.0
143.10	1299.0
145.00	336.0
145.90	116.0
148.10	204.0
155.10	220.0
157.10	185.0
159.00	110.0
171.00	187.0
172.10	724.0
174.10	54408.0
175.10	4321.0
176.10	51968.0
177.10	3504.0
178.10	119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

m/z	Abundance
36.00	830.0
37.00	4839.0
38.00	4399.0
39.10	1834.0
44.00	698.0
45.00	920.0
46.00	142.0
47.00	986.0
48.00	593.0
49.10	4114.0
50.10	18128.0
51.10	5731.0
52.00	287.0
52.90	115.0
55.00	259.0
56.00	1449.0
57.10	2713.0
60.00	886.0
61.00	4739.0
62.10	4860.0
63.10	4179.0
64.10	638.0
65.10	701.0
67.10	241.0
68.10	9741.0
69.10	9148.0
70.10	746.0
72.00	678.0
73.10	4264.0
74.10	15749.0
75.10	46240.0
76.10	3902.0
77.00	573.0
78.00	363.0
79.00	4240.0
80.00	1075.0
81.00	4174.0
82.00	1012.0
87.00	3447.0
88.10	3463.0
91.00	419.0
92.10	2725.0
93.10	4339.0
94.10	10656.0
95.10	82768.0
96.10	5691.0
97.10	177.0
103.90	474.0
104.90	181.0
105.90	513.0
107.00	101.0
111.00	144.0
116.00	373.0
117.00	707.0
117.90	321.0
119.00	615.0
128.00	280.0
129.00	168.0
130.00	304.0
130.90	118.0
135.00	160.0
136.90	133.0
141.00	876.0
142.00	124.0
143.00	1352.0
144.00	102.0
145.00	340.0
145.90	135.0
148.10	236.0
155.10	233.0
157.10	194.0
159.00	110.0
161.00	115.0
171.00	175.0
172.10	847.0
174.10	58784.0
175.10	4491.0
176.10	56568.0
177.10	3788.0
178.10	147.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

m/z	Abundance
36.00	761.0
37.00	4582.0
38.10	4150.0
39.10	1690.0
44.00	713.0
45.00	832.0
46.00	106.0
47.00	952.0
48.00	545.0
49.10	3843.0
50.10	17184.0
51.10	5372.0
52.00	275.0
55.00	248.0
56.00	1433.0
57.10	2466.0
58.10	110.0
60.00	818.0
61.00	4420.0
62.10	4537.0
63.10	3925.0
64.10	563.0
65.10	675.0
67.20	218.0
68.10	9032.0
69.10	8668.0
70.10	695.0
72.10	568.0
73.10	4157.0
74.10	14748.0
75.10	43464.0
76.10	3582.0
77.00	605.0
78.00	317.0
79.00	3831.0
80.00	1124.0
81.00	3924.0
81.90	942.0
83.00	103.0
86.00	118.0
87.00	3162.0
88.10	3280.0
91.00	416.0
92.10	2515.0
93.10	4217.0
94.10	10355.0
95.10	78848.0
96.10	5131.0
97.10	150.0
103.90	453.0
104.90	175.0
105.90	415.0
111.00	124.0
112.90	119.0
116.00	368.0
117.00	692.0
117.90	334.0
119.00	570.0
128.00	245.0
129.00	152.0
130.00	281.0
130.90	150.0
135.00	163.0
137.00	124.0
141.00	849.0
142.00	127.0
143.00	1266.0
145.00	346.0
145.90	124.0
148.10	219.0
155.00	244.0
157.10	159.0
161.00	121.0
171.10	131.0
172.10	858.0
174.10	57664.0
175.10	4305.0
176.10	55440.0
177.10	3653.0
178.10	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

m/z	Abundance
44.00	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04