

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110323\
 Data File : VU056077.D
 Acq On : 03 Nov 2023 13:21
 Operator : MD/SY
 Sample : 05174-26
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AN9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056077.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	107	rBV	128625	153129	14.12%	1.654%
2	1.914	186	194	213	rVB	107070	146527	13.51%	1.583%
3	2.567	384	397	415	rBV	226289	373484	34.43%	4.034%
4	3.049	534	547	560	rVB3	14357	27126	2.50%	0.293%
5	4.640	1026	1042	1090	rBV	110992	398372	36.72%	4.303%
6	5.062	1157	1173	1195	rBV2	217498	558367	51.47%	6.031%
7	5.724	1359	1379	1401	rBV2	413468	1084827	100.00%	11.717%
8	6.248	1527	1542	1565	rBV	392449	788335	72.67%	8.515%
9	6.689	1663	1679	1703	rBV	250230	507806	46.81%	5.485%
10	7.563	1937	1951	1979	rBV	122171	229718	21.18%	2.481%
11	7.894	2039	2054	2081	rBV	473032	894991	82.50%	9.667%
12	8.177	2130	2142	2163	rBV2	71189	131245	12.10%	1.418%
13	8.470	2220	2233	2245	rBV3	7480	14517	1.34%	0.157%
14	8.634	2272	2284	2326	rBV2	462420	1069171	98.56%	11.548%
15	9.415	2514	2527	2565	rBV	539875	971344	89.54%	10.491%
16	10.753	2931	2943	2960	rBV	185806	298647	27.53%	3.226%
17	10.888	2974	2985	2998	rVB	21782	36475	3.36%	0.394%
18	11.811	3259	3272	3290	rBV	501730	849178	78.28%	9.172%
19	12.190	3376	3390	3415	rBV	426361	725421	66.87%	7.835%




Sum of corrected areas: 9258680

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110323\
Data File : VU056077.D
Acq On : 03 Nov 2023 13:21
Operator : MD/SY
Sample : 05174-26
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

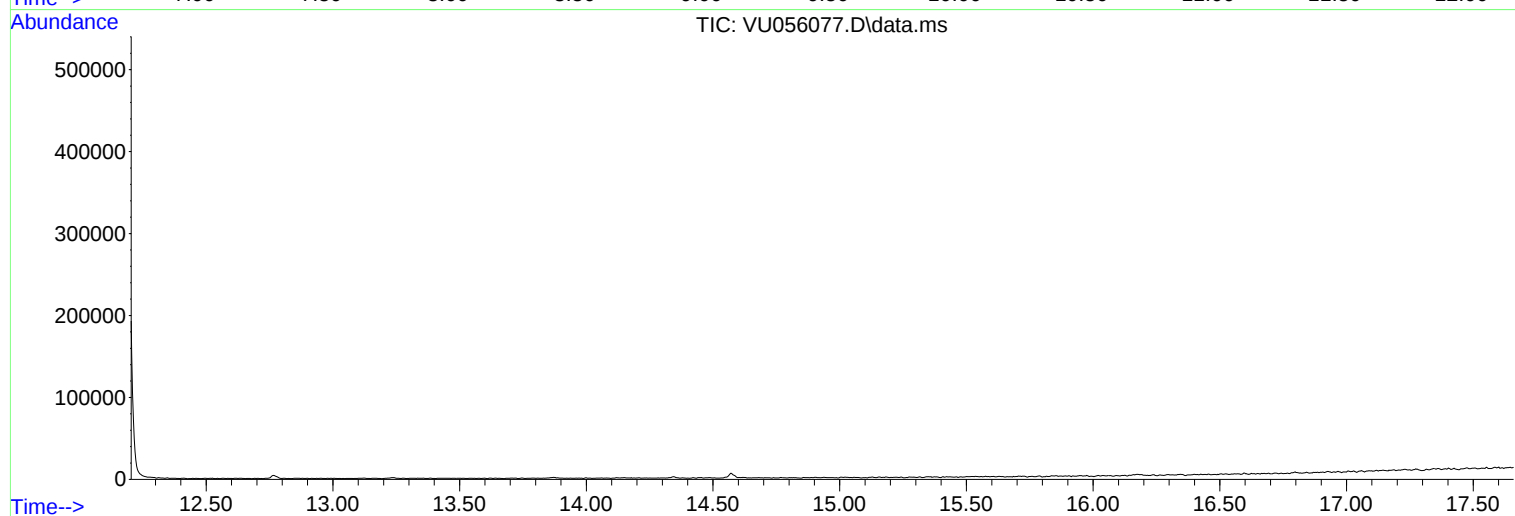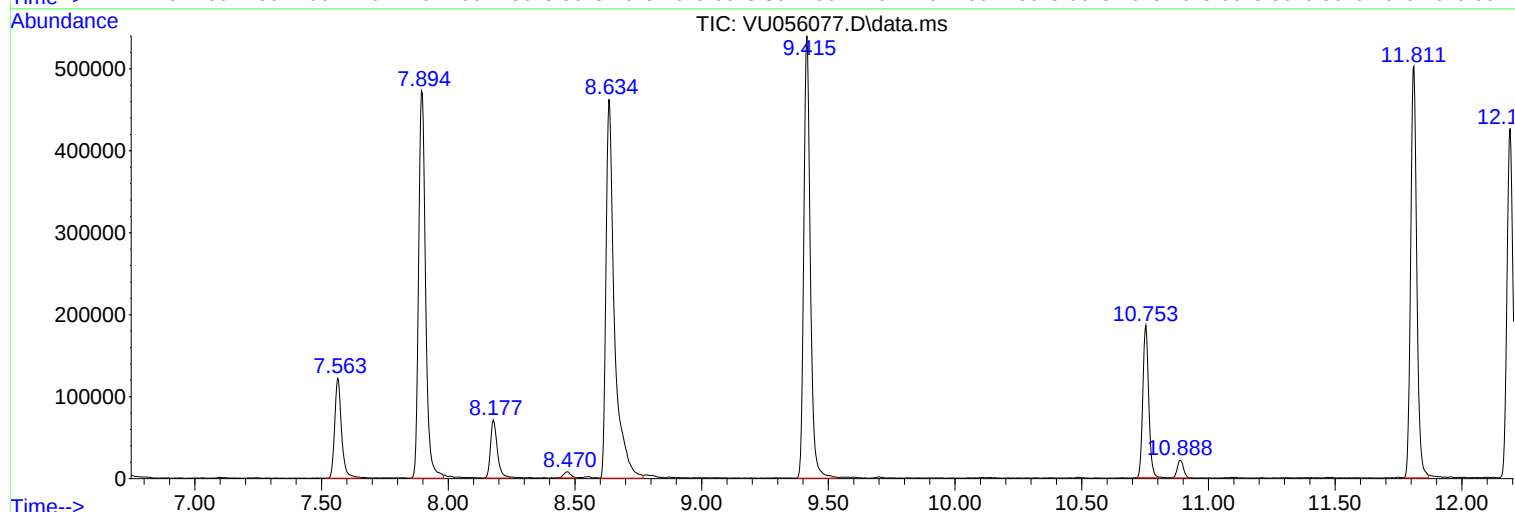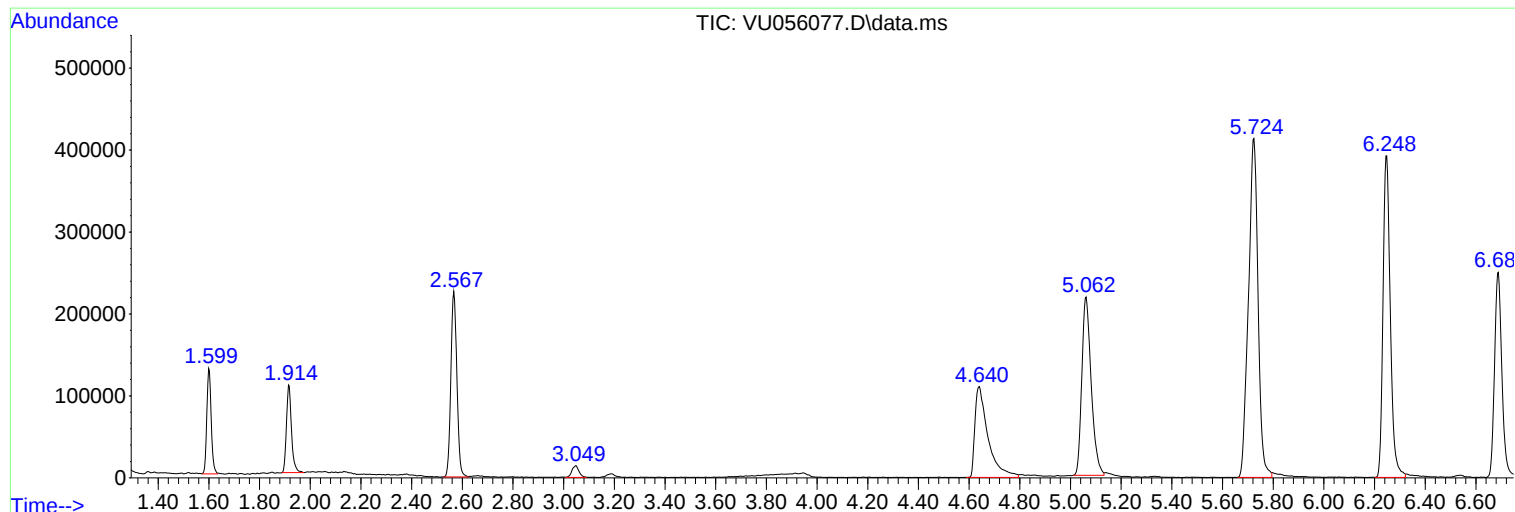

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110323\
Data File : VU056077.D
Acq On : 03 Nov 2023 13:21
Operator : MD/SY
Sample : 05174-26
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110323\
Data File : VU056077.D
Acq On : 03 Nov 2023 13:21
Operator : MD/SY
Sample : 05174-26
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AN9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------