

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110323\
 Data File : VU056078.D
 Acq On : 03 Nov 2023 13:45
 Operator : MD/SY
 Sample : 05174-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056078.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	87	96	109	rBV	139317	161090	13.97%	1.690%
2	1.914	186	194	211	rBV	111343	156002	13.53%	1.637%
3	2.567	384	397	418	rBV	240467	399298	34.62%	4.190%
4	3.046	534	546	563	rBV2	20828	40936	3.55%	0.430%
5	4.640	1027	1042	1085	rBV2	113314	419374	36.36%	4.401%
6	5.058	1157	1172	1196	rBV	222567	514532	44.61%	5.399%
7	5.721	1357	1378	1408	rBV2	438371	1153428	100.00%	12.103%
8	6.245	1528	1541	1568	rBV	388197	777681	67.42%	8.160%
9	6.685	1665	1678	1699	rBV	266893	533781	46.28%	5.601%
10	7.563	1937	1951	1977	rBV	130724	244113	21.16%	2.562%
11	7.894	2039	2054	2088	rBV	502019	943566	81.81%	9.901%
12	8.177	2130	2142	2161	rBV2	75374	137430	11.91%	1.442%
13	8.470	2221	2233	2244	rBV2	17670	33559	2.91%	0.352%
14	8.634	2272	2284	2321	rBV2	493529	1132538	98.19%	11.884%
15	9.415	2514	2527	2551	rBV	538758	949405	82.31%	9.962%
16	10.753	2929	2943	2965	rBV2	190601	317144	27.50%	3.328%
17	10.891	2972	2986	3000	rBV2	35769	60393	5.24%	0.634%
18	11.807	3259	3271	3295	rBV	476745	805439	69.83%	8.452%
19	12.190	3377	3390	3416	rBV	428857	738487	64.03%	7.749%
20	12.769	3559	3570	3584	rVB2	7400	11652	1.01%	0.122%




Sum of corrected areas: 9529848

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110323\
Data File : VU056078.D
Acq On : 03 Nov 2023 13:45
Operator : MD/SY
Sample : 05174-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

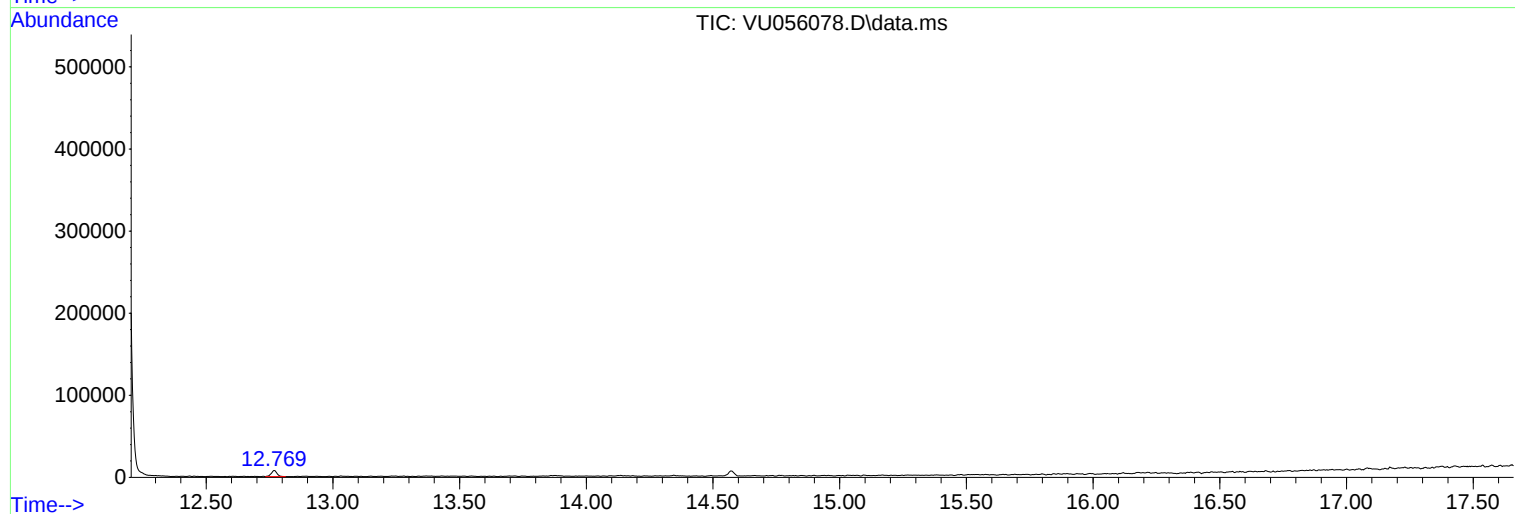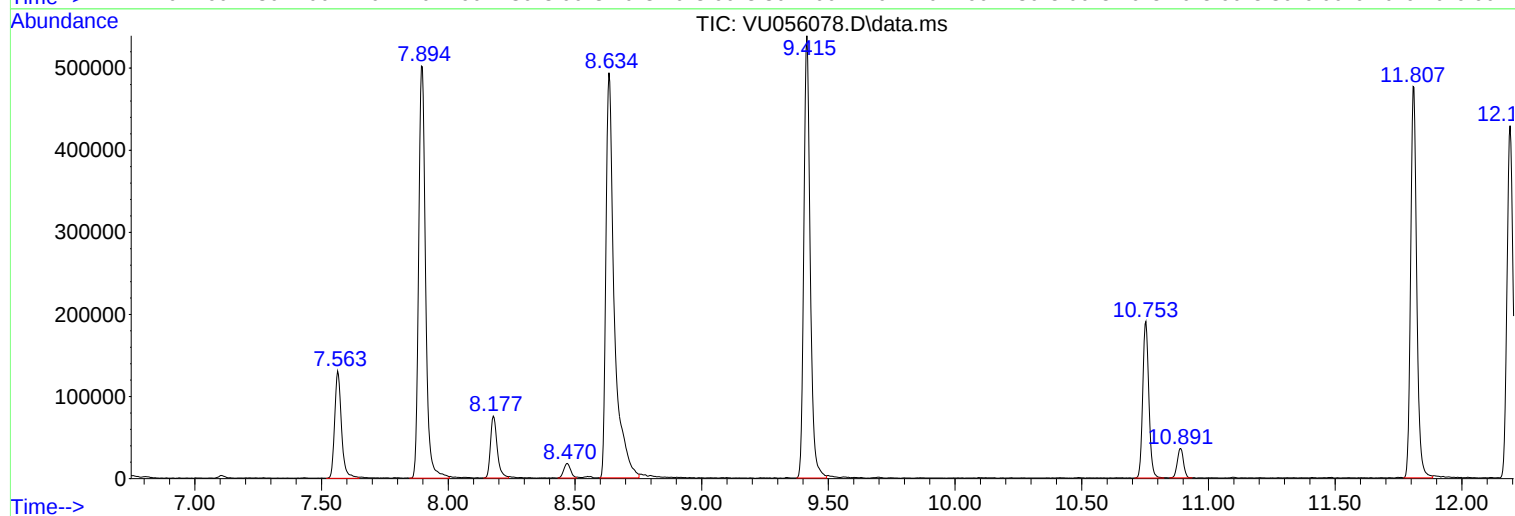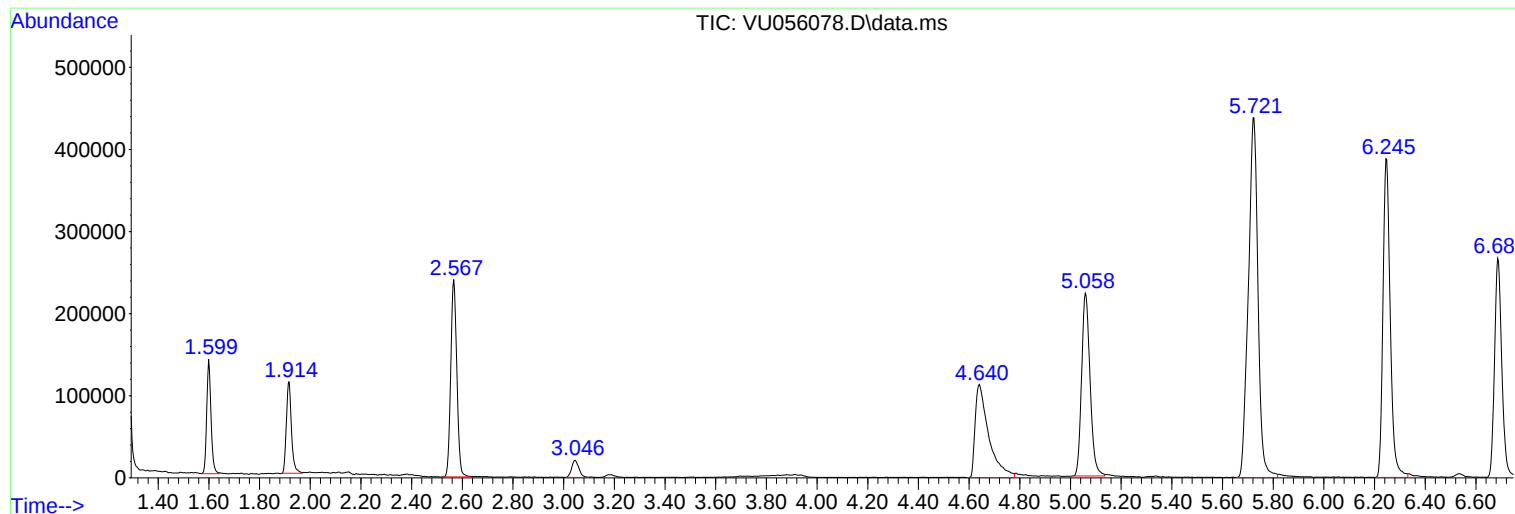

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110323\
Data File : VU056078.D
Acq On : 03 Nov 2023 13:45
Operator : MD/SY
Sample : 05174-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110323\
Data File : VU056078.D
Acq On : 03 Nov 2023 13:45
Operator : MD/SY
Sample : 05174-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc