


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110323\
Data File : VU056073.D
Acq On : 03 Nov 2023 09:05
Operator : MD/SY
Sample : BFB065
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB065

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Nov 04 01:40:01 2023

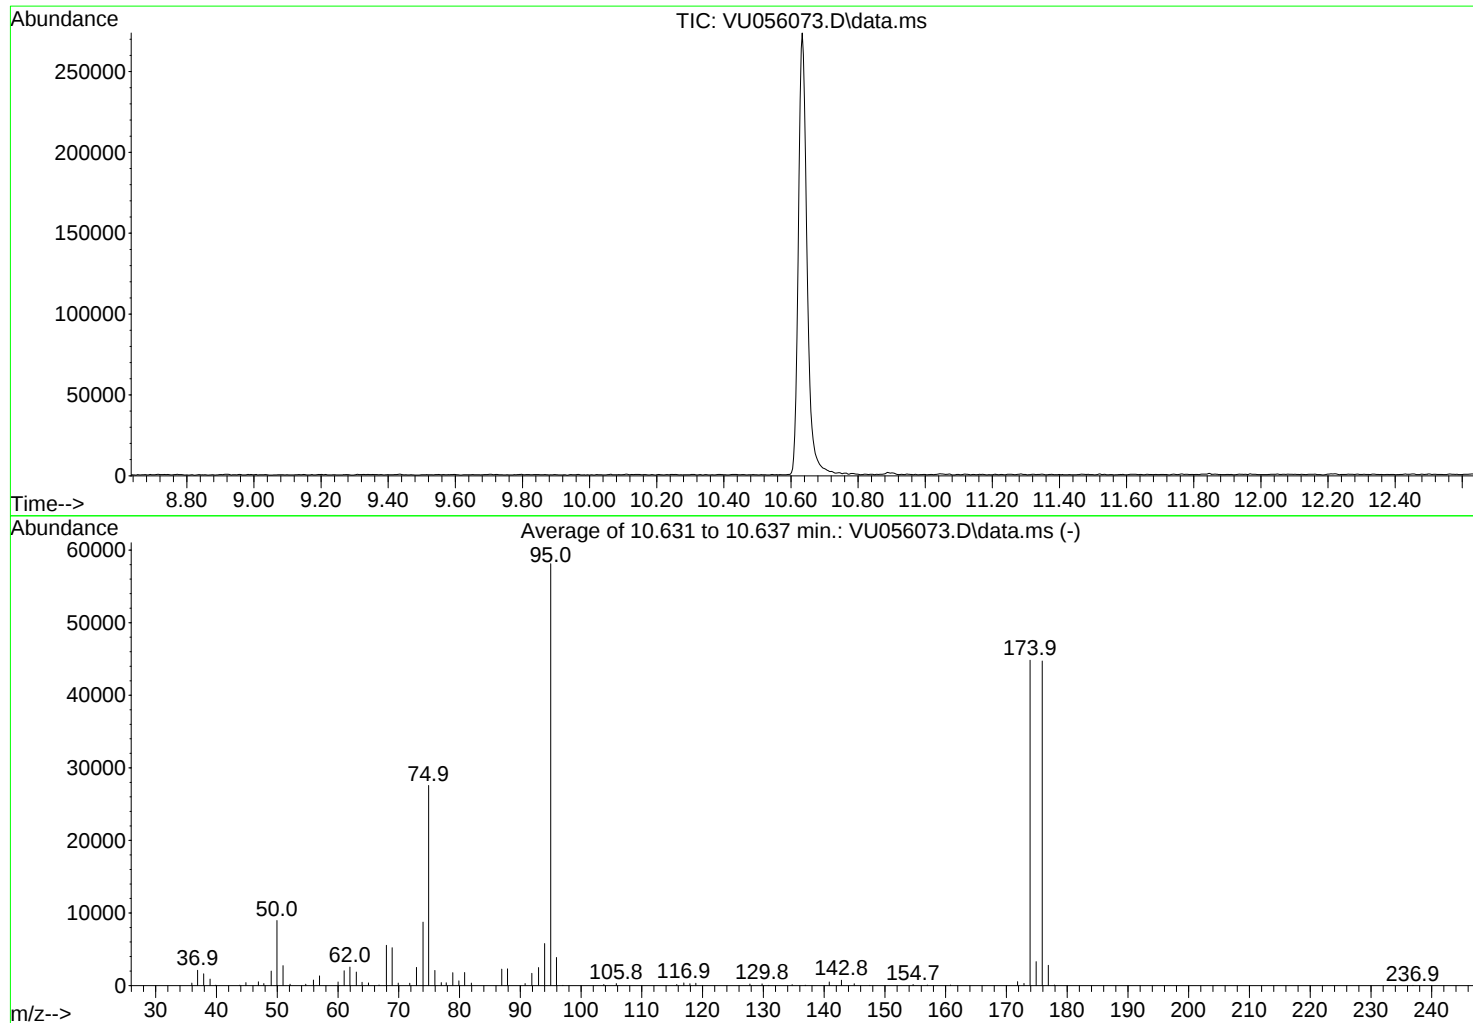

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2892

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	8973	PASS
75	95	30	80	47.4	27571	PASS
95	95	100	100	100.0	58120	PASS
96	95	5	9	6.7	3881	PASS
173	174	0.00	2	0.7	308	PASS
174	95	50	120	77.1	44829	PASS
175	174	5	9	7.4	3302	PASS
176	174	95	101	99.8	44723	PASS
177	176	5	9	6.2	2793	PASS

Scan 2892 (10.589 min): VU056073.D\data.ms
BFB065

m/z	Abundance
40.00	265.0
43.80	477.0

Instrument :
MSVOA_U
ClientSampleId :
BFB065

m/z	Abundance
35.90	344.0
36.90	2260.0
37.90	1766.0
38.90	961.0
39.90	317.0
43.90	519.0
44.90	395.0
46.90	453.0
47.80	240.0
49.00	2024.0
49.90	9014.0
51.00	3006.0
52.10	263.0
54.70	188.0
56.00	654.0
56.90	1520.0
60.00	485.0
61.00	2273.0
62.00	2597.0
63.00	1753.0
64.00	433.0
65.00	396.0
67.90	5613.0
68.90	5295.0
70.00	344.0
71.80	329.0
72.90	2242.0
74.00	8522.0
74.90	27504.0
76.00	2299.0
77.00	393.0
77.80	360.0
78.90	1813.0
79.90	614.0
80.90	1734.0
81.90	351.0
86.90	2298.0
87.90	2455.0
90.80	282.0
91.90	1617.0
93.00	2368.0
94.00	5935.0
95.00	58056.0
96.00	3828.0
97.00	126.0
103.80	149.0
105.80	215.0
115.70	170.0
116.90	353.0
117.90	283.0
118.90	358.0
127.80	215.0
129.70	224.0
134.80	126.0
140.80	610.0
142.80	694.0
145.00	247.0
154.80	158.0
157.00	114.0
171.80	471.0
172.90	467.0
173.90	43448.0
174.90	3427.0
175.90	43392.0
176.90	2787.0

Instrument :
MSVOA_U
ClientSampleId :
BFB065

m/z	Abundance
36.00	377.0
36.90	2135.0
37.90	1561.0
38.90	930.0
39.90	326.0
43.90	532.0
44.90	407.0
46.90	548.0
47.80	279.0
49.00	2063.0
50.00	9319.0
50.90	2807.0
52.10	201.0
54.70	189.0
55.90	761.0
56.90	1311.0
60.00	550.0
61.00	2037.0
61.90	2539.0
63.00	1919.0
64.00	467.0
65.00	370.0
66.70	118.0
67.90	5677.0
68.90	5428.0
69.80	350.0
71.80	358.0
72.90	2562.0
74.00	8951.0
74.90	28536.0
75.90	2063.0
77.00	430.0
77.80	418.0
78.90	1858.0
79.90	666.0
80.80	1845.0
81.90	366.0
86.90	2298.0
87.90	2358.0
90.80	321.0
91.90	1685.0
93.00	2521.0
94.00	5872.0
95.00	59632.0
95.90	3971.0
103.70	145.0
105.80	292.0
115.80	160.0
116.90	367.0
117.90	277.0
118.90	330.0
127.80	224.0
129.80	226.0
134.80	147.0
140.80	509.0
142.80	744.0
144.90	284.0
154.60	137.0
157.00	115.0
160.80	103.0
171.90	564.0
172.90	456.0
173.90	46240.0
174.90	3406.0
175.90	46240.0
176.90	2851.0
177.90	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB065

m/z	Abundance
36.00	326.0
36.90	1933.0
37.90	1529.0
39.00	769.0
39.90	292.0
44.00	553.0
44.80	436.0
46.90	574.0
47.80	307.0
49.00	1876.0
50.00	8585.0
50.90	2430.0
52.10	103.0
54.70	156.0
55.90	861.0
57.00	1160.0
60.00	456.0
61.00	1840.0
61.90	2515.0
63.00	1894.0
63.90	447.0
65.00	347.0
66.80	132.0
68.00	5325.0
68.90	4930.0
69.90	356.0
71.80	303.0
72.90	2678.0
74.00	8724.0
74.90	26672.0
75.90	1884.0
77.00	382.0
77.80	389.0
78.90	1658.0
79.90	687.0
80.80	1800.0
82.00	323.0
87.00	2162.0
87.90	2120.0
90.80	252.0
91.90	1770.0
93.00	2556.0
94.00	5566.0
95.00	56672.0
95.90	3844.0
103.70	157.0
105.80	298.0
115.80	129.0
116.90	351.0
117.90	211.0
118.90	270.0
127.80	191.0
129.90	235.0
130.90	126.0
134.70	100.0
136.90	143.0
140.90	401.0
142.90	800.0
144.90	254.0
147.50	122.0
154.60	132.0
160.80	115.0
171.80	585.0
173.90	44800.0
174.90	3073.0
175.90	44536.0
176.90	2740.0
177.90	122.0
236.90	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB065