


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110419\
 Data File : VU035598.D
 Acq On : 04 Nov 2019 08:37
 Operator : JC/SP
 Sample : BFB29
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB29

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR110419WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Nov 05 02:35:58 2019

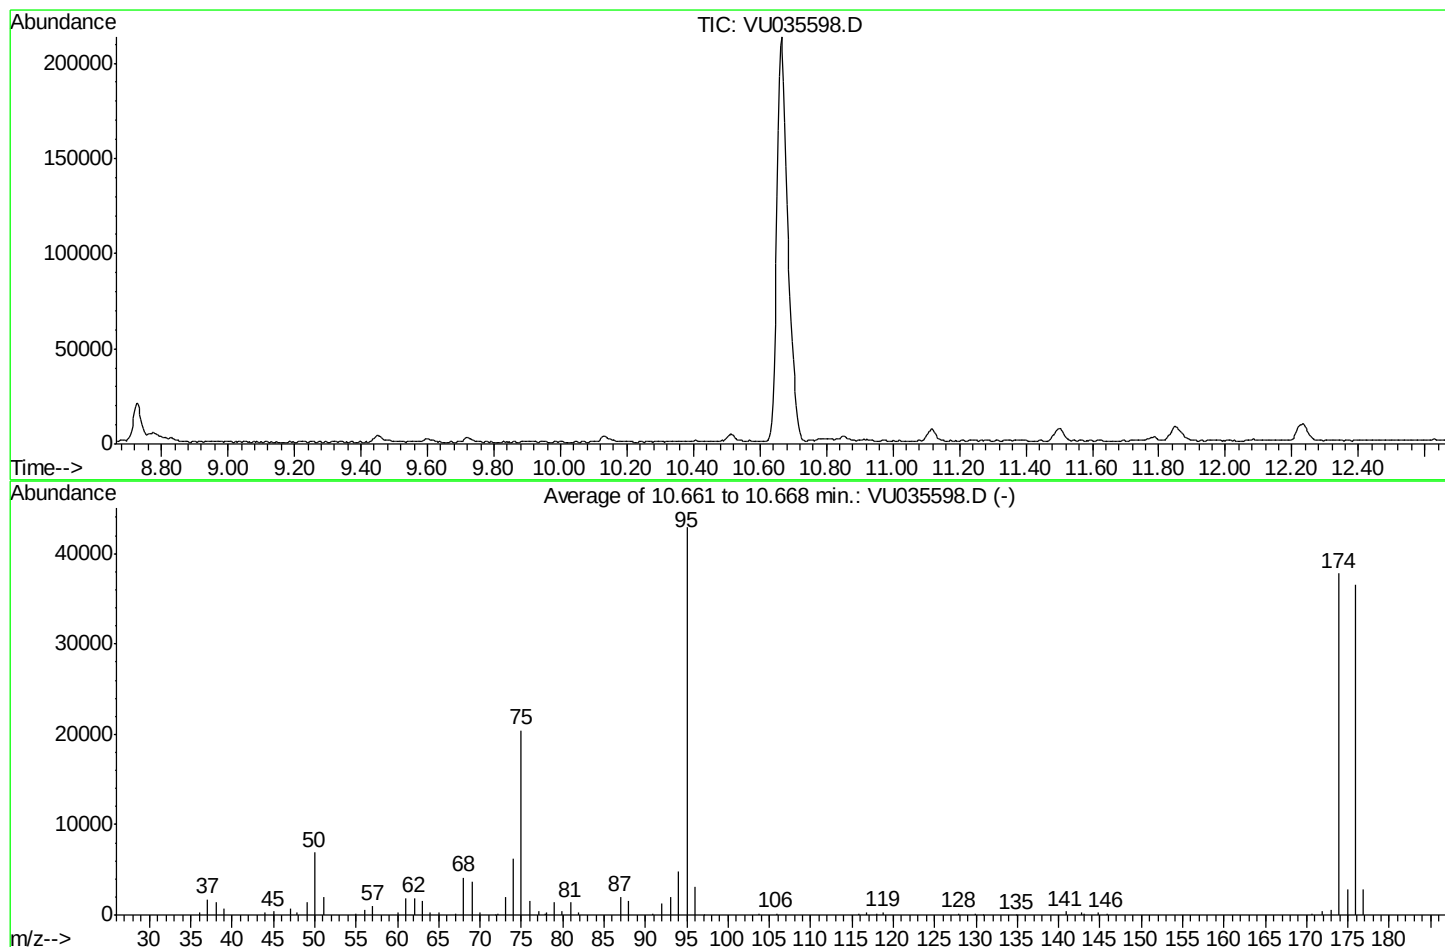

AutoFind: Scans 2899, 2900, 2901; Background Corrected with Scan 2885

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	6902	PASS
75	95	30	80	47.7	20458	PASS
95	95	100	100	100.0	42906	PASS
96	95	5	9	7.2	3076	PASS
173	174	0.00	2	1.4	532	PASS
174	95	50	120	88.1	37792	PASS
175	174	5	9	7.6	2860	PASS
176	174	95	101	96.7	36536	PASS
177	176	5	9	7.6	2776	PASS

m/z	Abundance
36.00	516.0
37.00	1801.0
38.00	1445.0
39.00	660.0
39.90	158.0
44.00	1149.0
45.00	384.0
47.00	642.0
47.90	276.0
49.00	1414.0
50.00	6948.0
51.10	2060.0
55.00	173.0
56.00	582.0
57.00	1010.0
60.10	296.0
61.00	1811.0
62.10	1959.0
63.00	1508.0
63.90	281.0
65.00	339.0
67.00	130.0
68.00	4237.0
69.00	3658.0
70.00	301.0
72.10	218.0
73.10	1966.0
74.10	6358.0
75.00	20960.0
76.00	1617.0
77.10	402.0
77.80	239.0
78.10	271.0
78.90	1421.0
79.80	428.0
80.90	1392.0
81.90	309.0
87.00	2103.0
88.00	1560.0
91.00	208.0
92.00	1235.0
93.00	2009.0
94.00	4963.0
95.00	43664.0
96.00	3237.0
103.80	195.0
105.90	202.0
115.80	108.0
116.80	274.0
118.00	167.0
118.80	330.0
127.90	204.0
129.90	119.0
130.90	103.0
140.90	386.0
142.80	444.0
144.80	261.0
145.90	155.0
170.70	109.0
172.00	542.0
173.00	522.0
173.90	38272.0
174.90	2935.0
175.90	37232.0
176.90	2898.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

m/z	Abundance
36.00	563.0
37.00	1765.0
38.00	1433.0
39.10	660.0
40.00	193.0
44.00	1135.0
45.00	397.0
47.00	661.0
47.90	285.0
49.00	1452.0
50.00	6949.0
51.10	1972.0
55.00	170.0
56.00	603.0
57.00	1010.0
60.10	350.0
61.00	1828.0
62.10	1837.0
63.00	1361.0
64.00	301.0
65.10	272.0
67.00	136.0
68.00	4077.0
69.00	3637.0
70.00	371.0
71.90	187.0
73.10	2065.0
74.10	6476.0
75.00	20552.0
76.00	1636.0
77.10	408.0
78.10	323.0
78.90	1315.0
79.90	365.0
80.90	1320.0
81.90	366.0
87.00	1946.0
88.00	1564.0
90.90	179.0
92.00	1310.0
93.00	1943.0
94.00	4742.0
95.00	43344.0
96.00	3137.0
97.00	138.0
103.80	159.0
105.80	208.0
116.80	324.0
117.90	182.0
118.80	308.0
127.90	134.0
129.90	129.0
134.90	115.0
140.90	389.0
142.80	500.0
144.80	250.0
145.90	124.0
170.60	103.0
172.00	430.0
173.00	537.0
173.90	37232.0
174.90	2771.0
175.90	35784.0
176.90	2835.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

Scan 2885 (10.616 min): VU035598.D
BFB29

m/z	Abundance
36.00	264.0
39.90	217.0
44.00	873.0
207.10	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

m/z	Abundance
36.00	491.0
37.00	1631.0
38.00	1494.0
39.00	672.0
39.90	165.0
44.00	1069.0
45.00	337.0
47.00	628.0
47.80	254.0
49.00	1354.0
50.00	6809.0
51.10	2034.0
55.00	194.0
56.00	549.0
57.00	1032.0
59.90	313.0
60.90	1769.0
62.00	1885.0
63.00	1654.0
63.90	214.0
65.00	360.0
68.00	4099.0
69.00	3705.0
70.10	239.0
72.10	223.0
73.10	1724.0
74.00	6052.0
75.00	19864.0
76.00	1547.0
77.10	319.0
78.00	242.0
78.90	1371.0
79.80	443.0
80.90	1450.0
81.80	282.0
87.00	2104.0
87.90	1494.0
91.00	237.0
92.00	1107.0
93.00	1936.0
94.00	4739.0
95.00	41712.0
96.00	2856.0
103.80	237.0
105.90	204.0
115.80	139.0
116.70	225.0
118.00	138.0
118.80	284.0
127.90	205.0
130.00	109.0
130.80	107.0
140.90	386.0
143.00	414.0
144.90	277.0
145.80	168.0
170.80	115.0
171.90	533.0
173.00	538.0
174.00	37872.0
174.90	2876.0
175.90	36592.0
176.90	2595.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29