

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU110420\
 Data File : VU041094.D
 Acq On : 04 Nov 2020 11:31
 Operator : SY/MD
 Sample : L4575-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AA2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	75	82	101	rVB	24034	26986	5.21%	1.088%
2	1.925	173	182	192	rVB	19013	23761	4.59%	0.958%
3	2.093	224	234	242	rBV	15641	21198	4.09%	0.855%
4	2.151	242	252	265	rVB	122269	178137	34.38%	7.183%
5	2.578	375	385	403	rBV	35190	58387	11.27%	2.354%
6	3.597	692	702	716	rBV2	2887	6355	1.23%	0.256%
7	4.655	1014	1031	1070	rBV2	41234	144092	27.81%	5.810%
8	5.080	1149	1163	1181	rBB2	36150	80238	15.49%	3.235%
9	5.739	1348	1368	1384	rBV2	68128	181983	35.12%	7.338%
10	6.260	1517	1530	1550	rBV	74706	135289	26.11%	5.455%
11	6.552	1612	1621	1631	rBB5	7912	14239	2.75%	0.574%
12	6.700	1653	1667	1682	rBV2	45588	87925	16.97%	3.545%
13	7.572	1928	1938	1951	rBB	21508	37076	7.16%	1.495%
14	7.906	2027	2042	2061	rBV	69218	120762	23.31%	4.869%
15	8.186	2118	2129	2141	rBV2	14987	25144	4.85%	1.014%
16	8.555	2231	2244	2258	rVV	308473	518114	100.00%	20.892%
17	8.639	2258	2270	2308	rVB	167142	298359	57.59%	12.031%
18	9.417	2501	2512	2531	rBV	108567	179649	34.67%	7.244%
19	10.755	2918	2928	2945	rVB	40092	64558	12.46%	2.603%
20	10.890	2962	2970	2979	rBV2	3703	5605	1.08%	0.226%
21	11.806	3238	3255	3270	rBV	96419	152883	29.51%	6.165%
22	12.185	3362	3373	3390	rVB	74692	119261	23.02%	4.809%


Sum of corrected areas: 2480001

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU110420\
Data File : VU041094.D
Acq On : 04 Nov 2020 11:31
Operator : SY/MD
Sample : L4575-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AA2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

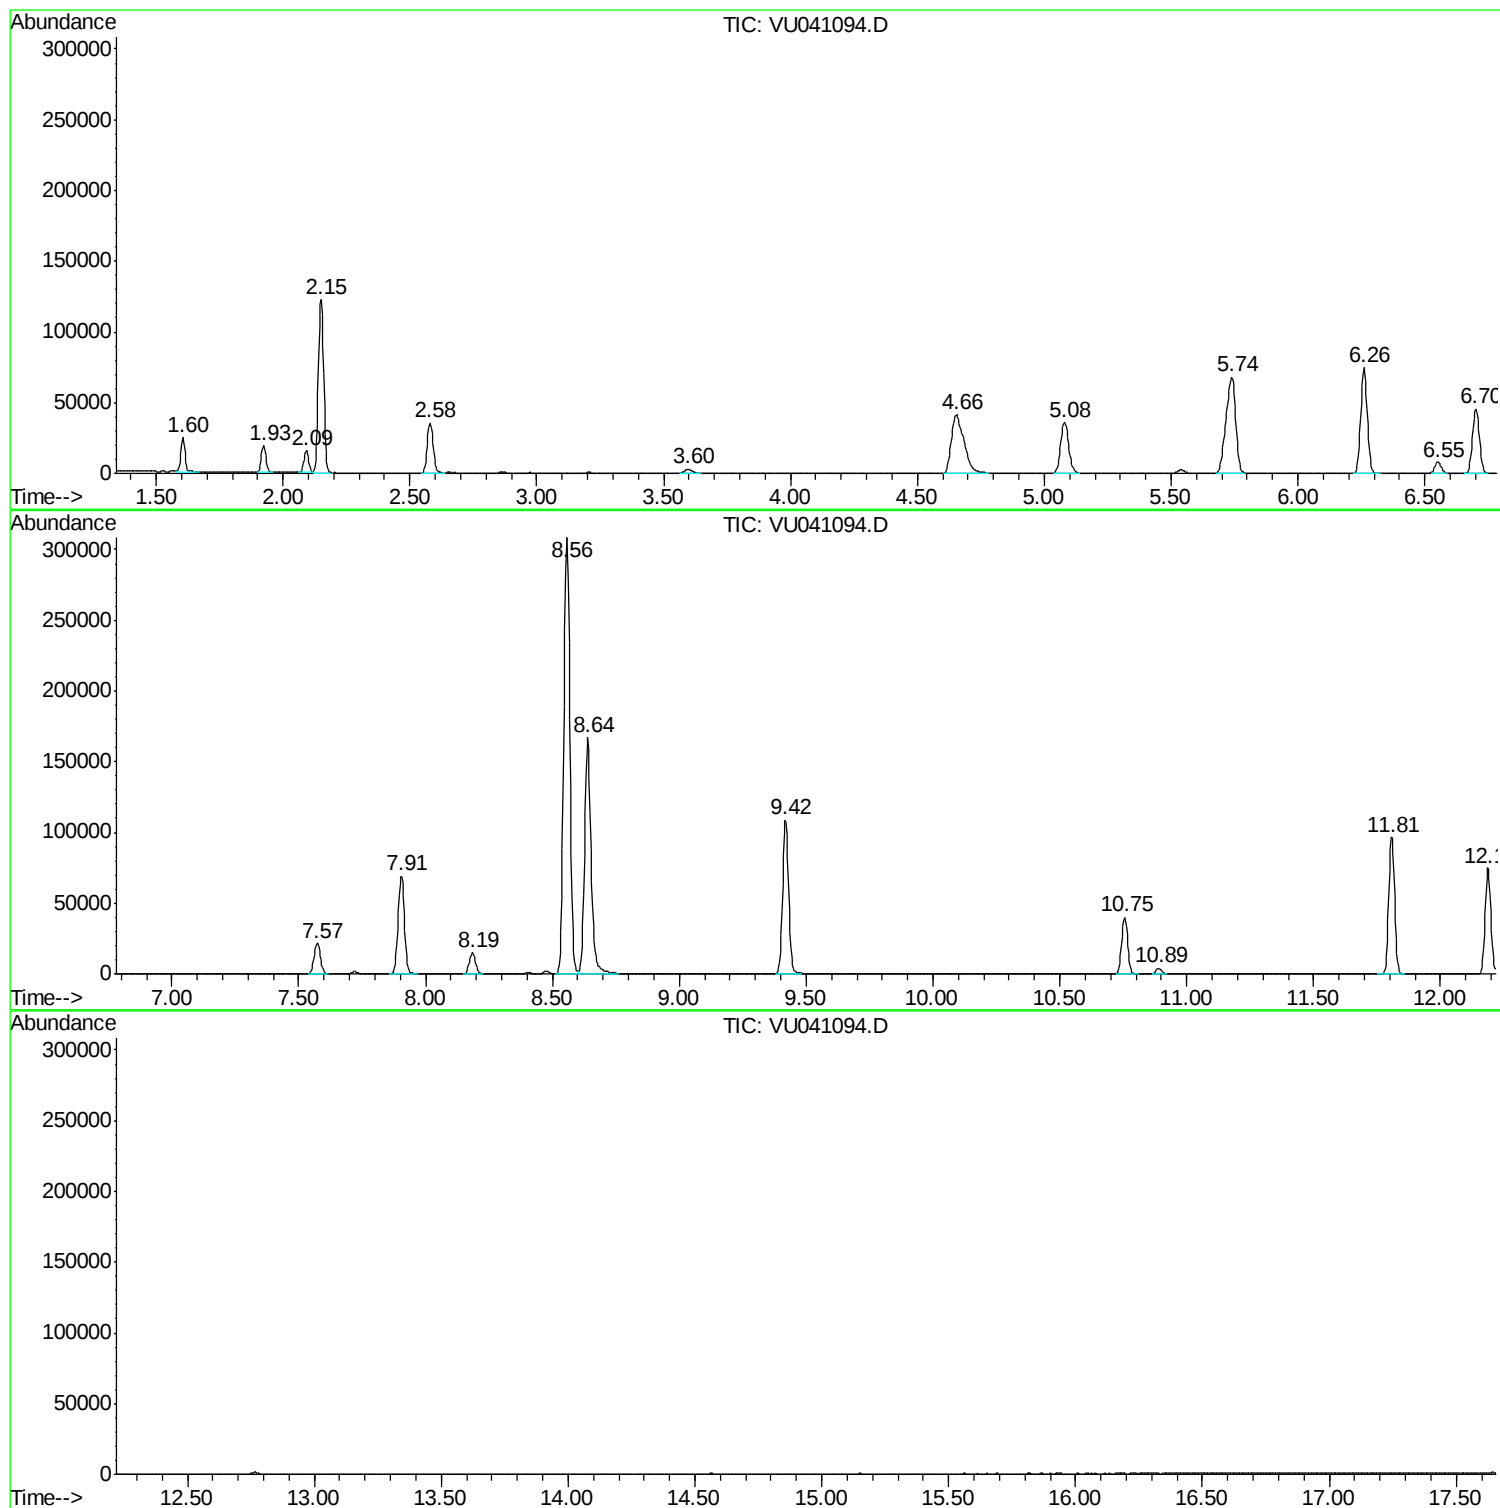

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU110420\
Data File : VU041094.D
Acq On : 04 Nov 2020 11:31
Operator : SY/MD
Sample : L4575-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AA2










Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorodichloromethane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.09	0.78 ug/L	21198	1,4-Difluorobenzene	6.26

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
2			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
3			Fluorodichloromethane	102	CHCl2F	000075-43-4	83
4			1-Hexyne	82	C6H10	000693-02-7	7
5			Chlorine dioxide	67	ClO2	010049-04-4	5

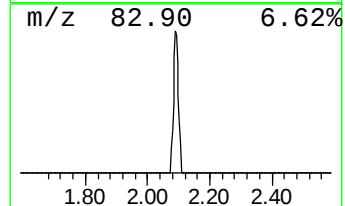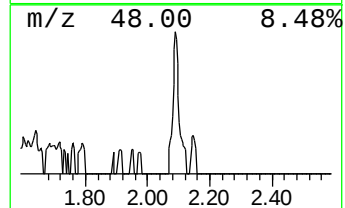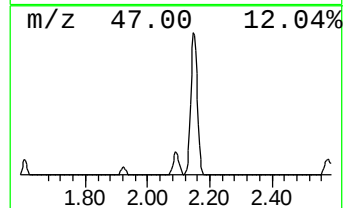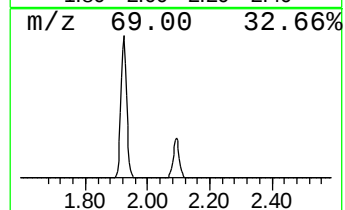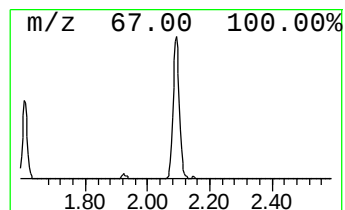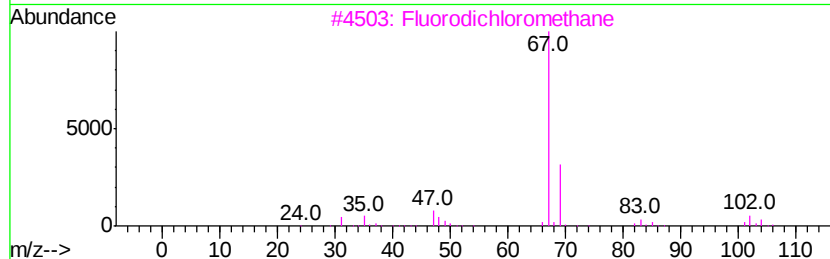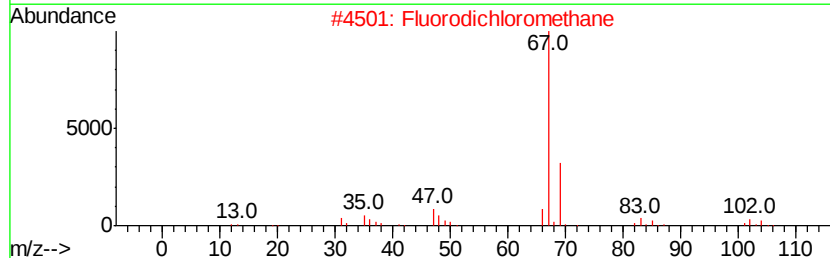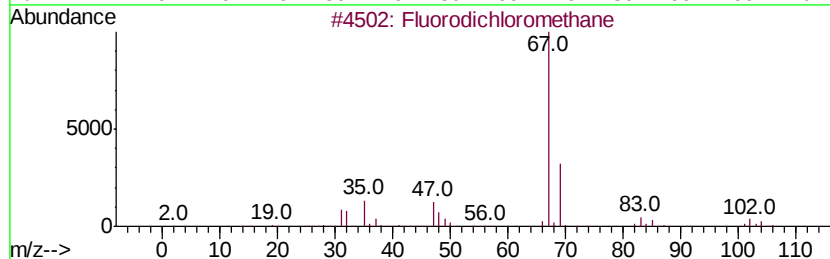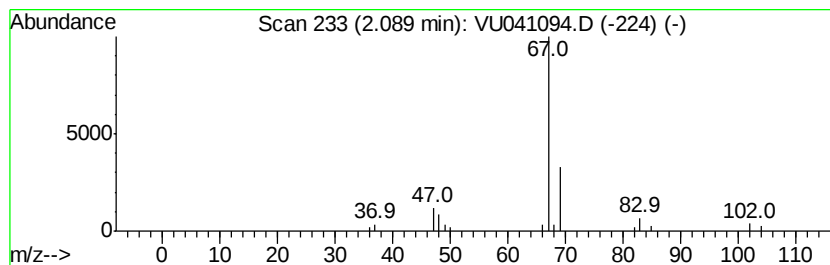

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU110420\
Data File : VU041094.D
Acq On : 04 Nov 2020 11:31
Operator : SY/MD
Sample : L4575-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AA2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Fluorodichloromet...	2.09	0.8	ug/L	21198	1	6.26	135289	5.0