


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU110420\
 Data File : VU041091.D
 Acq On : 04 Nov 2020 09:29
 Operator : SY/MD
 Sample : BFB05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB05

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Nov 05 19:34:14 2020

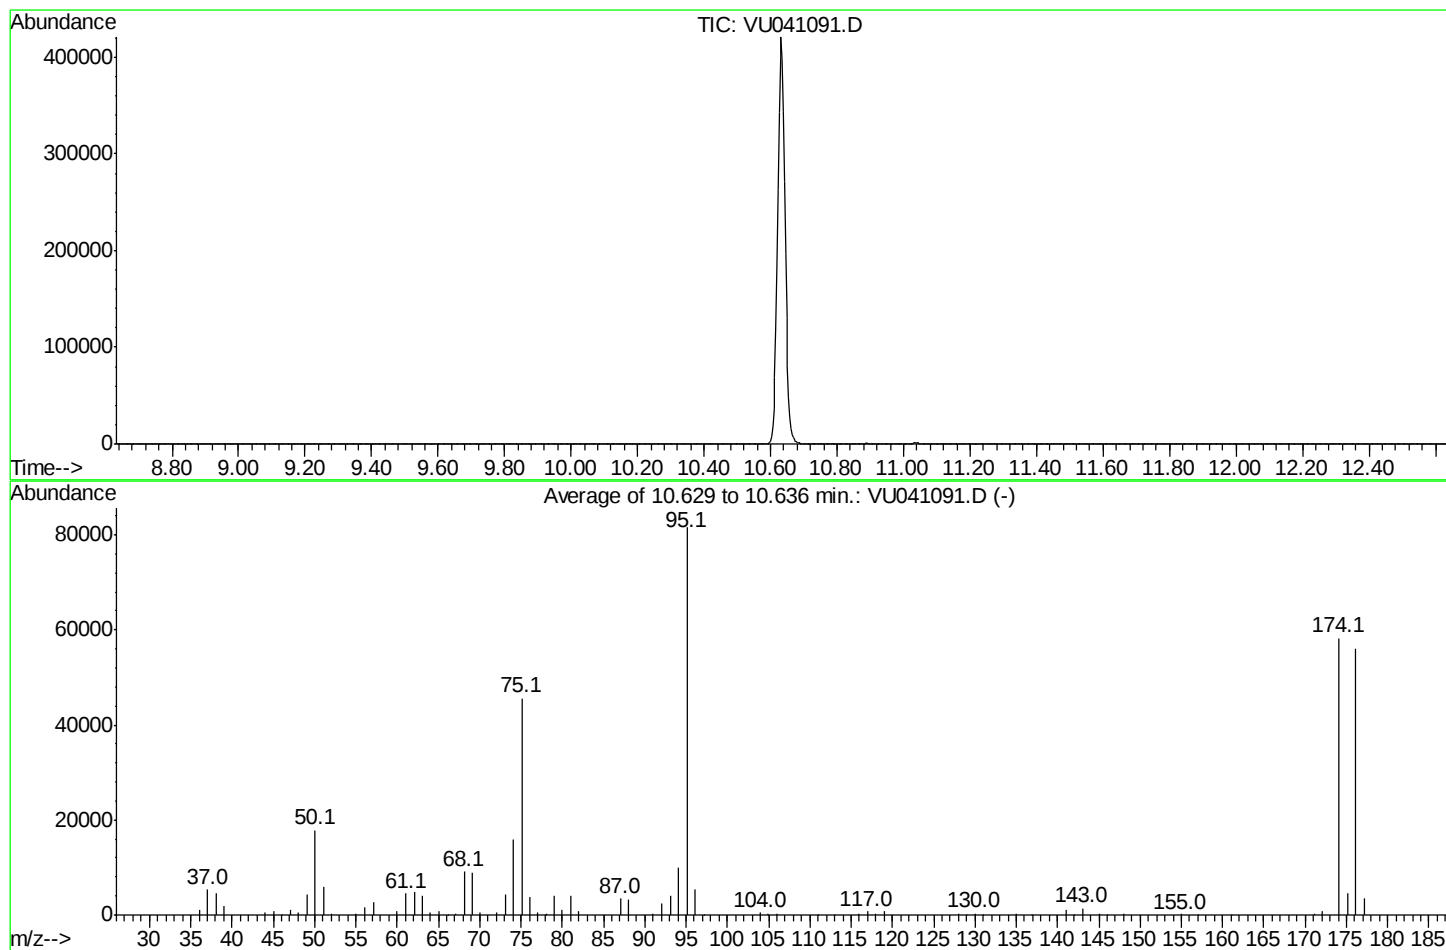

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	17845	PASS
75	95	30	80	55.9	45605	PASS
95	95	100	100	100.0	81586	PASS
96	95	5	9	6.6	5413	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.4	58258	PASS
175	174	5	9	7.8	4543	PASS
176	174	95	101	96.0	55938	PASS
177	176	5	9	6.3	3549	PASS

m/z	Abundance
44.00	135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
36.00	940.0
37.10	5166.0
38.10	4349.0
39.00	1736.0
44.00	741.0
45.10	851.0
46.00	135.0
47.00	995.0
47.90	576.0
49.10	4151.0
50.10	17312.0
51.10	5601.0
52.00	232.0
55.00	288.0
56.00	1489.0
57.10	2524.0
60.00	878.0
61.10	4434.0
62.10	4727.0
63.10	3888.0
64.10	486.0
65.10	639.0
67.10	316.0
68.10	8732.0
69.10	8539.0
70.00	626.0
72.00	550.0
73.10	4196.0
74.10	15516.0
75.10	44408.0
76.10	3605.0
77.10	518.0
77.90	268.0
79.00	3783.0
79.90	995.0
81.00	3946.0
81.90	827.0
87.00	3364.0
88.10	3139.0
91.00	375.0
92.10	2394.0
93.10	3994.0
94.10	9628.0
95.10	80040.0
96.10	5165.0
97.10	131.0
104.00	530.0
104.90	168.0
106.00	359.0
111.00	116.0
116.00	310.0
117.00	697.0
118.00	380.0
119.00	631.0
128.00	323.0
129.00	129.0
130.00	322.0
130.90	109.0
135.00	127.0
136.90	103.0
141.00	1060.0
142.10	119.0
143.00	1376.0
145.00	312.0
146.00	114.0
148.00	181.0
155.00	193.0
157.00	101.0
161.00	111.0
171.00	154.0
172.00	841.0
174.10	58464.0
175.10	4395.0
176.10	56584.0
177.10	3484.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
36.00	996.0
37.00	5661.0
38.10	4703.0
39.10	1854.0
44.00	822.0
45.10	900.0
46.00	139.0
47.00	1029.0
47.90	613.0
49.10	4567.0
50.10	18416.0
51.10	6085.0
52.00	241.0
55.00	315.0
56.10	1625.0
57.10	2761.0
60.00	976.0
61.10	4713.0
62.10	4841.0
63.10	4214.0
64.10	543.0
65.10	751.0
66.10	110.0
67.10	346.0
68.10	9329.0
69.10	9383.0
70.10	676.0
72.00	551.0
73.10	4420.0
74.10	16648.0
75.10	47248.0
76.10	3878.0
77.00	586.0
78.10	284.0
79.00	4049.0
80.00	1044.0
81.00	4182.0
82.00	924.0
87.10	3590.0
88.10	3278.0
91.00	396.0
92.10	2627.0
93.10	4250.0
94.10	10186.0
95.10	84400.0
96.10	5575.0
97.10	151.0
104.00	486.0
104.90	156.0
106.00	366.0
111.00	106.0
113.00	104.0
116.00	367.0
117.00	794.0
118.00	386.0
119.00	717.0
128.00	340.0
129.00	128.0
130.00	373.0
130.90	129.0
135.00	143.0
136.90	112.0
141.00	1080.0
142.00	127.0
143.00	1453.0
145.00	341.0
145.90	115.0
148.00	193.0
155.00	197.0
157.00	110.0
161.00	131.0
171.10	168.0
172.00	964.0
174.10	60160.0
175.10	4707.0
176.10	57872.0
177.10	3696.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
36.00	999.0
37.00	5321.0
38.10	4684.0
39.10	1793.0
44.00	806.0
45.00	856.0
46.00	119.0
47.10	954.0
48.00	612.0
49.10	4428.0
50.10	17808.0
51.10	5841.0
52.00	246.0
55.00	318.0
56.10	1595.0
57.10	2711.0
60.00	954.0
61.10	4567.0
62.10	4660.0
63.10	4162.0
64.00	584.0
65.10	841.0
66.10	104.0
67.10	315.0
68.10	9212.0
69.10	9166.0
70.10	677.0
72.00	507.0
73.10	4180.0
74.10	15934.0
75.10	45160.0
76.10	3821.0
77.00	586.0
78.20	292.0
79.00	3958.0
80.00	1028.0
81.00	4011.0
82.00	930.0
87.00	3393.0
88.00	3154.0
91.00	401.0
92.10	2644.0
93.10	4019.0
94.10	9862.0
95.10	80320.0
96.10	5499.0
97.10	145.0
104.00	380.0
105.00	118.0
106.00	372.0
113.00	100.0
116.00	361.0
117.00	836.0
118.00	358.0
119.00	734.0
128.00	293.0
128.90	107.0
130.00	365.0
131.00	126.0
135.00	164.0
136.90	133.0
141.00	950.0
141.90	121.0
143.00	1399.0
145.00	386.0
145.90	102.0
148.00	162.0
155.00	173.0
161.00	130.0
171.10	158.0
172.00	927.0
174.10	56152.0
175.10	4529.0
176.10	53360.0
177.10	3467.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05