


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110421\
Data File : VU045529.D
Acq On : 03 Nov 2021 18:38
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U102821W.M
Title : SW846 8260
Last Update : Fri Oct 29 11:09:42 2021

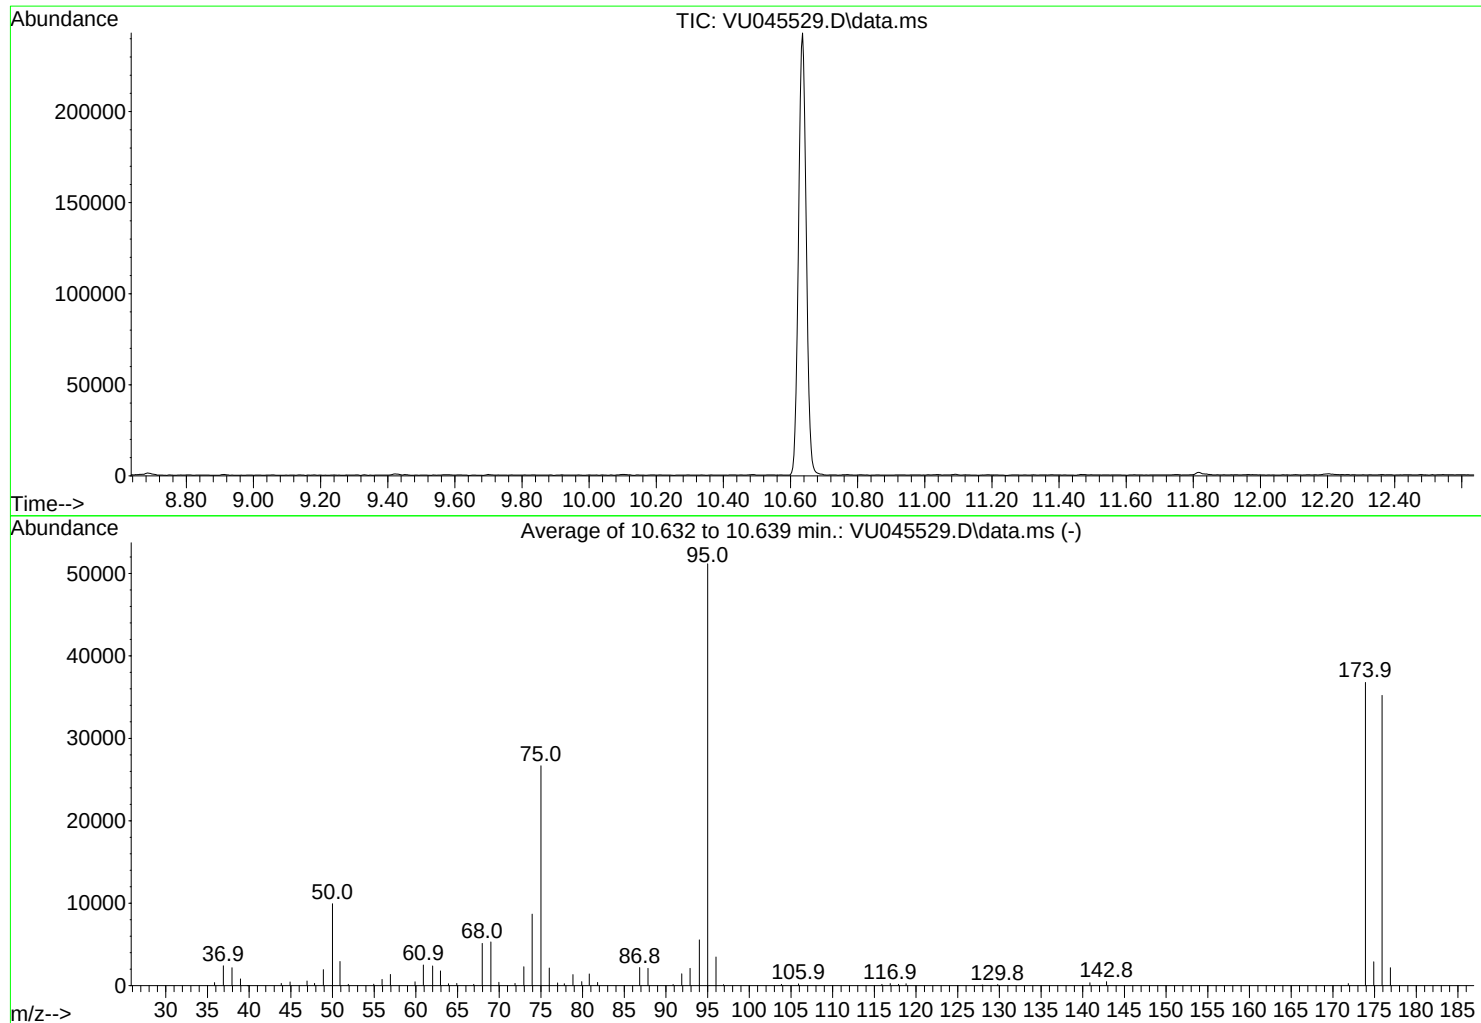

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	9932	PASS
75	95	30	60	52.1	26680	PASS
95	95	100	100	100.0	51171	PASS
96	95	5	9	6.8	3485	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	71.9	36792	PASS
175	174	5	9	7.9	2901	PASS
176	174	95	101	95.7	35216	PASS
177	176	5	9	6.2	2180	PASS