


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110519\
Data File : VU035616.D
Acq On : 05 Nov 2019 08:20
Operator : JC/SP
Sample : BFB25
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB25

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
Title : VOC Analysis
Last Update : Fri Nov 15 01:03:04 2019

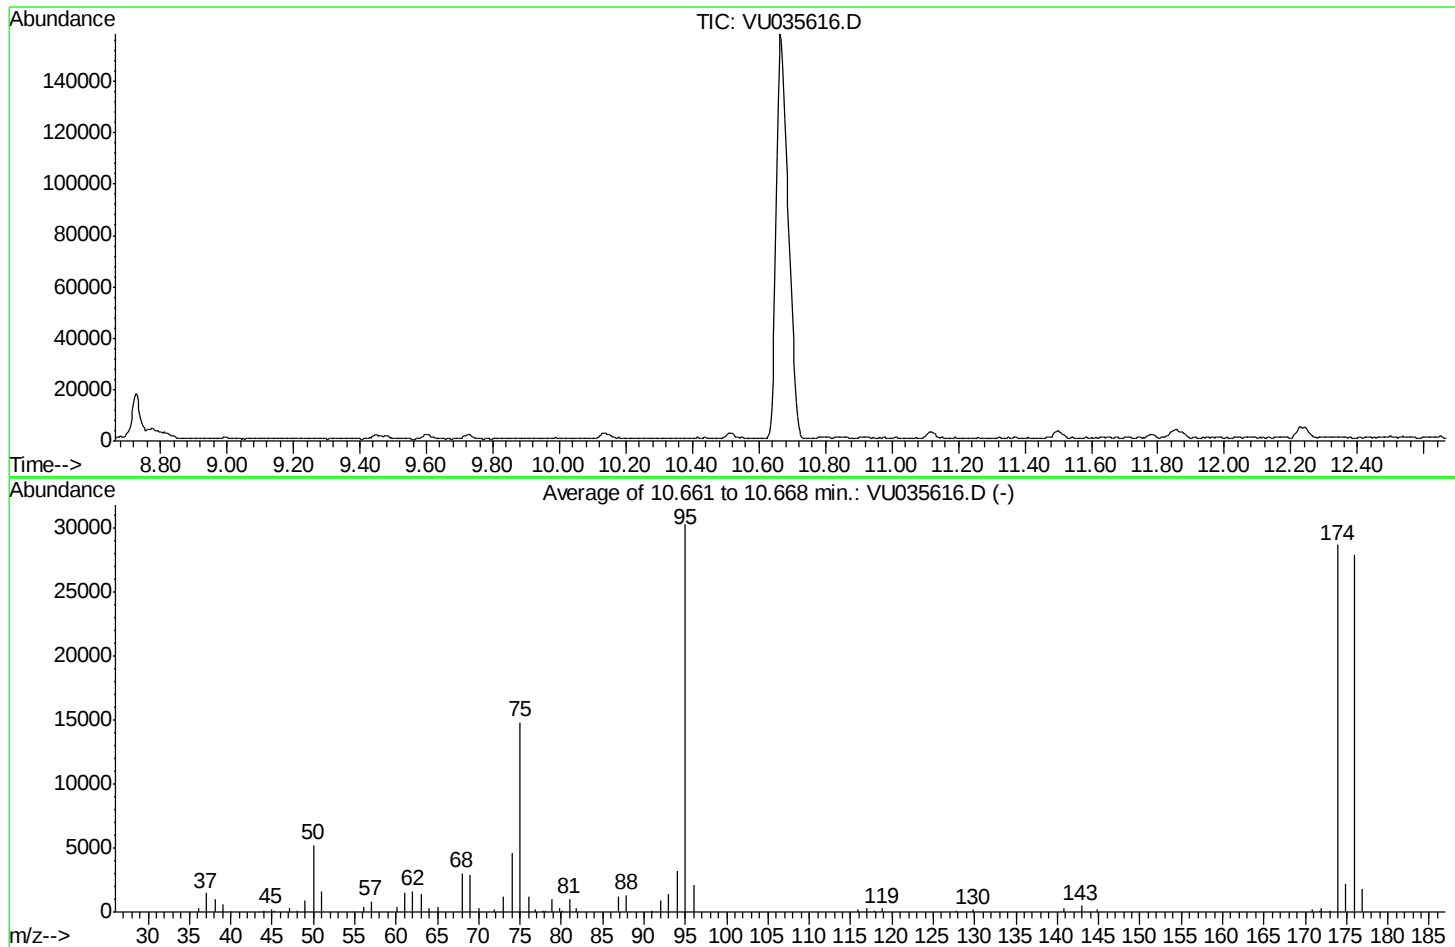

AutoFind: Scans 2899, 2900, 2901; Background Corrected with Scan 2886

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	5207	PASS
75	95	30	80	49.0	14830	PASS
95	95	100	100	100.0	30240	PASS
96	95	5	9	7.1	2141	PASS
173	174	0.00	2	0.4	106	PASS
174	95	50	120	94.8	28656	PASS
175	174	5	9	7.7	2217	PASS
176	174	95	101	97.3	27888	PASS
177	176	5	9	6.4	1793	PASS

Scan 2886 (10.619 min): VU035616.D
BFB25

m/z	Abundance
40.00	195.0
44.00	841.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
36.10	341.0
37.00	1477.0
38.10	992.0
39.10	525.0
39.90	195.0
44.00	904.0
44.90	261.0
47.10	229.0
48.10	109.0
49.00	840.0
50.00	4856.0
51.00	1485.0
56.00	407.0
57.00	779.0
60.10	287.0
61.00	1565.0
62.00	1483.0
63.10	1245.0
64.10	342.0
65.00	444.0
68.00	3045.0
69.00	2836.0
70.00	250.0
72.00	148.0
73.00	1247.0
74.00	4662.0
75.00	14064.0
76.10	1169.0
76.90	193.0
77.80	208.0
78.90	929.0
79.70	276.0
80.10	234.0
81.00	1018.0
81.80	306.0
86.90	1085.0
87.90	1248.0
90.90	131.0
92.00	887.0
93.00	1509.0
94.00	3026.0
95.00	30048.0
96.00	1989.0
115.90	162.0
116.90	224.0
118.90	307.0
127.80	140.0
129.90	186.0
140.80	349.0
142.90	514.0
144.90	168.0
170.90	124.0
171.80	347.0
173.00	318.0
174.00	27880.0
174.90	2232.0
175.90	26640.0
177.00	1761.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
36.10	274.0
37.00	1563.0
38.00	1033.0
39.00	588.0
40.00	184.0
43.90	958.0
44.90	232.0
47.10	321.0
48.10	134.0
49.00	923.0
50.00	5277.0
51.10	1650.0
54.80	109.0
56.10	432.0
56.90	825.0
60.10	411.0
61.00	1573.0
62.00	1592.0
63.00	1423.0
64.10	342.0
65.00	474.0
68.00	3059.0
69.00	2999.0
70.00	259.0
72.00	158.0
73.00	1173.0
74.00	4693.0
75.00	15112.0
76.10	1252.0
76.90	214.0
77.80	234.0
78.20	235.0
78.90	1043.0
79.80	280.0
80.90	991.0
81.80	359.0
86.90	1190.0
87.90	1352.0
90.90	141.0
91.90	899.0
93.00	1460.0
94.00	3213.0
95.00	30848.0
96.10	2202.0
115.90	168.0
116.90	267.0
117.80	123.0
118.90	298.0
127.80	146.0
129.90	205.0
140.90	352.0
142.90	523.0
144.80	202.0
170.90	189.0
172.00	365.0
174.00	29280.0
174.90	2218.0
176.00	28584.0
177.00	1839.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
36.00	219.0
37.00	1340.0
38.00	1014.0
39.00	621.0
39.90	210.0
43.90	1067.0
44.90	191.0
45.20	193.0
47.00	373.0
48.10	144.0
49.00	1027.0
50.00	5489.0
51.10	1731.0
56.10	416.0
56.90	830.0
60.10	446.0
61.10	1438.0
62.00	1800.0
63.00	1446.0
64.00	276.0
65.00	358.0
68.00	2963.0
69.00	2868.0
70.00	253.0
71.90	163.0
73.00	1199.0
74.00	4481.0
75.00	15316.0
76.10	1172.0
76.80	209.0
78.00	221.0
78.90	1074.0
79.80	326.0
80.90	1019.0
81.80	369.0
86.90	1256.0
87.90	1399.0
90.90	148.0
91.90	872.0
93.00	1256.0
94.00	3400.0
95.00	29824.0
96.10	2234.0
115.90	138.0
116.90	284.0
117.80	146.0
118.80	228.0
127.90	132.0
129.80	156.0
140.90	342.0
142.90	448.0
144.80	236.0
170.90	185.0
172.00	420.0
174.00	28808.0
174.90	2202.0
175.90	28440.0
176.90	1780.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25