

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU110520\
 Data File : VU041114.D
 Acq On : 05 Nov 2020 18:58
 Operator : SY/MD
 Sample : L4648-03
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AB0

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	94	rVB	23619	26109	4.26%	0.964%
2	1.922	173	181	193	rVB	20775	26072	4.26%	0.963%
3	2.089	225	233	241	rBV	13286	17924	2.93%	0.662%
4	2.147	241	251	267	rVB	148697	218263	35.63%	8.059%
5	2.578	375	385	399	rBV	38087	61245	10.00%	2.261%
6	3.597	692	702	716	rBV3	3145	6997	1.14%	0.258%
7	4.652	1013	1030	1062	rBV2	47355	155721	25.42%	5.750%
8	5.083	1150	1164	1184	rBB3	38063	94169	15.37%	3.477%
9	5.539	1295	1306	1317	rBV2	3280	6173	1.01%	0.228%
10	5.738	1348	1368	1389	rBV2	74114	197072	32.17%	7.277%
11	6.263	1517	1531	1551	rBV	68422	124707	20.36%	4.605%
12	6.552	1612	1621	1631	rVB4	7577	13349	2.18%	0.493%
13	6.703	1654	1668	1684	rBB	53326	101196	16.52%	3.737%
14	7.574	1928	1939	1954	rVB	24172	39606	6.47%	1.462%
15	7.906	2029	2042	2064	rBV	76164	127759	20.86%	4.717%
16	8.185	2119	2129	2142	rBV2	16447	27679	4.52%	1.022%
17	8.558	2232	2245	2259	rBV	371148	612548	100.00%	22.618%
18	8.639	2259	2270	2298	rVB	180830	319012	52.08%	11.779%
19	9.420	2500	2513	2533	rBV	103720	170703	27.87%	6.303%
20	10.754	2912	2928	2944	rBV	45980	73165	11.94%	2.702%
21	10.889	2959	2970	2984	rBV3	5791	9181	1.50%	0.339%
22	11.809	3244	3256	3270	rBV	91531	144954	23.66%	5.352%
23	12.188	3362	3374	3386	rBV	84484	134636	21.98%	4.971%


Sum of corrected areas: 2708240

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU110520\
Data File : VU041114.D
Acq On : 05 Nov 2020 18:58
Operator : SY/MD
Sample : L4648-03
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AB0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

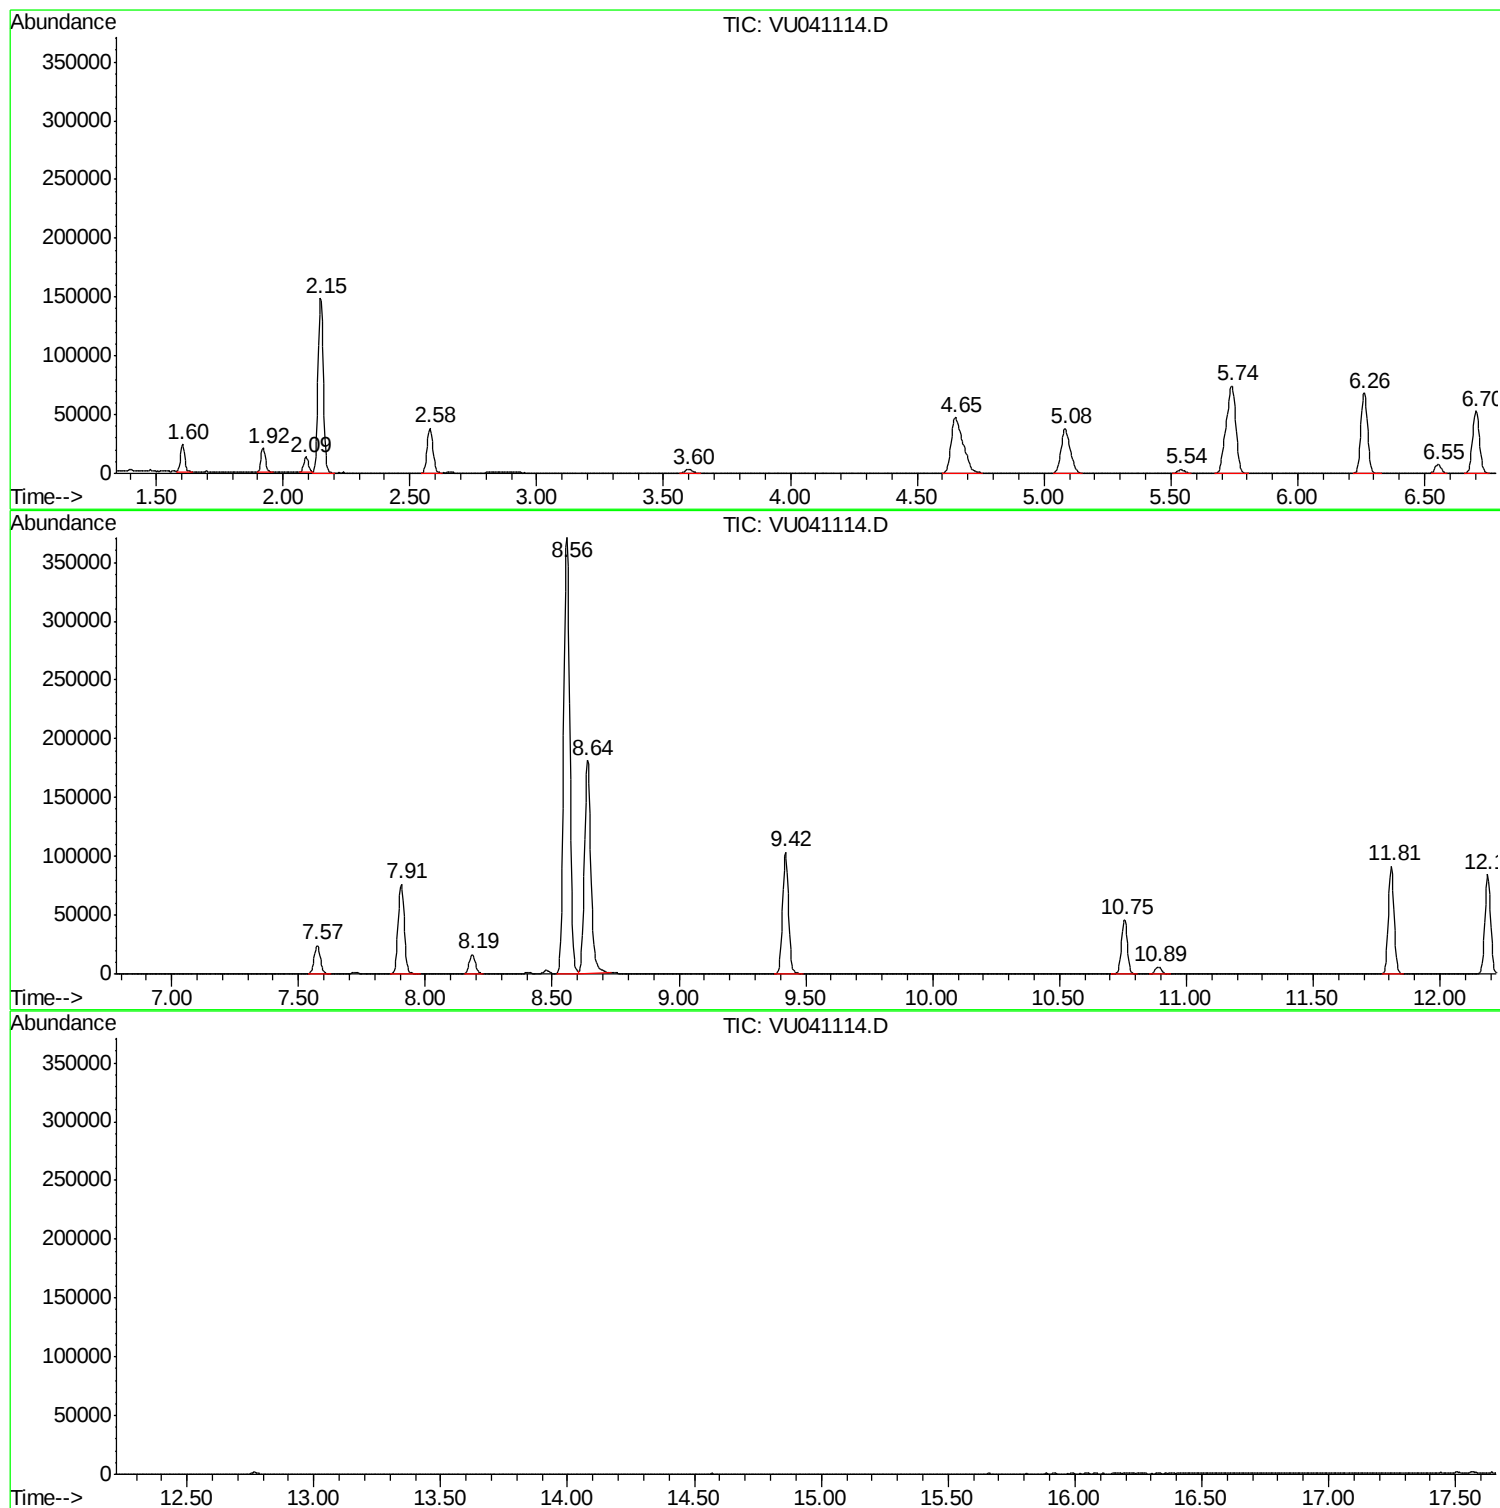

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU110520\
Data File : VU041114.D
Acq On : 05 Nov 2020 18:58
Operator : SY/MD
Sample : L4648-03
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AB0










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorodichloromethane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.09	0.72 ug/L	17924	1,4-Difluorobenzene	6.26

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Fluorodichloromethane	102	CHCl2F	000075-43-4	94
2		Fluorodichloromethane	102	CHCl2F	000075-43-4	91
3		Fluorodichloromethane	102	CHCl2F	000075-43-4	86
4		Chlorine dioxide	67	ClO2	010049-04-4	5
5		Methanamine, N,N-difluoro-	67	CH3F2N	000753-58-2	5

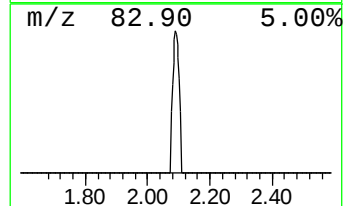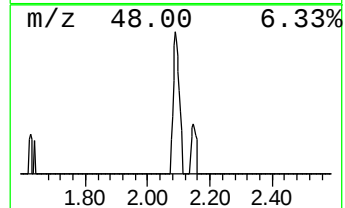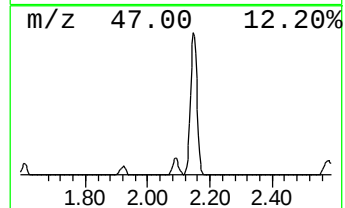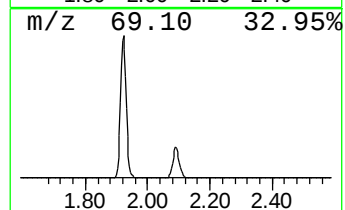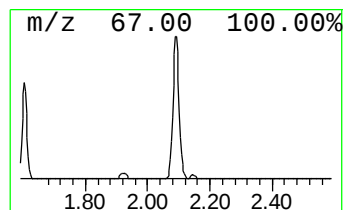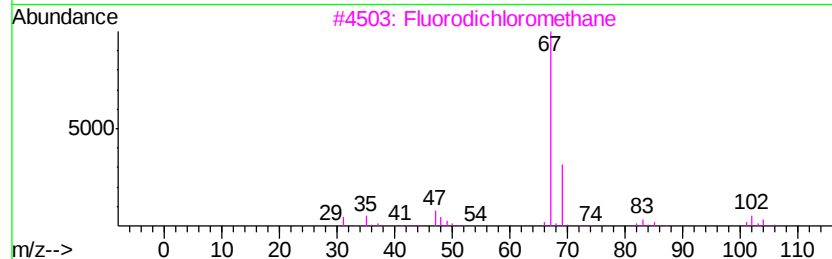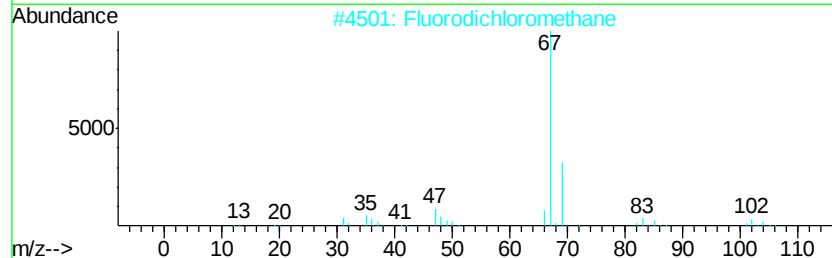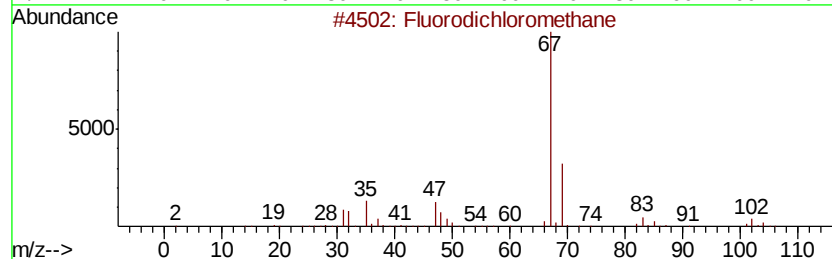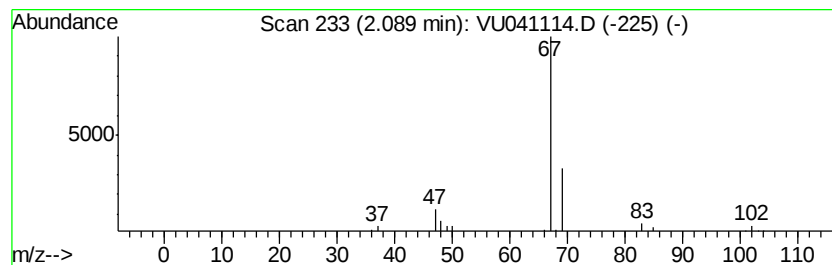

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU110520\
Data File : VU041114.D
Acq On : 05 Nov 2020 18:58
Operator : SY/MD
Sample : L4648-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AB0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Fluorodichloromet...	2.09	0.7	ug/L	17924	1	6.26	124707	5.0