


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU110520\
 Data File : VU041104.D
 Acq On : 05 Nov 2020 13:13
 Operator : SY/MD
 Sample : BFB06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB06

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Nov 06 01:44:25 2020

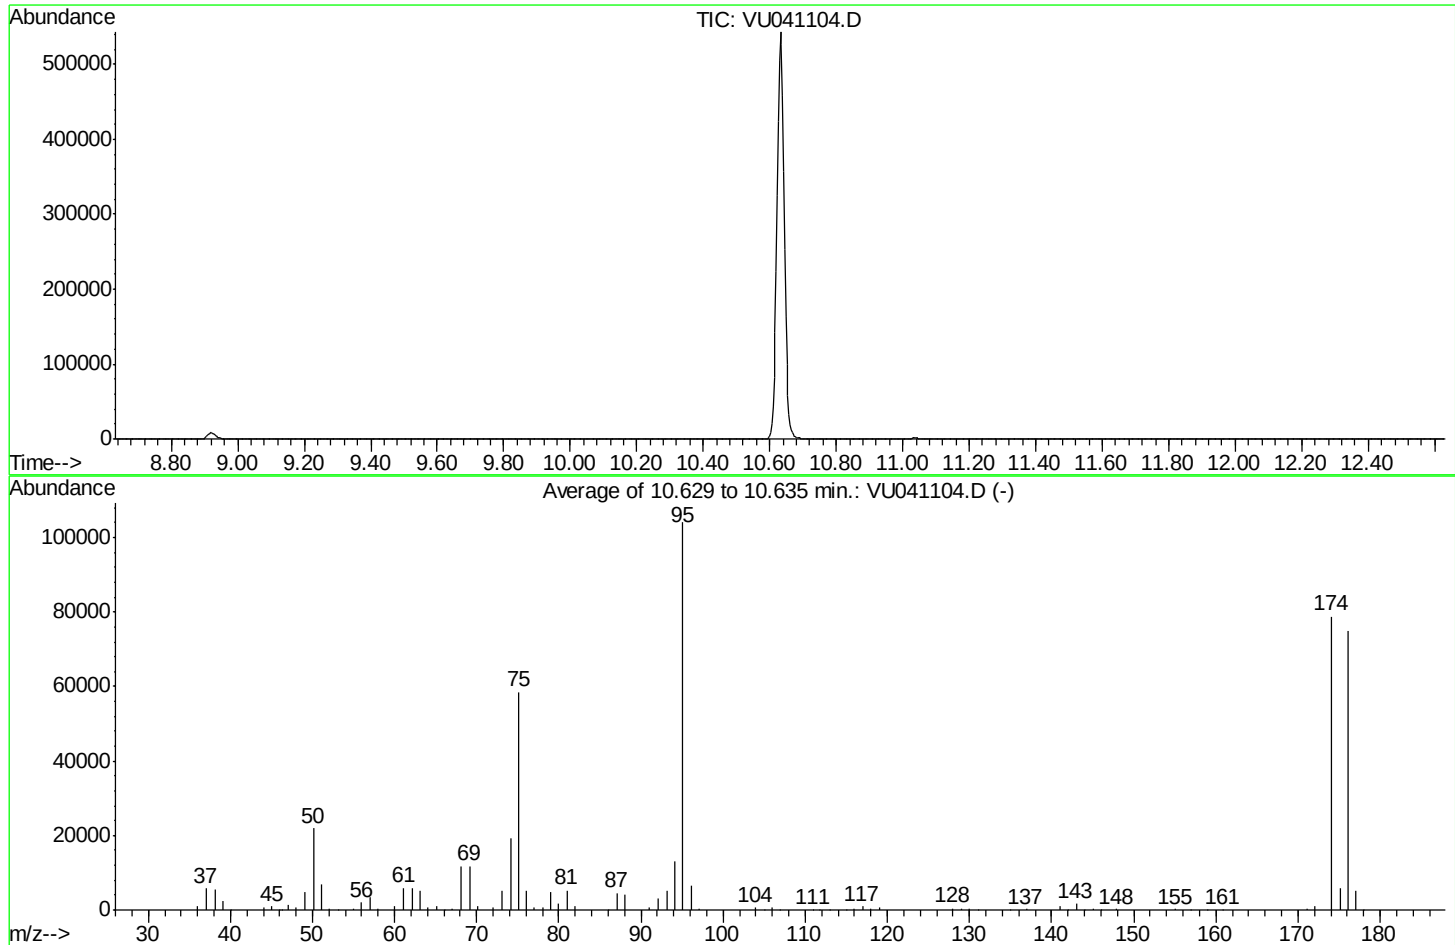

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	21896	PASS
75	95	30	80	56.2	58512	PASS
95	95	100	100	100.0	104072	PASS
96	95	5	9	6.4	6621	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.7	78744	PASS
175	174	5	9	7.5	5944	PASS
176	174	95	101	95.2	74946	PASS
177	176	5	9	6.7	5007	PASS

m/z	Abundance
36.00	1071.0
37.00	6019.0
38.10	5759.0
39.10	2360.0
40.00	110.0
44.00	921.0
45.00	1056.0
46.20	174.0
47.10	1585.0
47.90	832.0
49.10	5113.0
50.10	22712.0
51.10	7318.0
52.00	274.0
53.10	140.0
55.00	262.0
56.00	2039.0
57.10	3467.0
58.00	206.0
60.10	1014.0
61.10	6097.0
62.10	5930.0
63.10	5456.0
64.00	797.0
65.10	1007.0
66.00	104.0
67.00	374.0
68.10	11988.0
69.10	12119.0
70.10	913.0
72.00	736.0
73.10	5520.0
74.10	19832.0
75.10	60768.0
76.10	5385.0
77.00	648.0
78.00	560.0
79.00	5130.0
80.00	1625.0
81.00	5431.0
82.00	1241.0
86.00	148.0
87.10	4808.0
88.00	4184.0
91.00	556.0
92.00	3378.0
93.10	5217.0
94.10	13346.0
95.10	107608.0
96.10	6805.0
97.10	221.0
104.00	678.0
105.00	180.0
106.00	549.0
106.90	137.0
111.00	131.0
111.80	119.0
113.00	130.0
114.90	191.0
116.00	419.0
117.00	1023.0
118.00	444.0
119.00	868.0
128.00	431.0
129.00	202.0
130.00	332.0
131.10	145.0
135.00	142.0
136.90	242.0
141.00	1143.0
142.00	155.0
143.00	1737.0
144.10	112.0
145.10	475.0
146.00	154.0
147.90	248.0
155.10	272.0
157.00	176.0
159.00	172.0
171.10	260.0
172.10	1227.0
174.10	81576.0
175.10	6118.0
176.10	77448.0
177.10	5180.0
178.00	187.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

m/z	Abundance
36.00	1057.0
37.00	5595.0
38.10	5540.0
39.10	2303.0
40.00	119.0
44.00	899.0
45.00	927.0
46.00	192.0
47.10	1453.0
47.90	714.0
49.10	4745.0
50.10	21312.0
51.10	6815.0
52.00	313.0
53.10	158.0
55.00	275.0
56.00	1836.0
57.00	3292.0
58.00	179.0
60.00	919.0
61.10	6012.0
62.10	5658.0
63.10	5243.0
64.00	806.0
65.10	985.0
67.00	348.0
68.10	11180.0
69.10	11324.0
70.10	795.0
72.00	681.0
73.10	5189.0
74.10	18792.0
75.10	57064.0
76.10	5210.0
77.00	631.0
78.00	530.0
79.00	4976.0
80.00	1660.0
81.00	5134.0
82.00	1205.0
86.00	157.0
87.10	4220.0
88.10	3706.0
91.00	575.0
92.10	3110.0
93.10	4892.0
94.10	12540.0
95.10	100408.0
96.10	6513.0
97.10	205.0
104.00	668.0
105.00	189.0
106.00	505.0
107.00	128.0
111.00	102.0
113.00	119.0
115.00	183.0
116.00	413.0
117.00	1026.0
117.90	426.0
119.00	859.0
128.00	375.0
129.00	190.0
130.00	320.0
131.00	127.0
135.00	137.0
136.90	207.0
141.00	1066.0
142.00	158.0
143.00	1670.0
144.10	100.0
145.00	526.0
146.00	137.0
148.00	193.0
155.10	260.0
157.00	135.0
158.90	134.0
171.10	236.0
172.10	1199.0
174.10	73920.0
175.10	5810.0
176.10	70136.0
177.10	4805.0
177.90	154.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

m/z	Abundance
44.00	169.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

m/z	Abundance
36.00	1019.0
37.00	5796.0
38.10	5410.0
39.10	2202.0
44.00	994.0
45.10	1027.0
46.20	173.0
47.10	1522.0
48.00	839.0
49.10	4930.0
50.10	21664.0
51.10	6884.0
52.10	252.0
55.00	247.0
56.00	1981.0
57.10	3295.0
58.00	211.0
60.10	1068.0
61.10	5532.0
62.10	5699.0
63.10	5072.0
64.00	734.0
65.10	906.0
67.10	339.0
68.10	11460.0
69.10	11610.0
70.10	917.0
72.00	731.0
73.10	5175.0
74.10	19112.0
75.10	57704.0
76.10	4976.0
77.00	605.0
78.00	555.0
79.00	4847.0
80.00	1508.0
81.00	5130.0
82.00	1164.0
86.10	135.0
87.10	4624.0
88.00	4187.0
91.00	506.0
92.10	3312.0
93.10	4939.0
94.10	13145.0
95.10	104200.0
96.10	6547.0
97.10	193.0
104.00	657.0
105.00	164.0
106.00	543.0
106.90	114.0
111.00	159.0
111.80	114.0
113.00	117.0
114.90	154.0
115.90	377.0
117.00	915.0
118.00	438.0
119.00	757.0
128.00	436.0
129.00	205.0
130.00	342.0
131.10	149.0
134.90	153.0
136.90	248.0
141.00	1163.0
142.00	156.0
143.00	1607.0
144.00	100.0
145.10	350.0
146.00	140.0
147.90	295.0
155.10	266.0
157.00	204.0
159.00	156.0
160.90	126.0
171.10	229.0
172.10	1099.0
174.10	80736.0
175.10	5905.0
176.10	77256.0
177.10	5036.0
178.00	178.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06