


1,3-Dichloropropane

Response Ratio

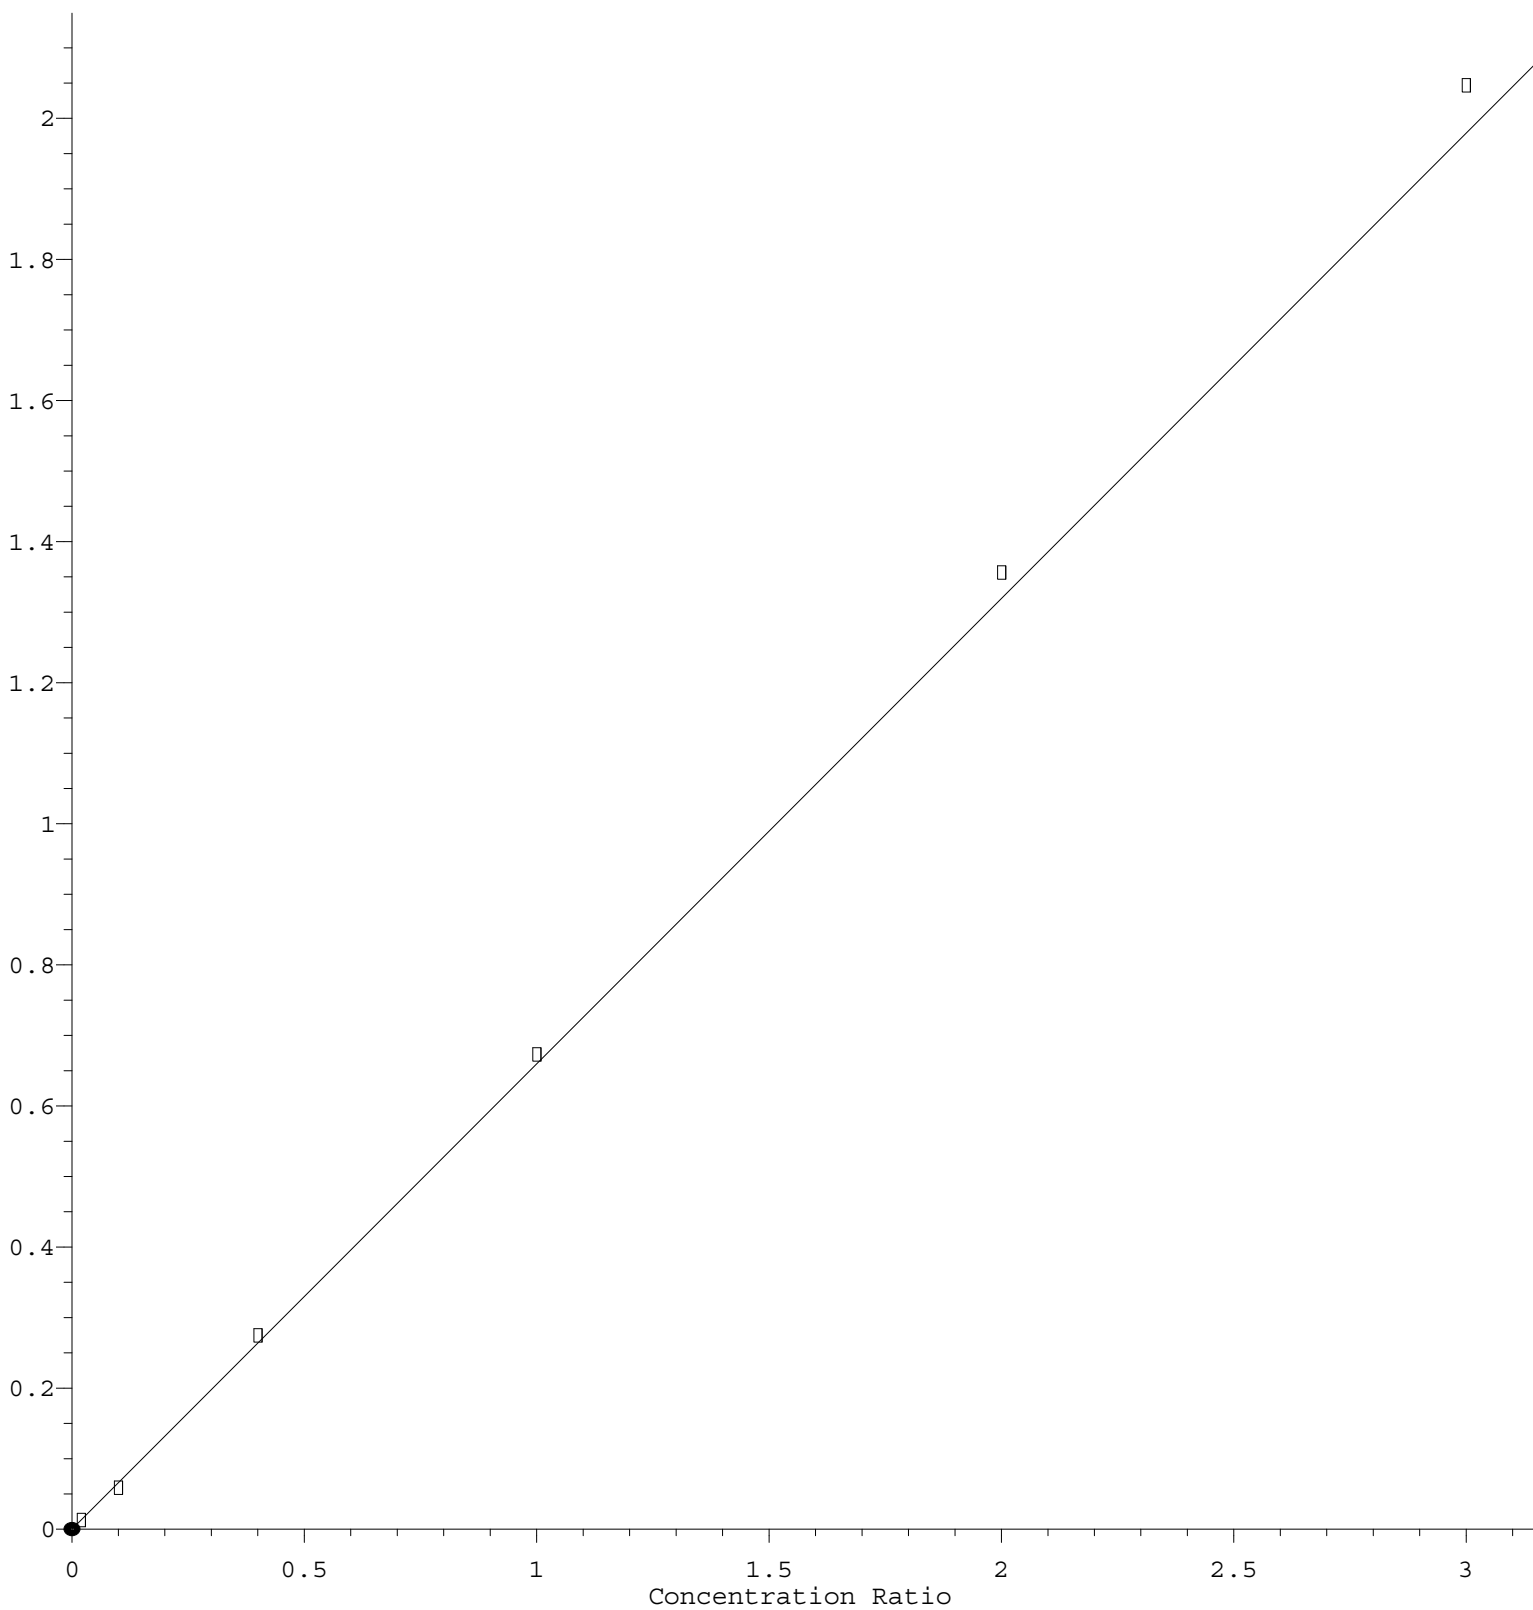

$$\text{Response} = 6.597\text{e-}001 * \text{Amt}$$


RF Rel Std Dev = 5.667% Curve Fit: Avg RF

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U110521W.M

Calibration Table Last Updated: Fri Nov 05 13:35:16 2021

2-Hexanone


Response Ratio

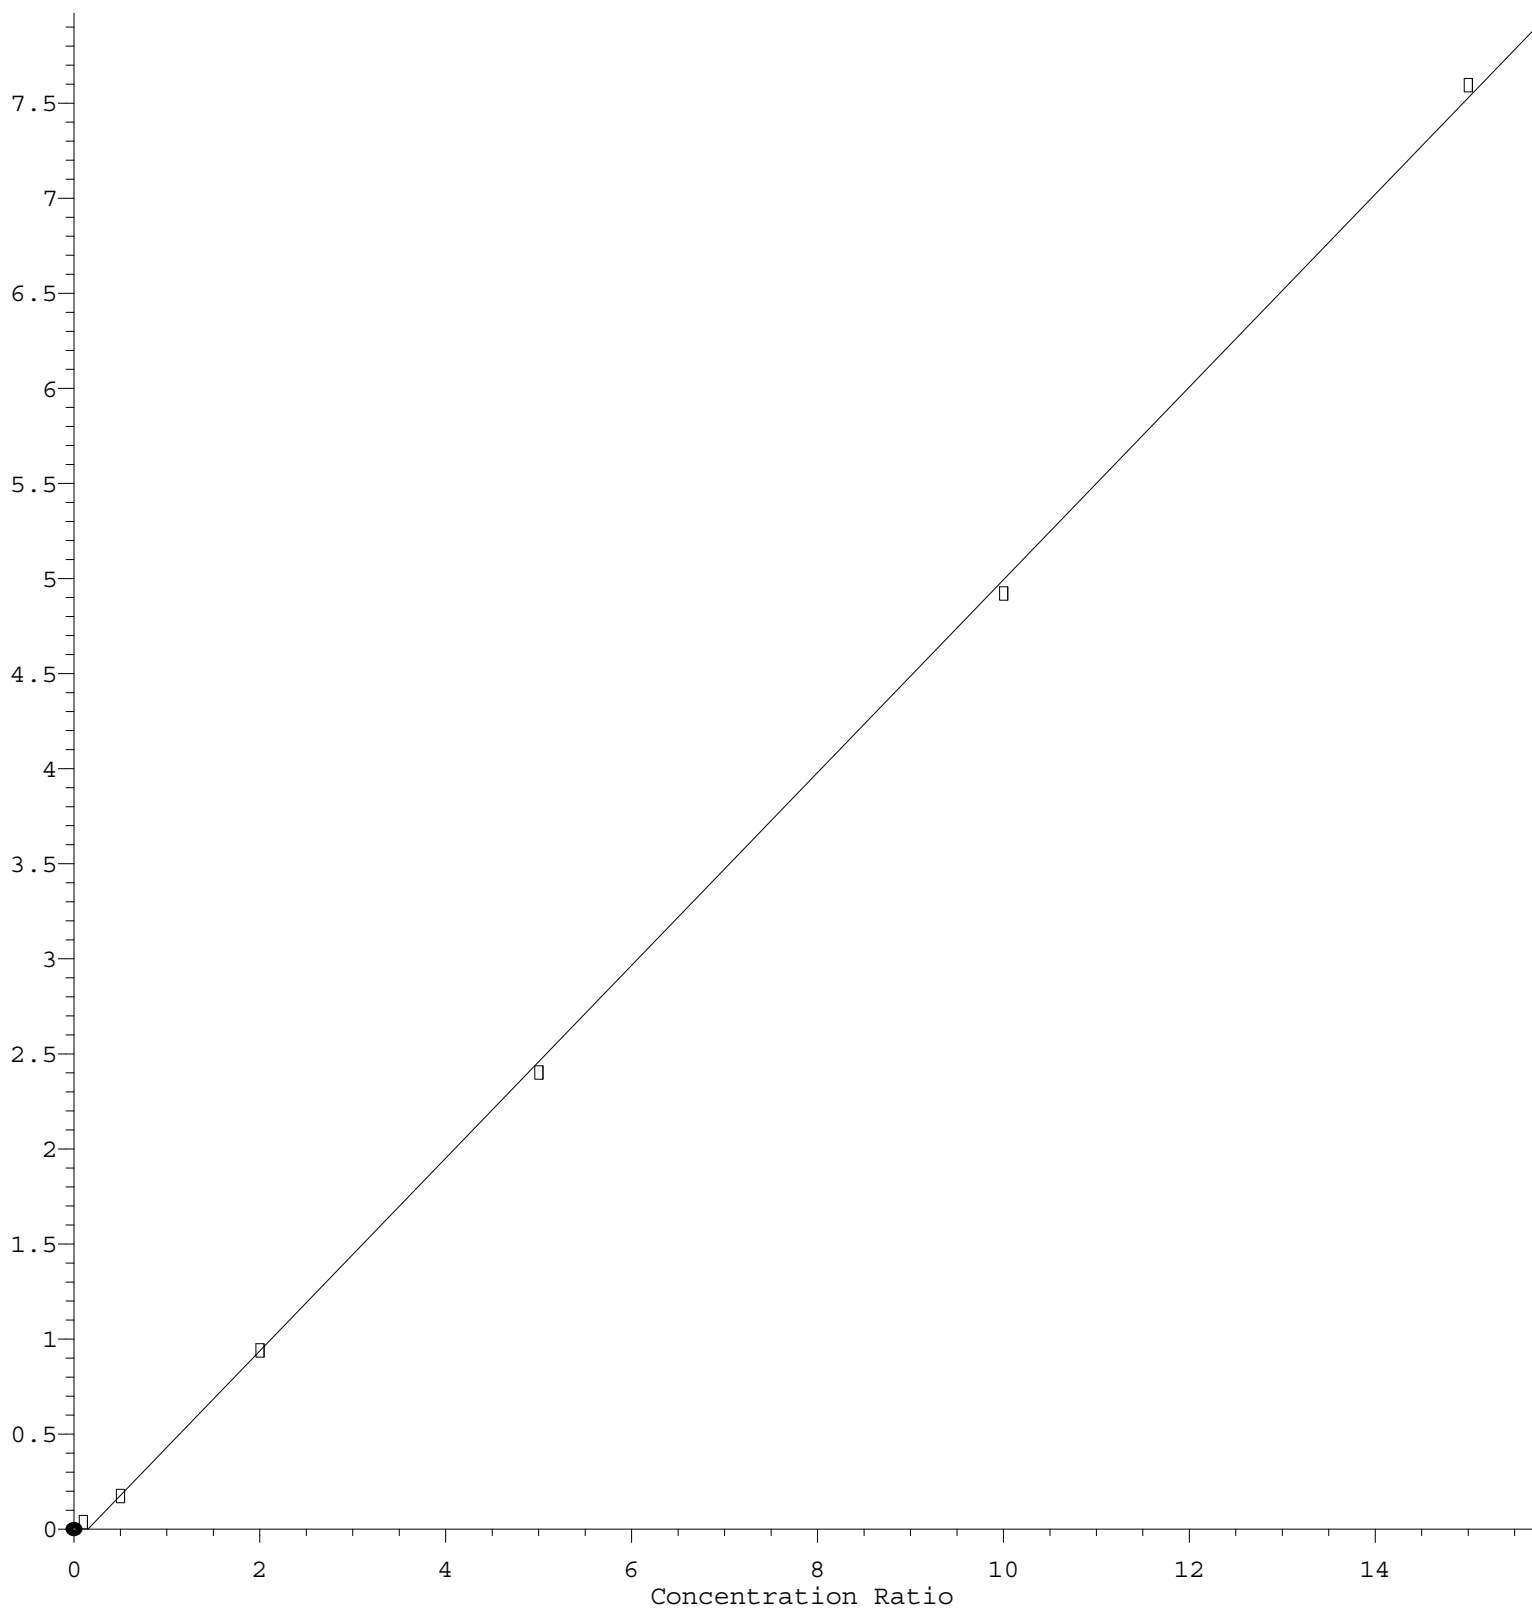

Response = 5.070e-001 * Amt - 7.640e-002
Coef of Det (r^2) = 0.999632 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U110521W.M
Calibration Table Last Updated: Fri Nov 05 13:35:16 2021

Bromoform

Response Ratio

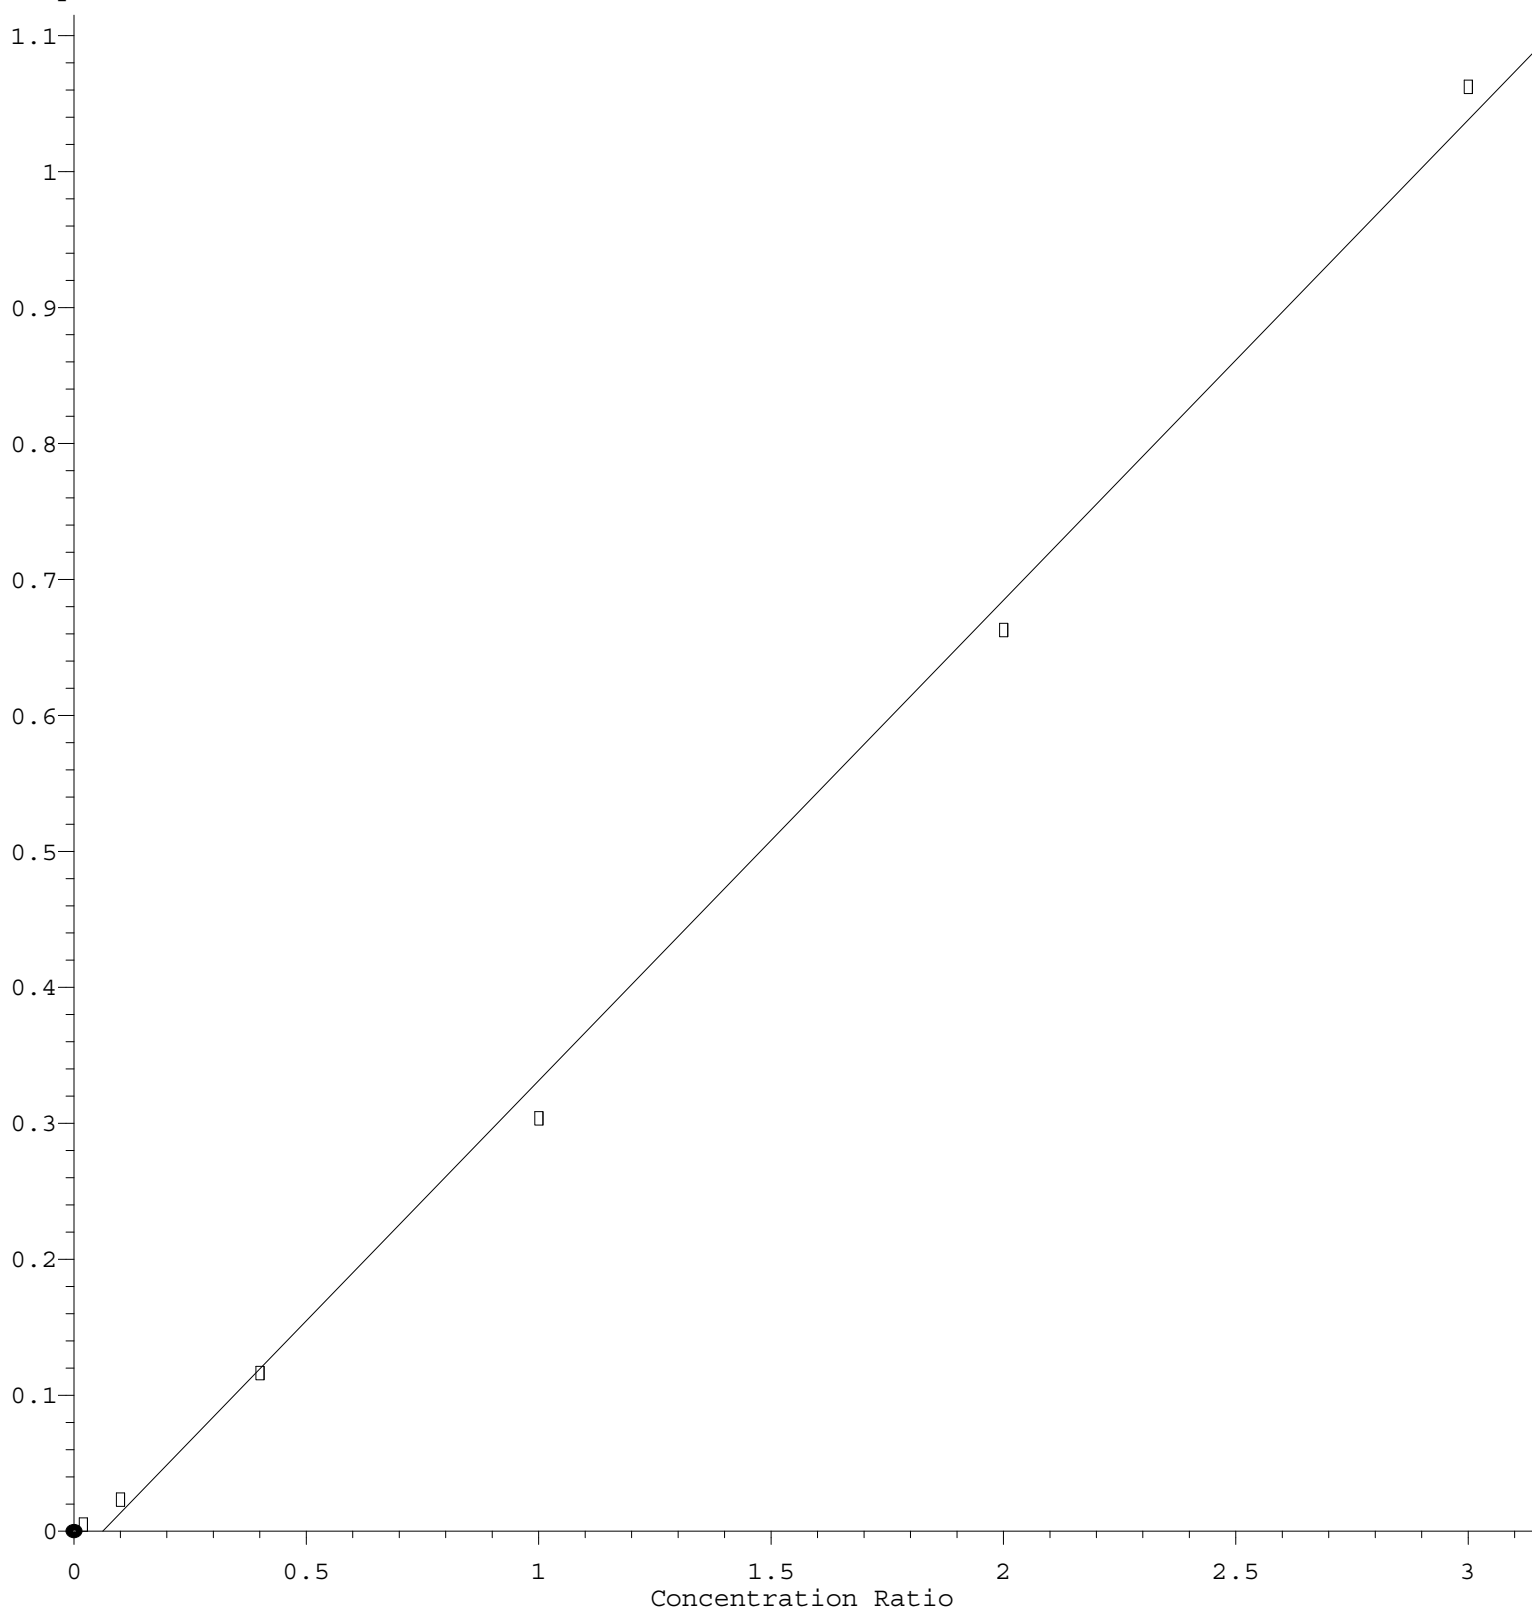

$$\text{Response} = 3.533\text{e-}001 * \text{Amt} - 2.181\text{e-}002$$


Coef of Det (r^2) = 0.997368 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U110521W.M

Calibration Table Last Updated: Fri Nov 05 13:35:16 2021

trans-1,4-Dichloro-2-butene

Response Ratio

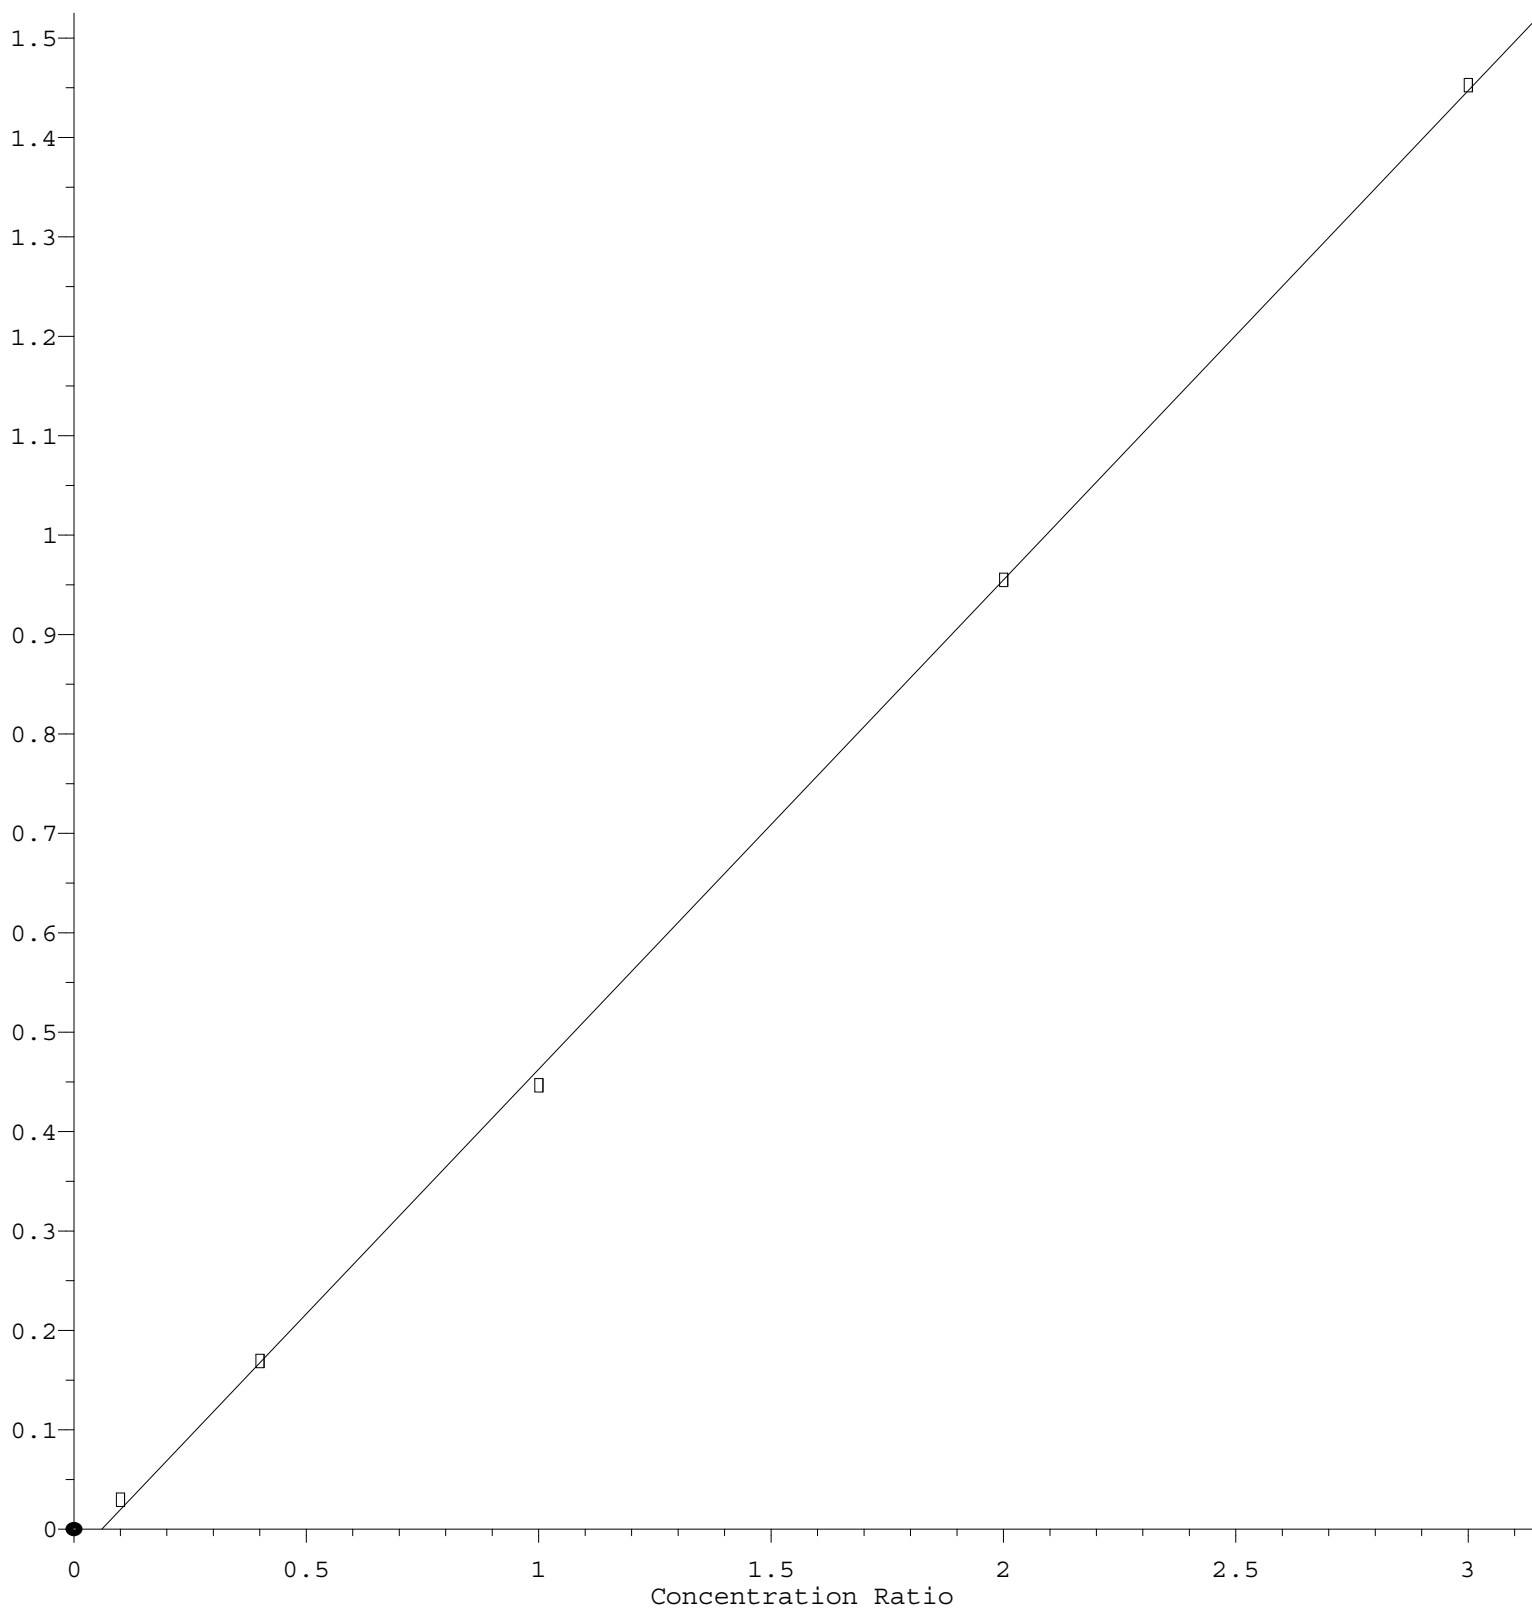

$$\text{Response} = 4.923\text{e-}001 * \text{Amt} - 2.946\text{e-}002$$


Coef of Det (r^2) = 0.999716 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U110521W.M

Calibration Table Last Updated: Fri Nov 05 13:35:16 2021

Naphthalene

Response Ratio

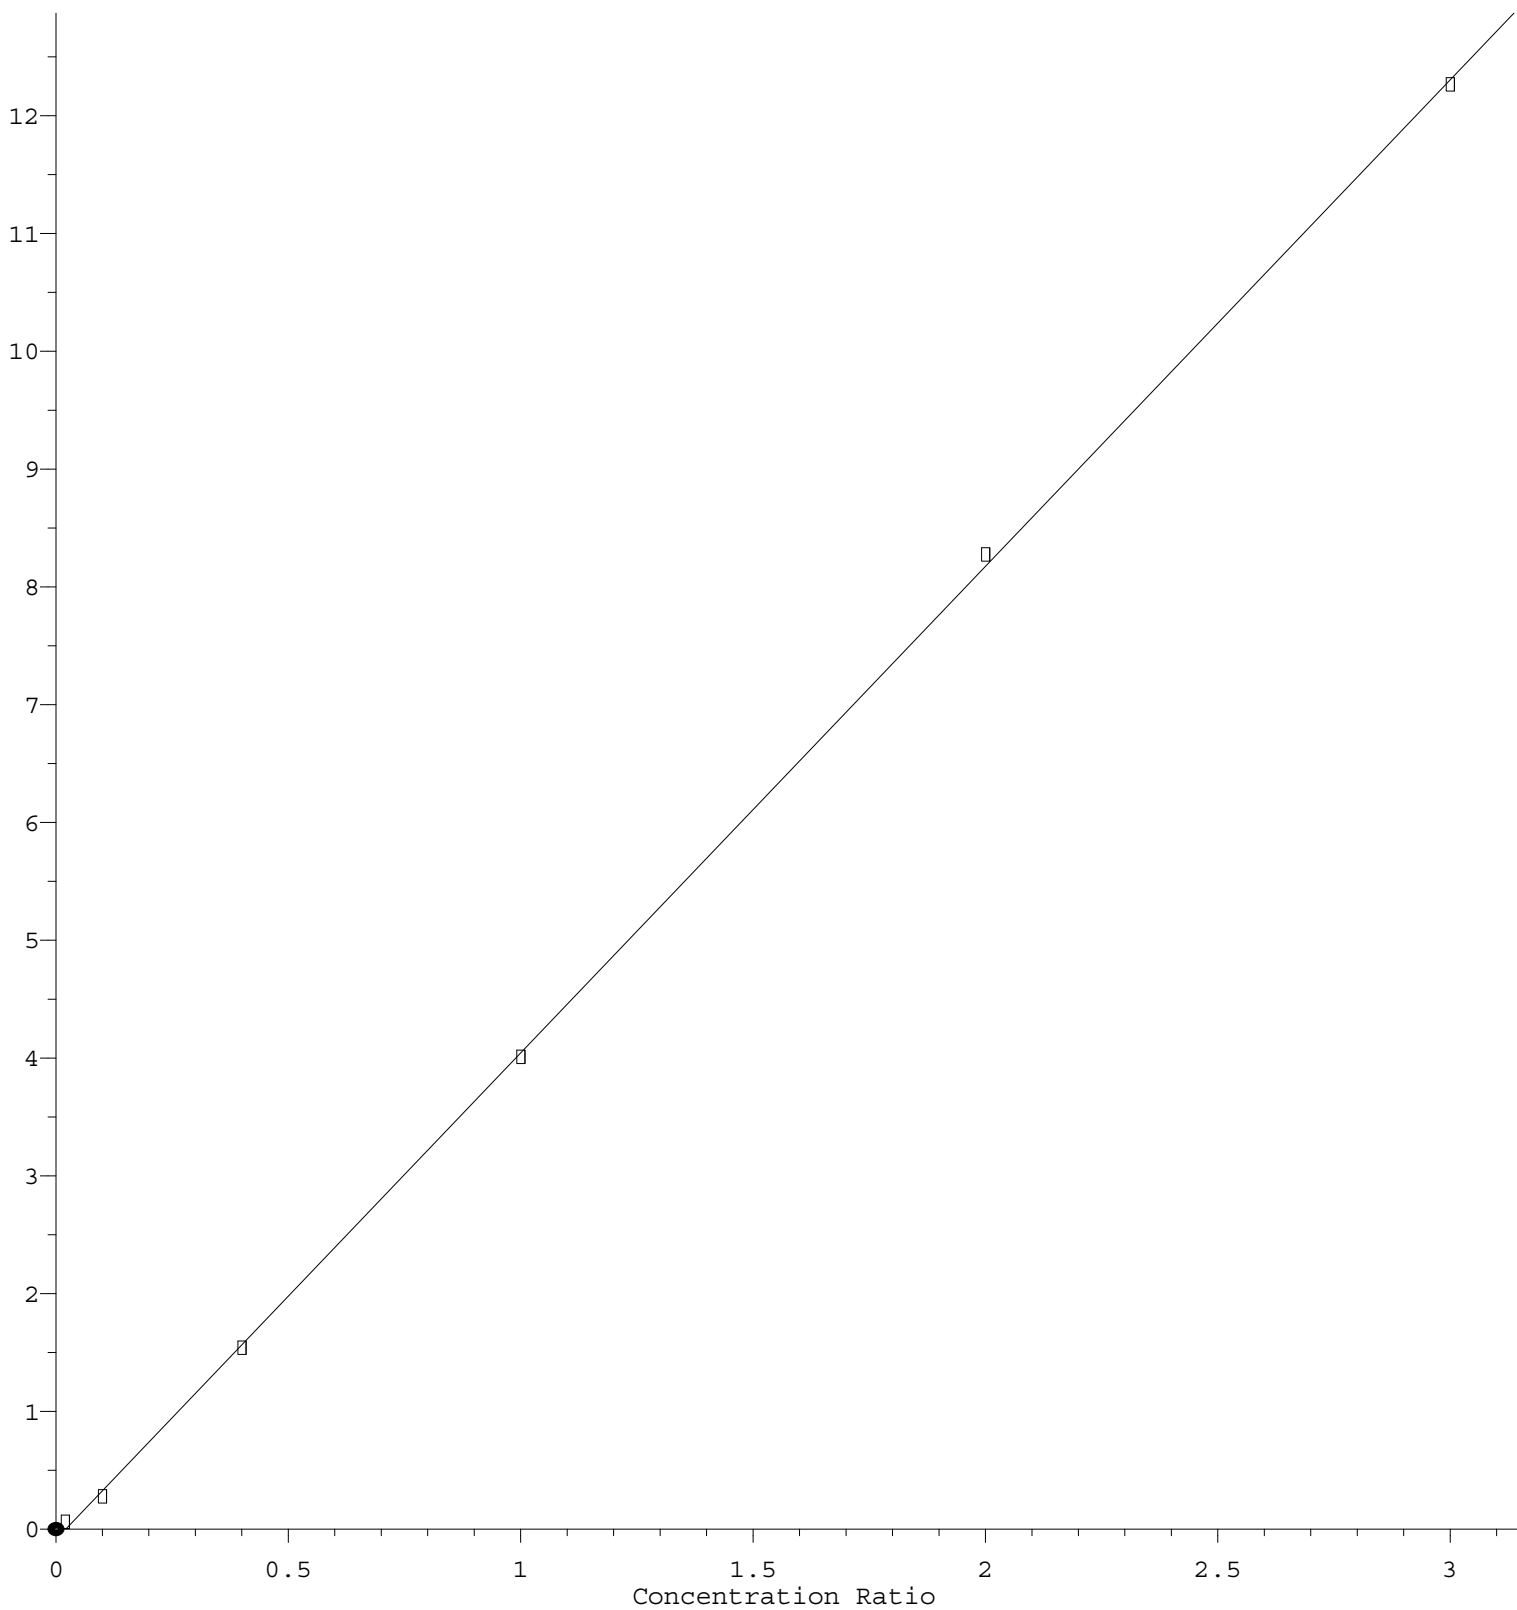

$$\text{Response} = 4.132\text{e}+000 * \text{Amt} - 8.503\text{e}-002$$

Coef of Det (r^2) = 0.999833 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U110521W.M

Calibration Table Last Updated: Fri Nov 05 13:35:16 2021