

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110521\
 Data File : VU045560.D
 Acq On : 05 Nov 2021 15:51
 Operator : SY/MD
 Sample : M4475-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TWP02

Quant Time: Nov 05 16:35:04 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 05 13:35:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.379	168	137657	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.253	114	258053	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.420	117	260561	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.812	152	129770	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.703	65	114922	55.745	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 111.480%	
35) Dibromofluoromethane	5.292	113	87417	50.739	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 101.480%	
50) Toluene-d8	7.899	98	338315	52.808	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 105.620%	
62) 4-Bromofluorobenzene	10.632	95	129150	50.273	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 100.540%	
Target Compounds						
					Qvalue	
16) Acetone	2.626	43	7253	6.911	ug/l	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110521\
Data File : VU045560.D
Acq On : 05 Nov 2021 15:51
Operator : SY/MD
Sample : M4475-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TWP02

Quant Time: Nov 05 16:35:04 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 05 13:35:16 2021
Response via : Initial Calibration




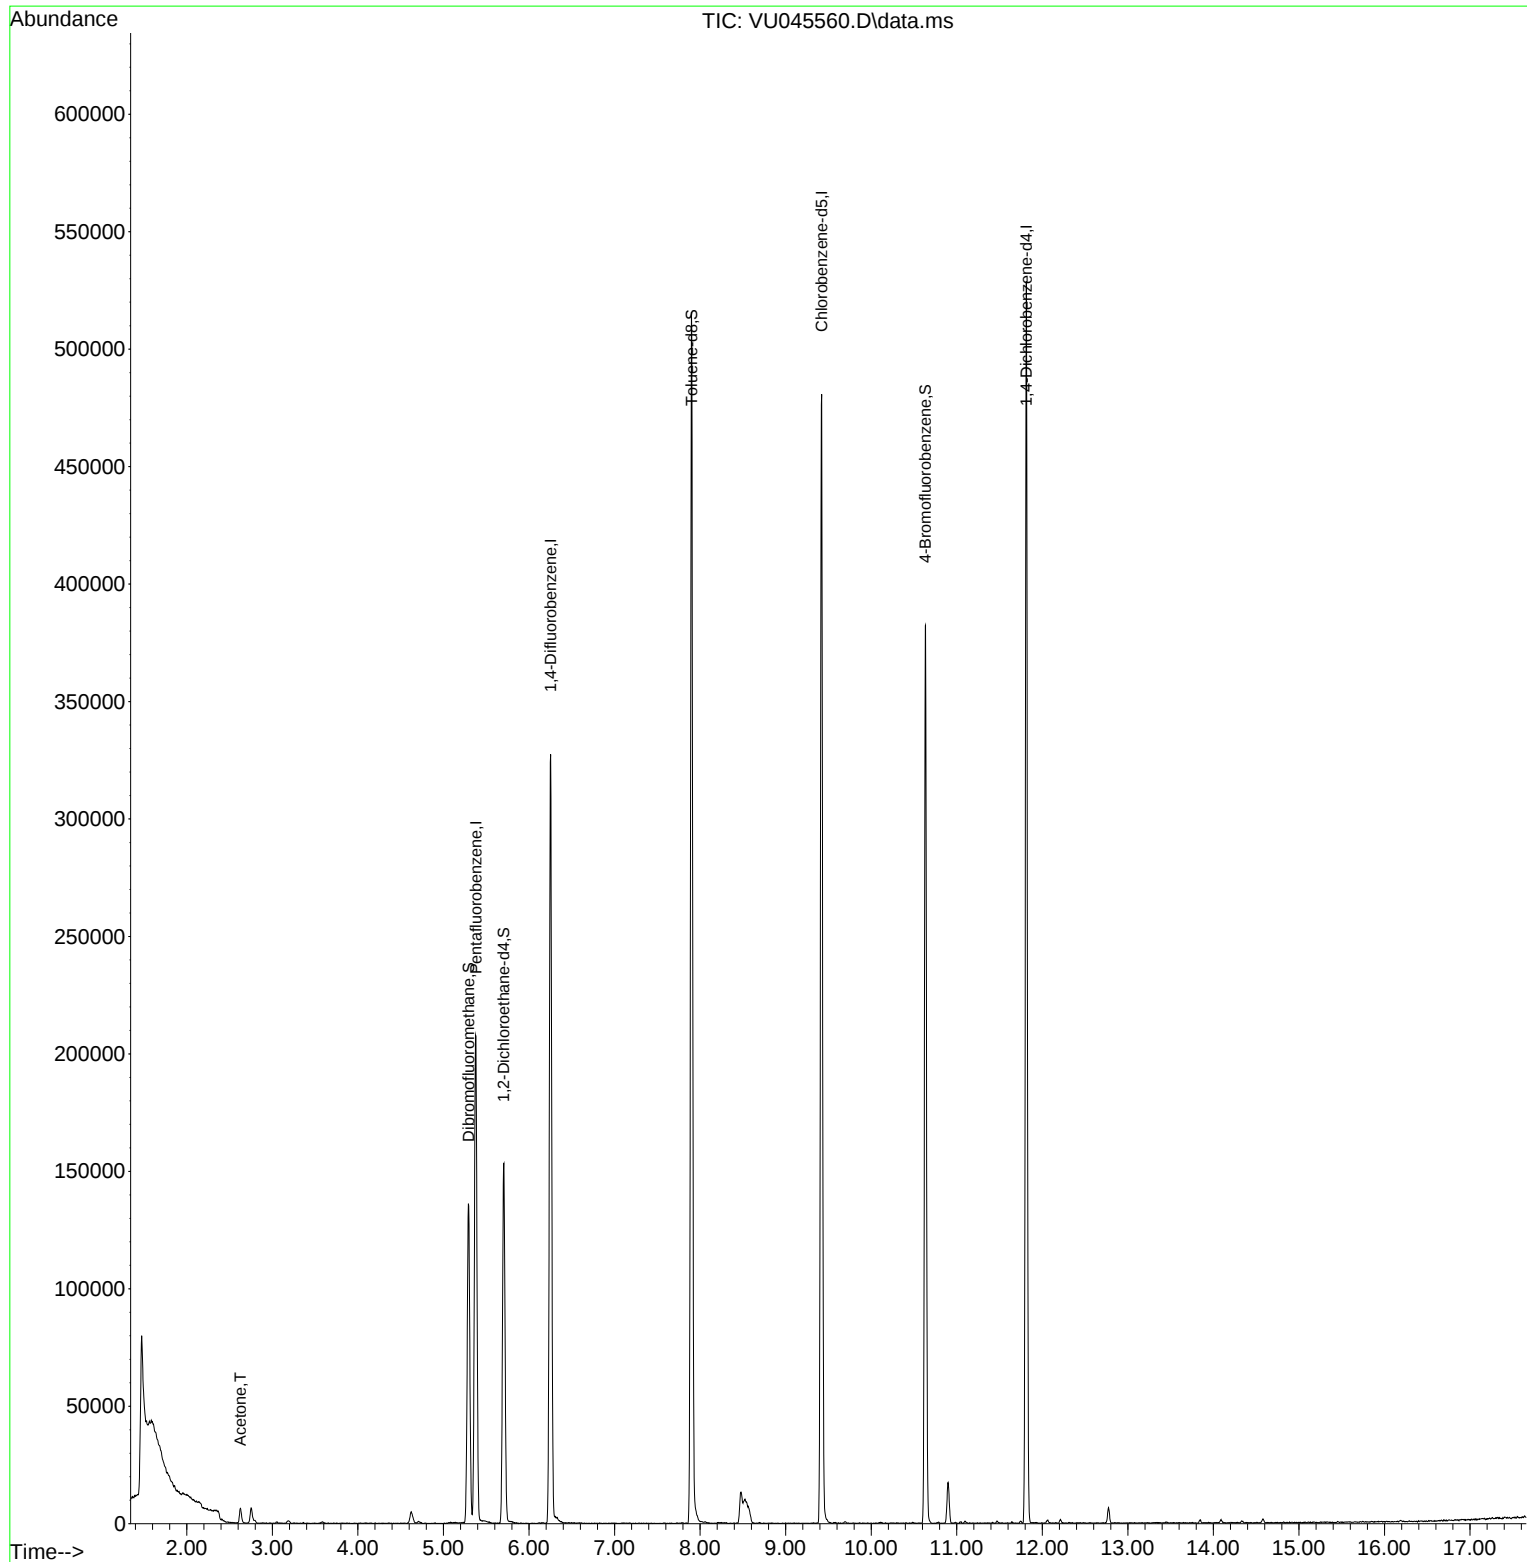




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.379 min Scan# 11
Delta R.T. 0.004 min
Lab File: VU045560.D
Acq: 05 Nov 2021 15:51




Instrument :
MSVOA_U
ClientSampleId :
TWP02


Tgt Ion:168 Resp: 137657
Ion Ratio Lower Upper
168 100
99 65.9 51.0 76.6

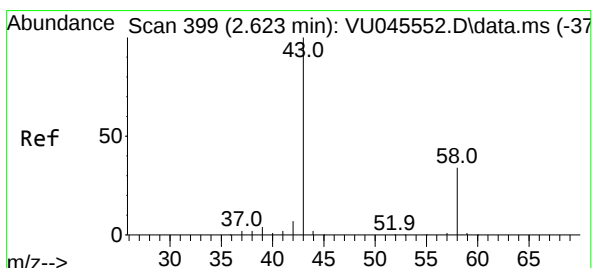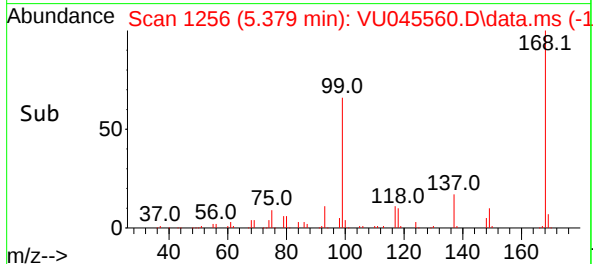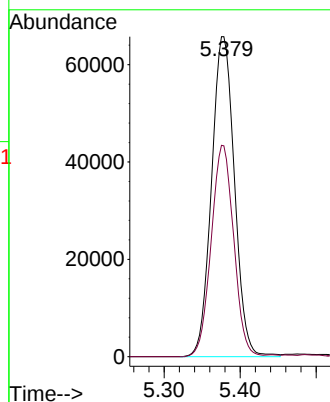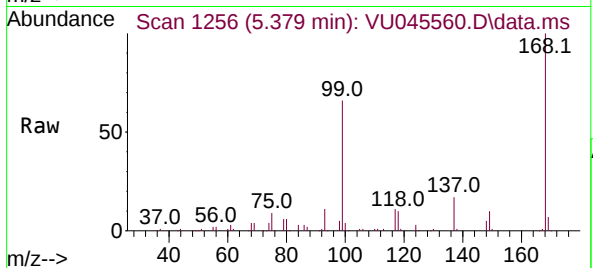

#16
Acetone
Concen: 6.911 ug/l
RT: 2.626 min Scan# 400
Delta R.T. 0.003 min
Lab File: VU045560.D
Acq: 05 Nov 2021 15:51

Tgt Ion: 43 Resp: 7253
Ion Ratio Lower Upper
43 100
58 32.9 26.2 39.2

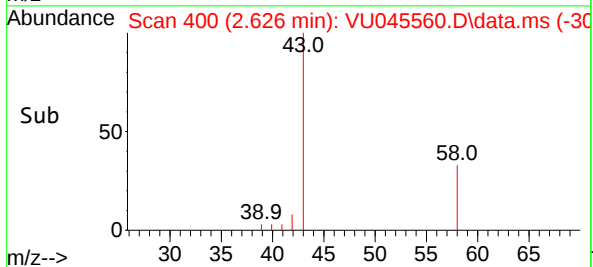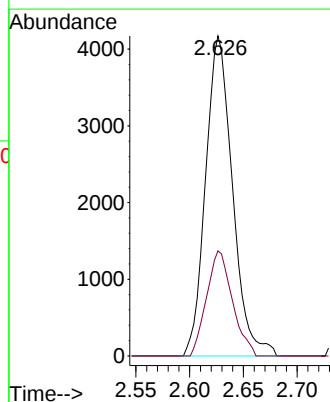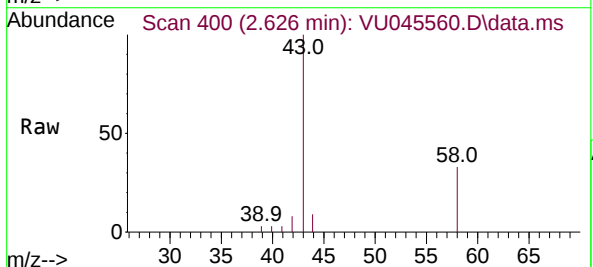

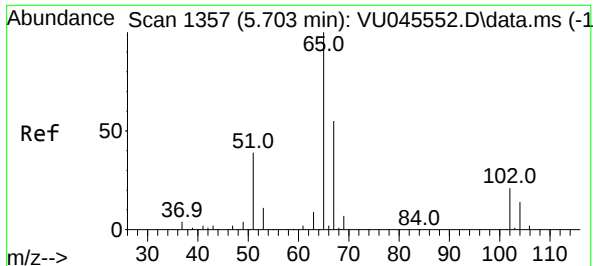

#33

1,2-Dichloroethane-d4

Concen: 55.745 ug/l

RT: 5.703 min Scan# 11

Delta R.T. 0.000 min

Lab File: VU045560.D

Acq: 05 Nov 2021 15:51

Instrument :

MSVOA_U

ClientSampleId :





TWP02

Tgt Ion: 65 Resp: 114922

Ion Ratio Lower Upper

65 100

67 52.0 0.0 105.8

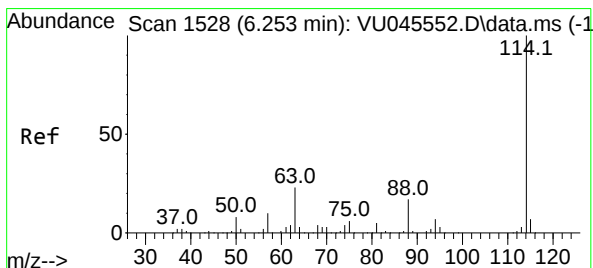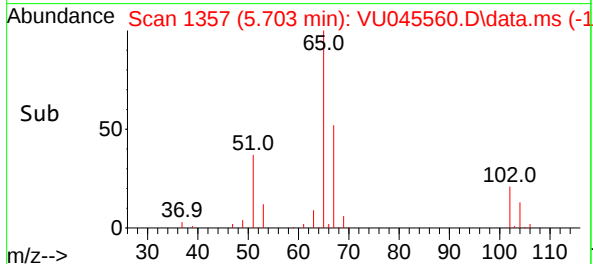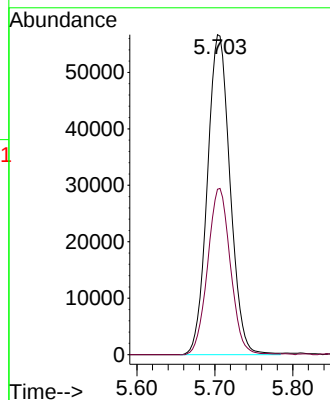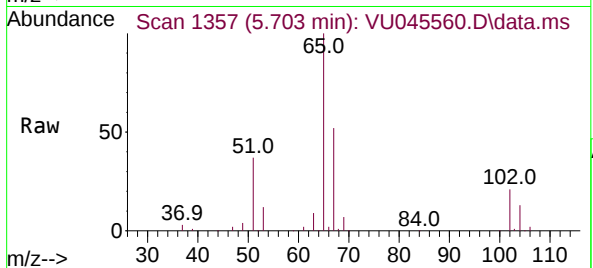

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.253 min Scan# 1528

Delta R.T. 0.000 min

Lab File: VU045560.D

Acq: 05 Nov 2021 15:51




Tgt Ion: 114 Resp: 258053


Ion Ratio Lower Upper

114 100

63 21.5 0.0 45.6

88 17.5 0.0 33.8

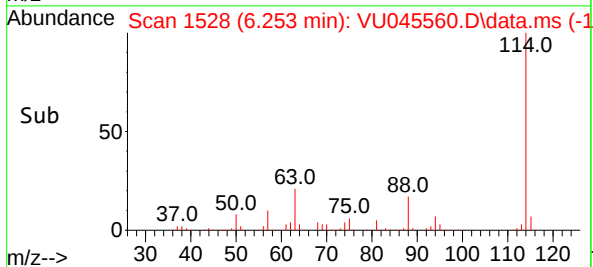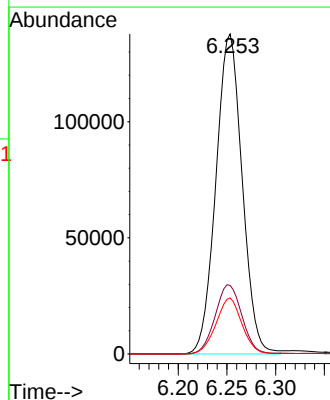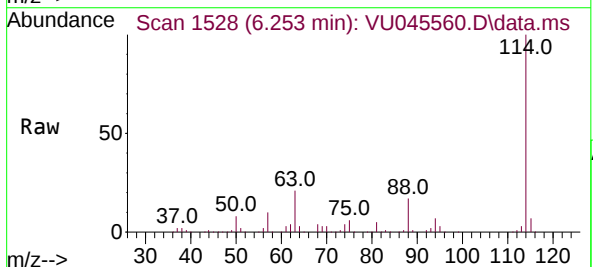

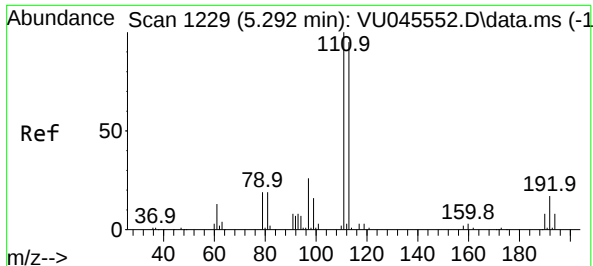

#35

Dibromofluoromethane

Concen: 50.739 ug/l

RT: 5.292 min Scan# 11

Delta R.T. 0.000 min

Lab File: VU045560.D

Acq: 05 Nov 2021 15:51

Instrument :

MSVOA_U

ClientSampleId :

TWP02





Tgt Ion:113 Resp: 87417

Ion Ratio Lower Upper

113 100

111 102.9 82.8 124.2

192 18.2 14.8 22.2

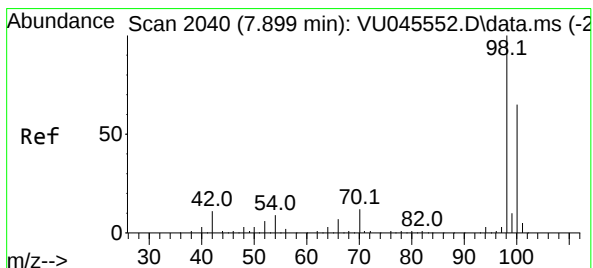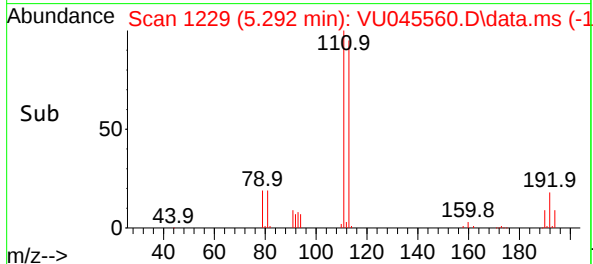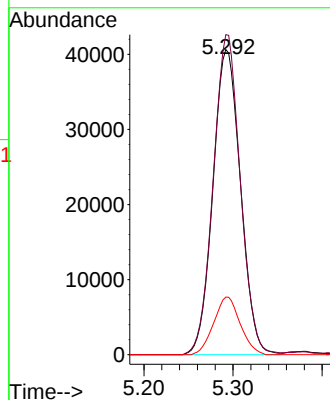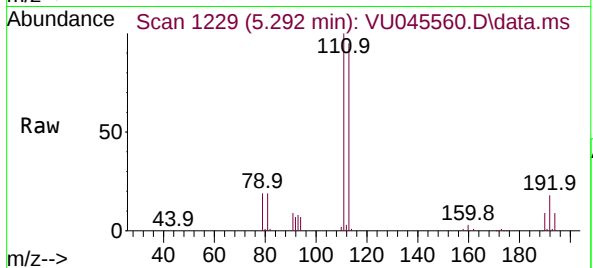

#50

Toluene-d8

Concen: 52.808 ug/l

RT: 7.899 min Scan# 2040

Delta R.T. 0.000 min

Lab File: VU045560.D




Acq: 05 Nov 2021 15:51


Tgt Ion: 98 Resp: 338315

Ion Ratio Lower Upper

98 100

100 66.4 52.5 78.7


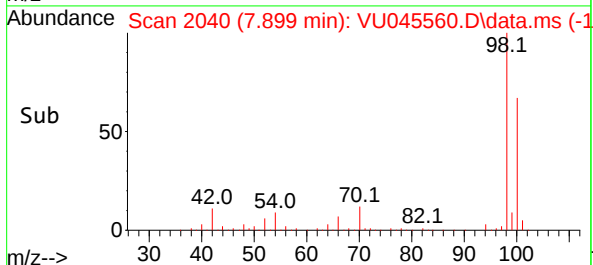
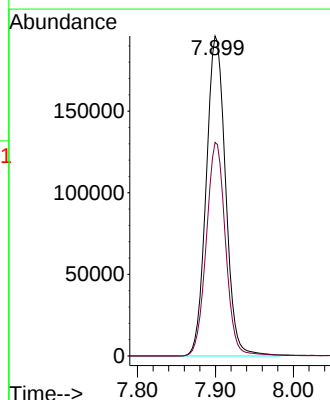
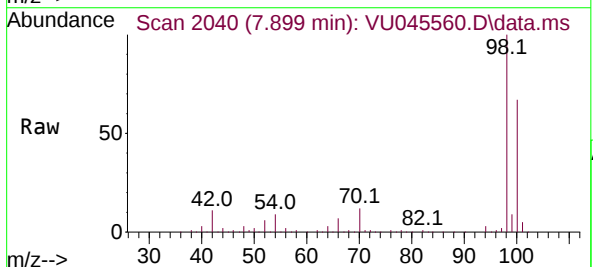


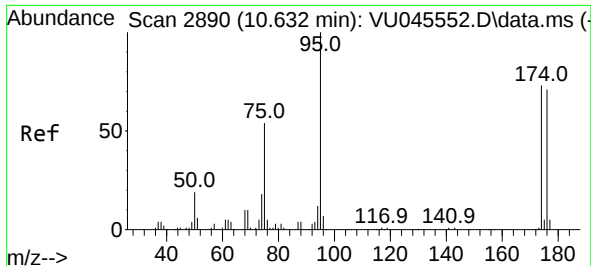

#62
4-Bromofluorobenzene
Concen: 50.273 ug/l
RT: 10.632 min Scan# 2890
Delta R.T. 0.000 min
Lab File: VU045560.D
Acq: 05 Nov 2021 15:51




Instrument :
MSVOA_U
ClientSampleId :
TWP02


Tgt Ion: 95 Resp: 129150
Ion Ratio Lower Upper
95 100
174 73.4 0.0 141.8
176 70.8 0.0 138.2

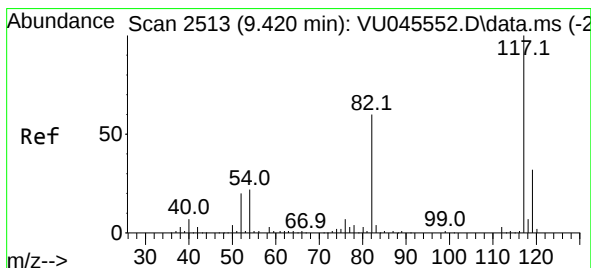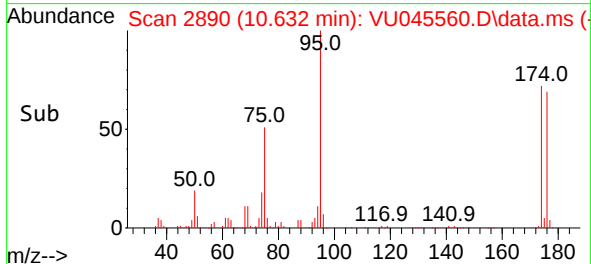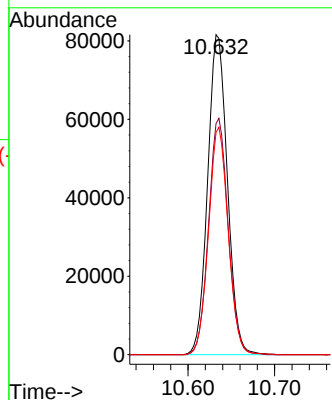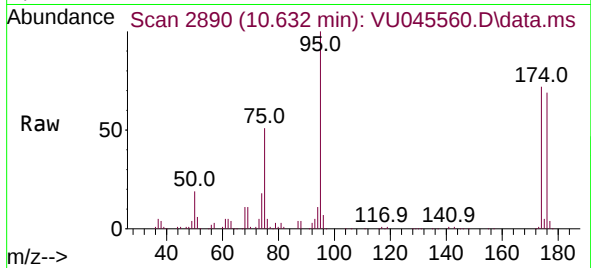

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.420 min Scan# 2513
Delta R.T. 0.000 min
Lab File: VU045560.D
Acq: 05 Nov 2021 15:51

Tgt Ion: 117 Resp: 260561
Ion Ratio Lower Upper
117 100
82 58.6 47.8 71.8
119 32.6 25.8 38.8

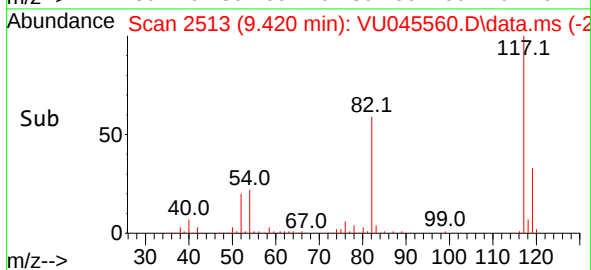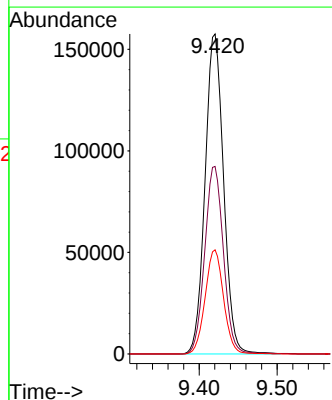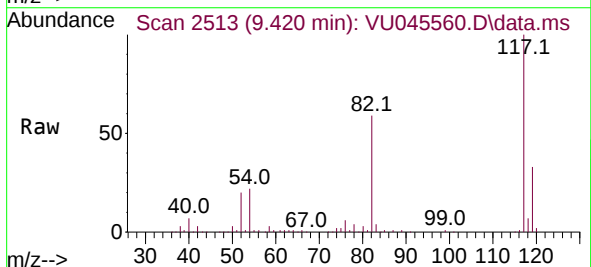

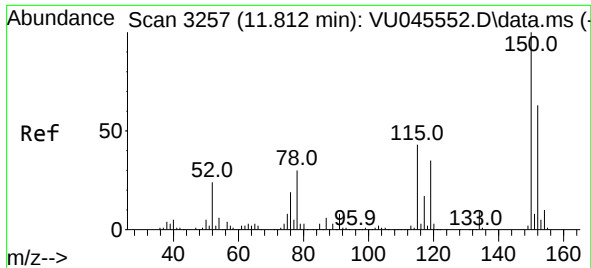

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 11.812 min Scan# 31

Delta R.T. 0.000 min

Lab File: VU045560.D


Acq: 05 Nov 2021 15:51

Instrument :

MSVOA_U

ClientSampleId :

TWP02

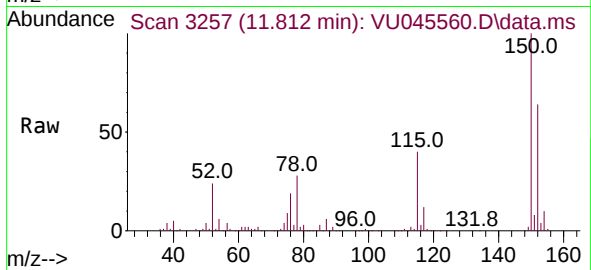

Tgt Ion:152 Resp: 129770

Ion Ratio Lower Upper

152 100

115 62.6 42.7 128.1

150 156.0 0.0 346.8

