

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110521\
 Data File : VU045565.D
 Acq On : 05 Nov 2021 17:43
 Operator : SY/MD
 Sample : M4475-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 FB01

Quant Time: Nov 05 18:31:34 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 05 13:35:16 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.379	168	135290	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.253	114	258645	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.420	117	258449	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.816	152	129472	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.706	65	114817	56.668	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	113.340%
35) Dibromofluoromethane	5.292	113	88250	51.105	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	102.220%
50) Toluene-d8	7.899	98	337860	52.616	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	105.240%
62) 4-Bromofluorobenzene	10.636	95	128582	49.937	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	99.880%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110521\
Data File : VU045565.D
Acq On : 05 Nov 2021 17:43
Operator : SY/MD
Sample : M4475-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
FB01

Quant Time: Nov 05 18:31:34 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 05 13:35:16 2021
Response via : Initial Calibration




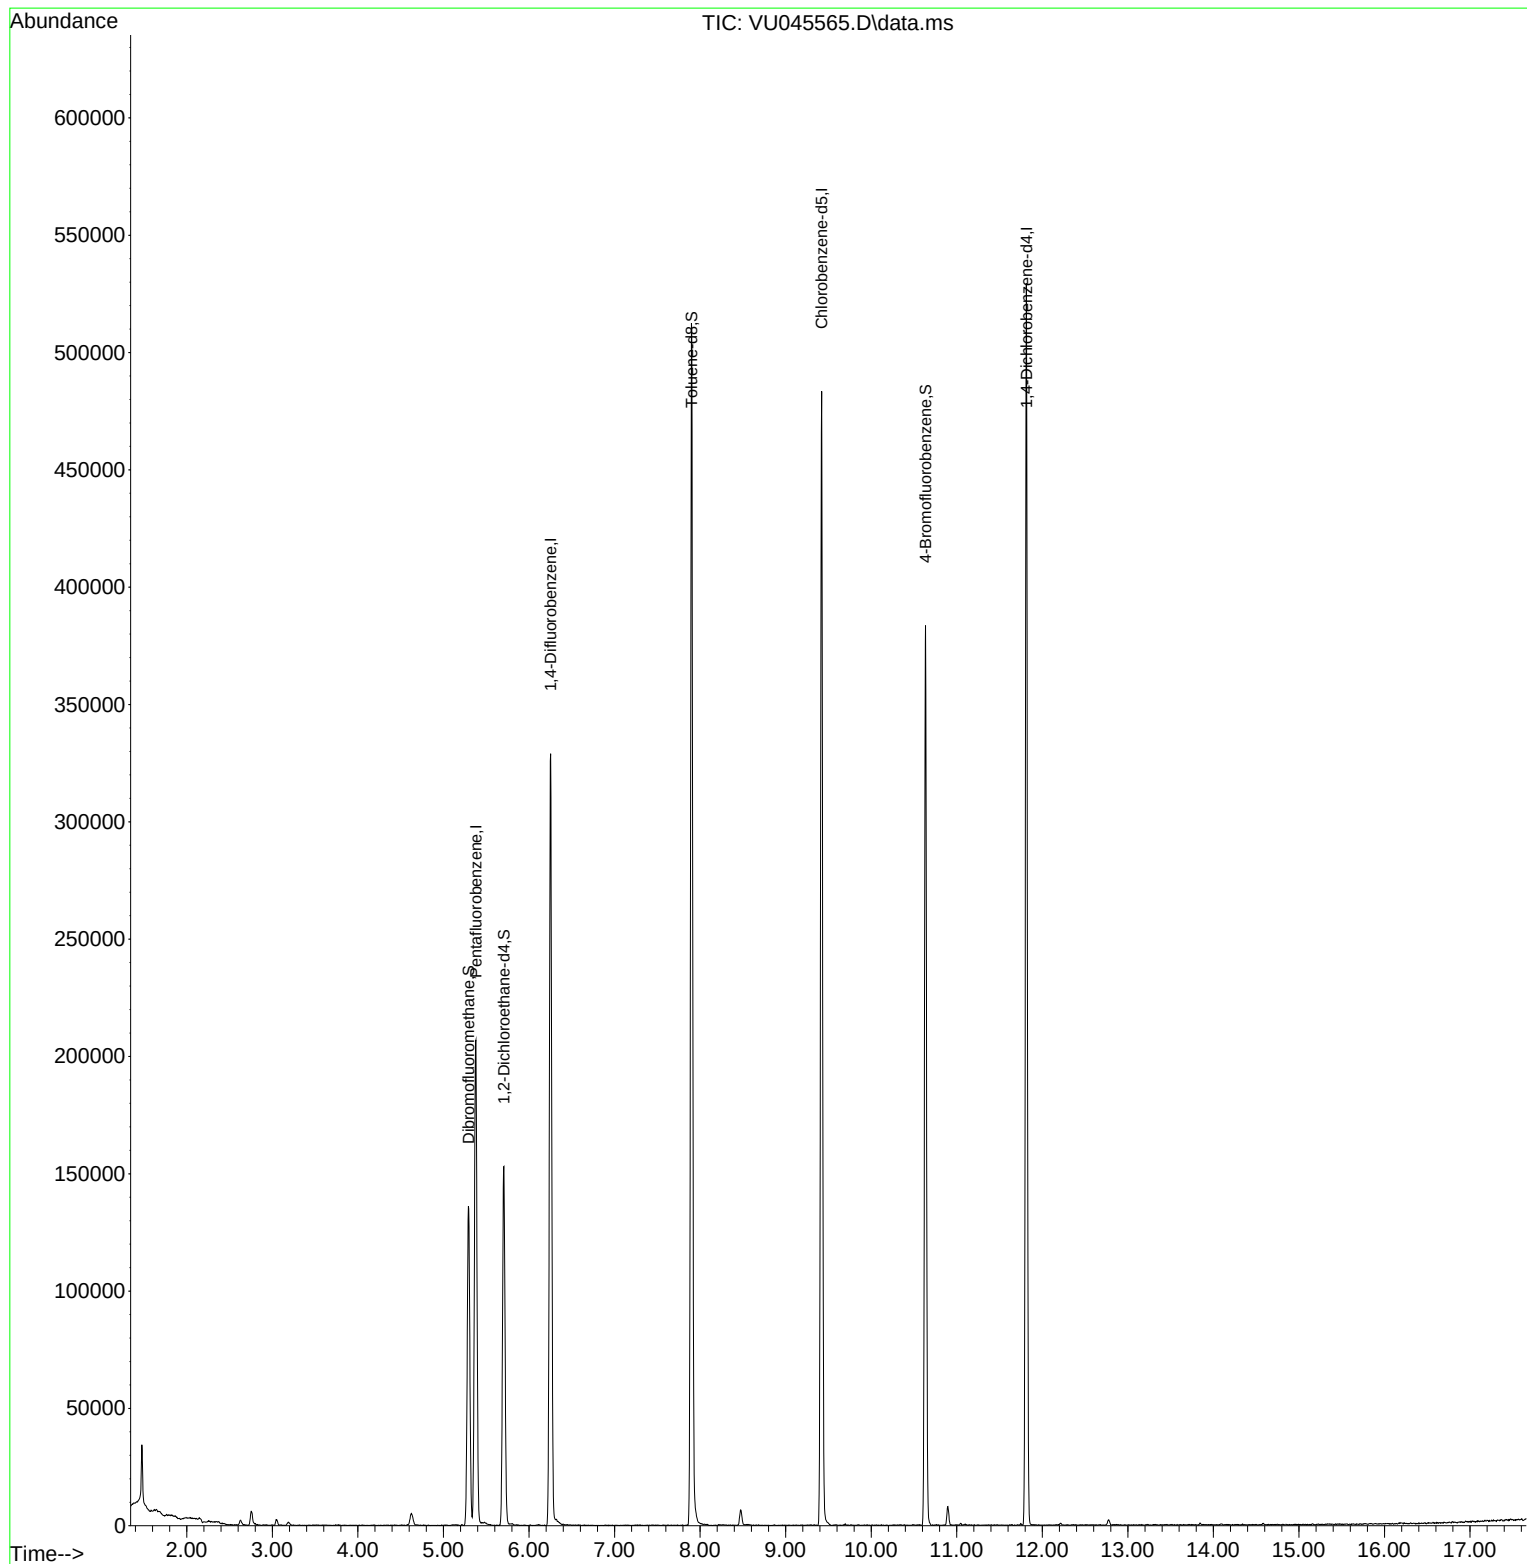


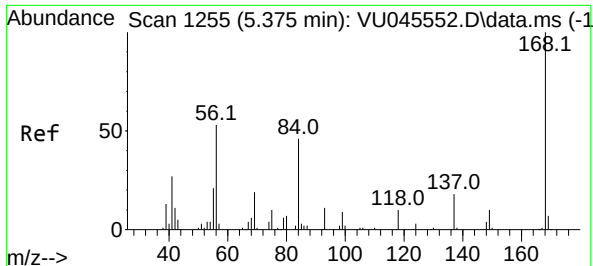

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.379 min Scan# 11
Delta R.T. 0.004 min
Lab File: VU045565.D
Acq: 05 Nov 2021 17:43




Instrument :
MSVOA_U
ClientSampleId :
FB01


Tgt Ion:168 Resp: 135290
Ion Ratio Lower Upper
168 100
99 65.4 51.0 76.6

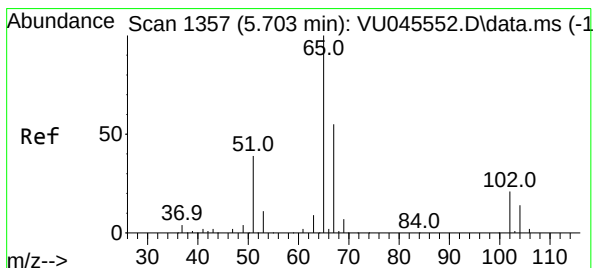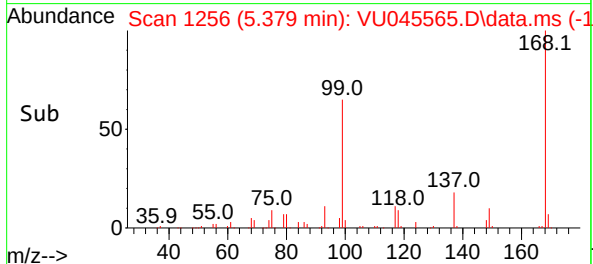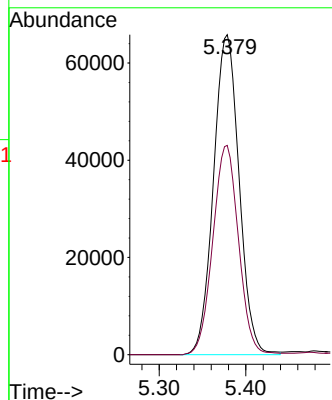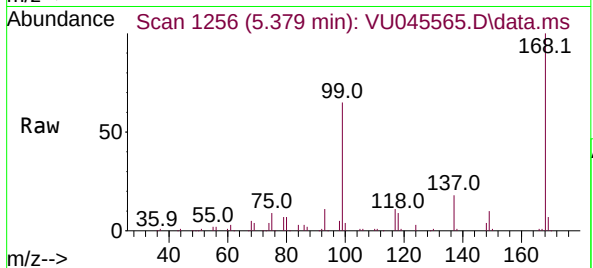

#33
1,2-Dichloroethane-d4
Concen: 56.668 ug/l
RT: 5.706 min Scan# 1358
Delta R.T. 0.003 min
Lab File: VU045565.D
Acq: 05 Nov 2021 17:43

Tgt Ion: 65 Resp: 114817
Ion Ratio Lower Upper
65 100
67 52.4 0.0 105.8

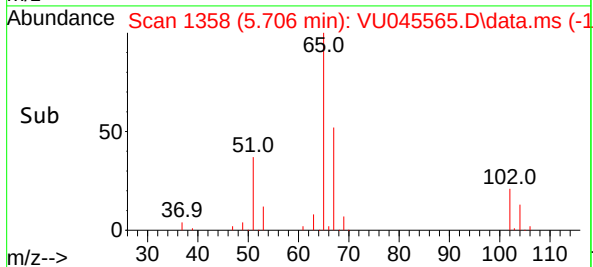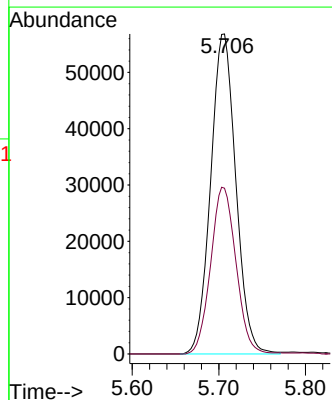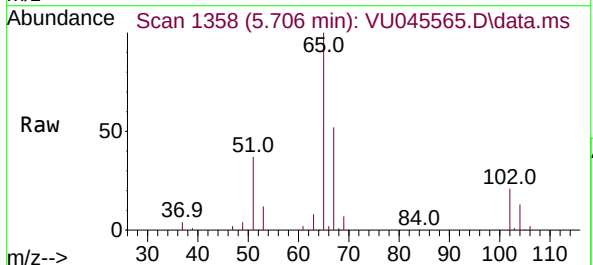

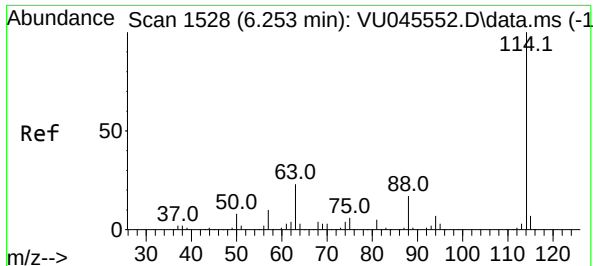

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.253 min Scan# 1

Delta R.T. 0.000 min

Lab File: VU045565.D

Acq: 05 Nov 2021 17:43

Instrument :

MSVOA_U

ClientSampleId :

FB01





Tgt Ion:114 Resp: 258645

Ion Ratio Lower Upper

114 100

63 23.1 0.0 45.6

88 17.2 0.0 33.8

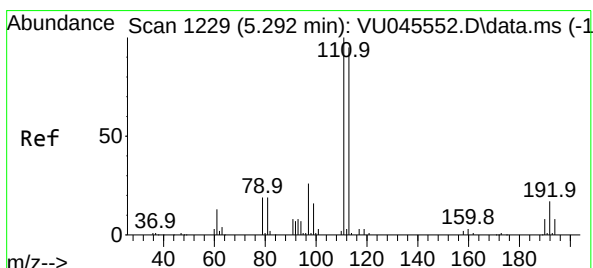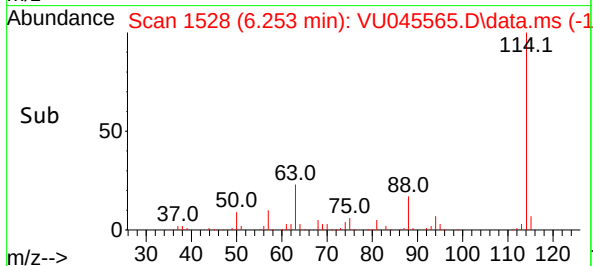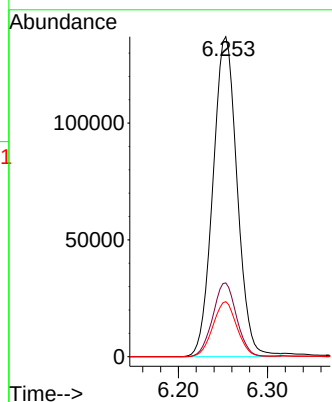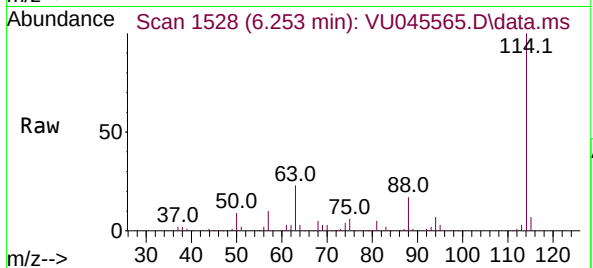

#35

Dibromofluoromethane

Concen: 51.105 ug/l

RT: 5.292 min Scan# 1229

Delta R.T. 0.000 min

Lab File: VU045565.D

Acq: 05 Nov 2021 17:43




Tgt Ion:113 Resp: 88250


Ion Ratio Lower Upper

113 100

111 102.6 82.8 124.2

192 18.0 14.8 22.2


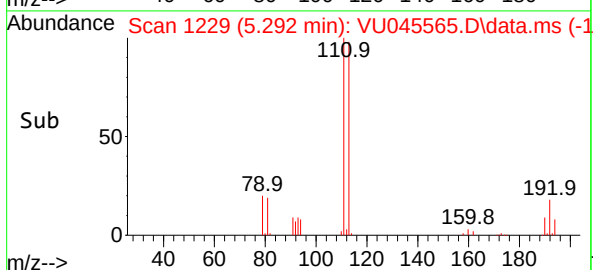
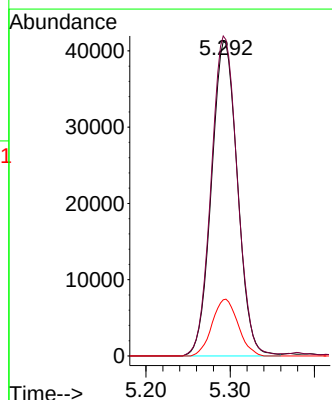
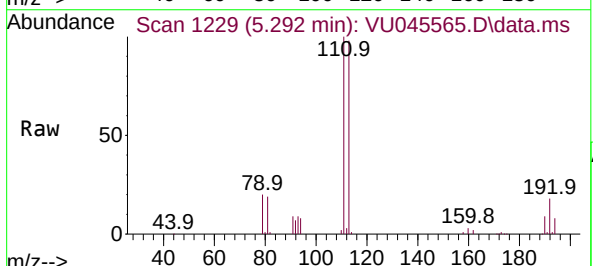


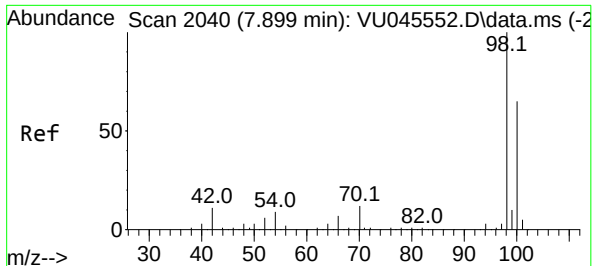

#50
Toluene-d8
Concen: 52.616 ug/l
RT: 7.899 min Scan# 2040
Delta R.T. 0.000 min
Lab File: VU045565.D
Acq: 05 Nov 2021 17:43




Instrument :
MSVOA_U
ClientSampleId :
FB01


Tgt Ion: 98 Resp: 337860
Ion Ratio Lower Upper
98 100
100 66.0 52.5 78.7

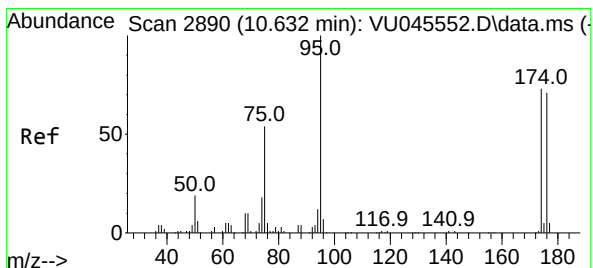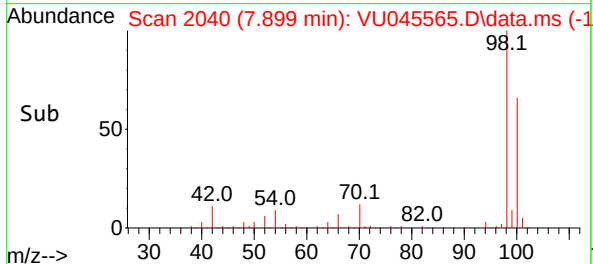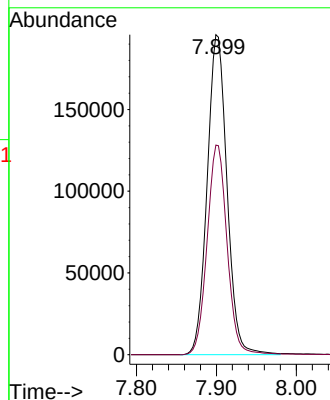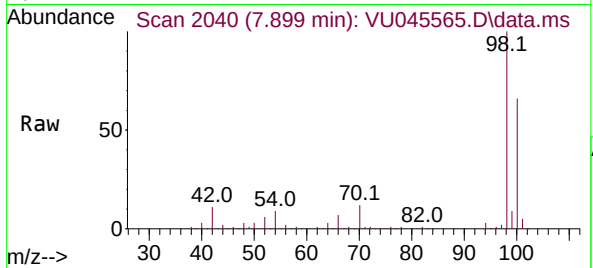

#62
4-Bromofluorobenzene
Concen: 49.937 ug/l
RT: 10.636 min Scan# 2891
Delta R.T. 0.003 min
Lab File: VU045565.D
Acq: 05 Nov 2021 17:43

Tgt Ion: 95 Resp: 128582
Ion Ratio Lower Upper
95 100
174 73.3 0.0 141.8
176 70.3 0.0 138.2


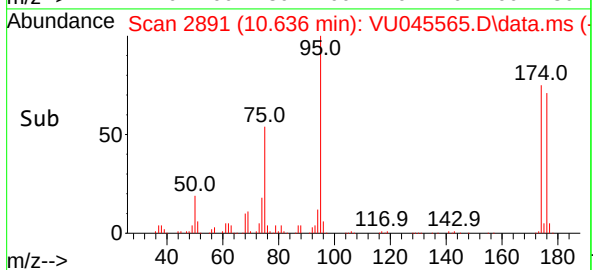
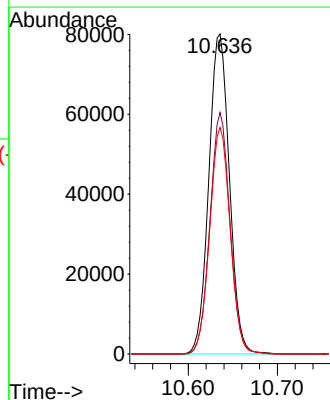
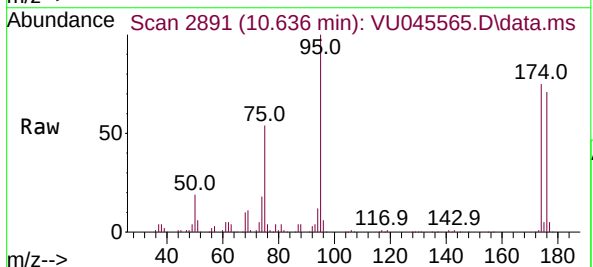


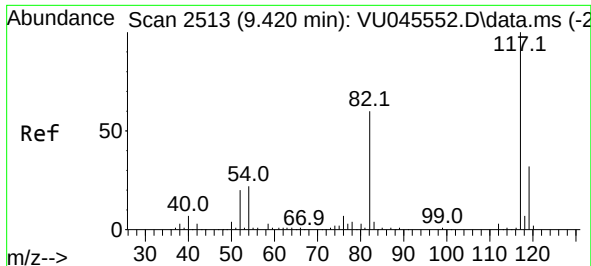

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.420 min Scan# 21
Delta R.T. 0.000 min
Lab File: VU045565.D
Acq: 05 Nov 2021 17:43

Instrument :
MSVOA_U
ClientSampleId :
FB01

Tgt Ion:117 Resp: 258449
Ion Ratio Lower Upper
117 100
82 58.0 47.8 71.8
119 32.1 25.8 38.8

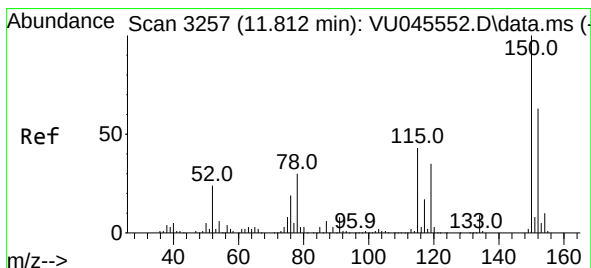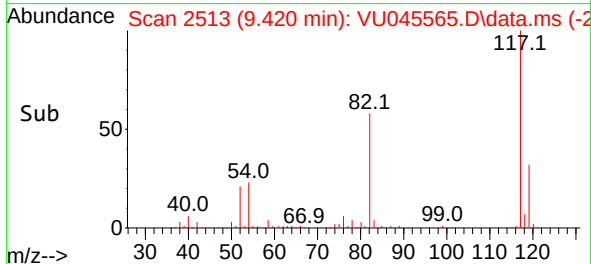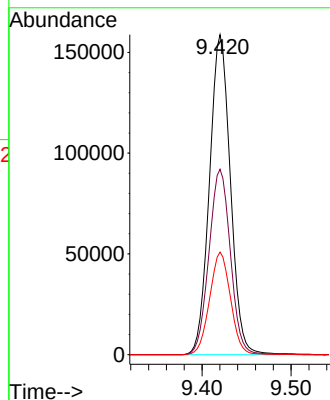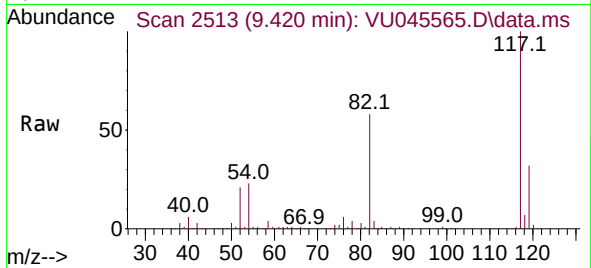

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.816 min Scan# 3258
Delta R.T. 0.003 min
Lab File: VU045565.D
Acq: 05 Nov 2021 17:43

Tgt Ion:152 Resp: 129472
Ion Ratio Lower Upper
152 100
115 62.9 42.7 128.1
150 157.4 0.0 346.8

