

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU110521\  
 Data File : VU045565.D  
 Acq On : 05 Nov 2021 17:43  
 Operator : SY/MD  
 Sample : M4475-14  
 Misc : 5.0mL/MSVOA\_U/WATER  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 FB01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U110521W.M  
 Title : SW846 8260

Signal : TIC: VU045565.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.475       | 37            | 42          | 73           | rVB      | 28409          | 41666         | 4.69%           | 0.861%        |
| 2         | 2.752       | 430           | 439         | 452          | rBV      | 5892           | 11274         | 1.27%           | 0.233%        |
| 3         | 4.626       | 1009          | 1022        | 1038         | rVB      | 4951           | 11829         | 1.33%           | 0.244%        |
| 4         | 5.292       | 1213          | 1229        | 1243         | rBV      | 136042         | 289677        | 32.59%          | 5.986%        |
| 5         | 5.379       | 1243          | 1256        | 1275         | rVB      | 206036         | 421555        | 47.43%          | 8.712%        |
| 6         | 5.706       | 1343          | 1358        | 1377         | rBV      | 152990         | 310346        | 34.92%          | 6.414%        |
| 7         | 6.253       | 1512          | 1528        | 1547         | rBV      | 328926         | 617895        | 69.53%          | 12.769%       |
| 8         | 7.899       | 2027          | 2040        | 2067         | rBV      | 512222         | 888731        | 100.00%         | 18.367%       |
| 9         | 8.475       | 2207          | 2219        | 2232         | rBV3     | 6580           | 12438         | 1.40%           | 0.257%        |
| 10        | 9.420       | 2499          | 2513        | 2547         | rBV      | 483300         | 792123        | 89.13%          | 16.370%       |
| 11        | 10.636      | 2878          | 2891        | 2912         | rBV      | 383429         | 605893        | 68.18%          | 12.521%       |
| 12        | 10.896      | 2958          | 2972        | 2982         | rBV      | 7979           | 12947         | 1.46%           | 0.268%        |
| 13        | 11.812      | 3244          | 3257        | 3274         | rBV      | 529139         | 822464        | 92.54%          | 16.997%       |




Sum of corrected areas: 4838838

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU110521\  
Data File : VU045565.D  
Acq On : 05 Nov 2021 17:43  
Operator : SY/MD  
Sample : M4475-14  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
FB01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U110521W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

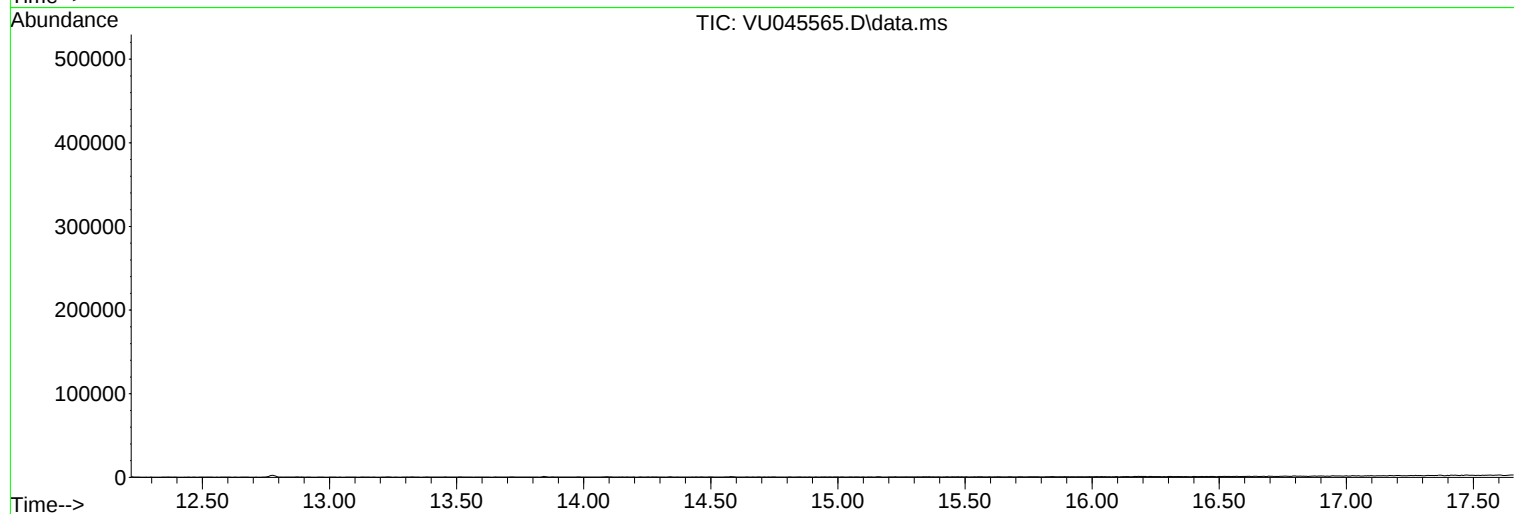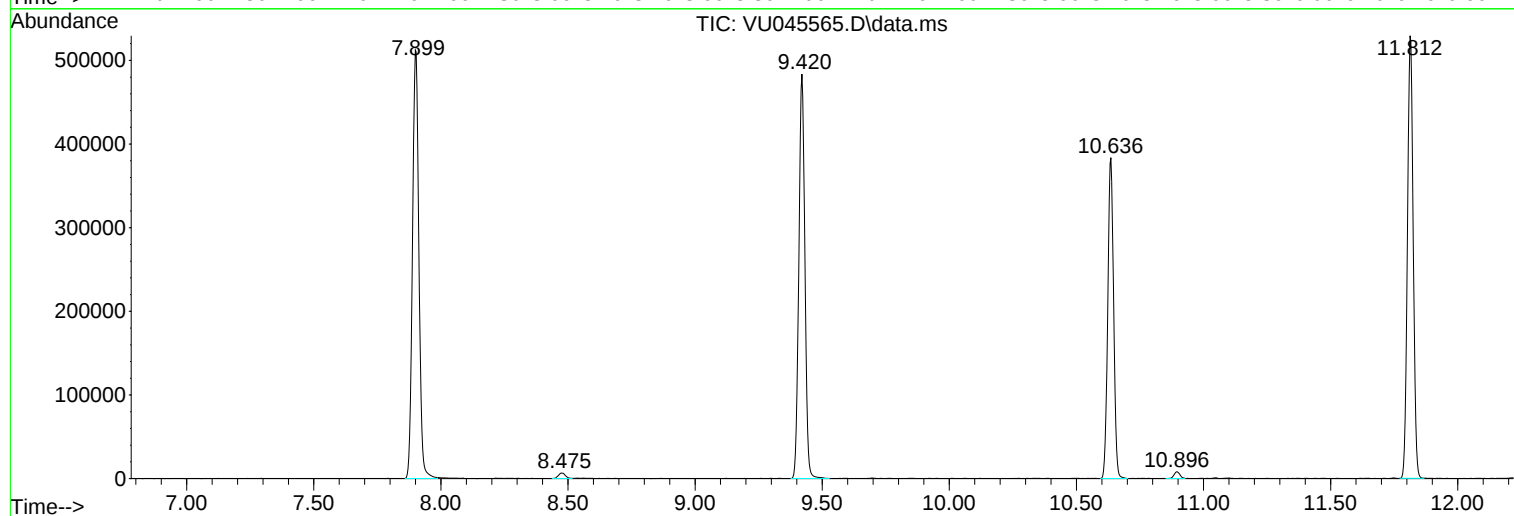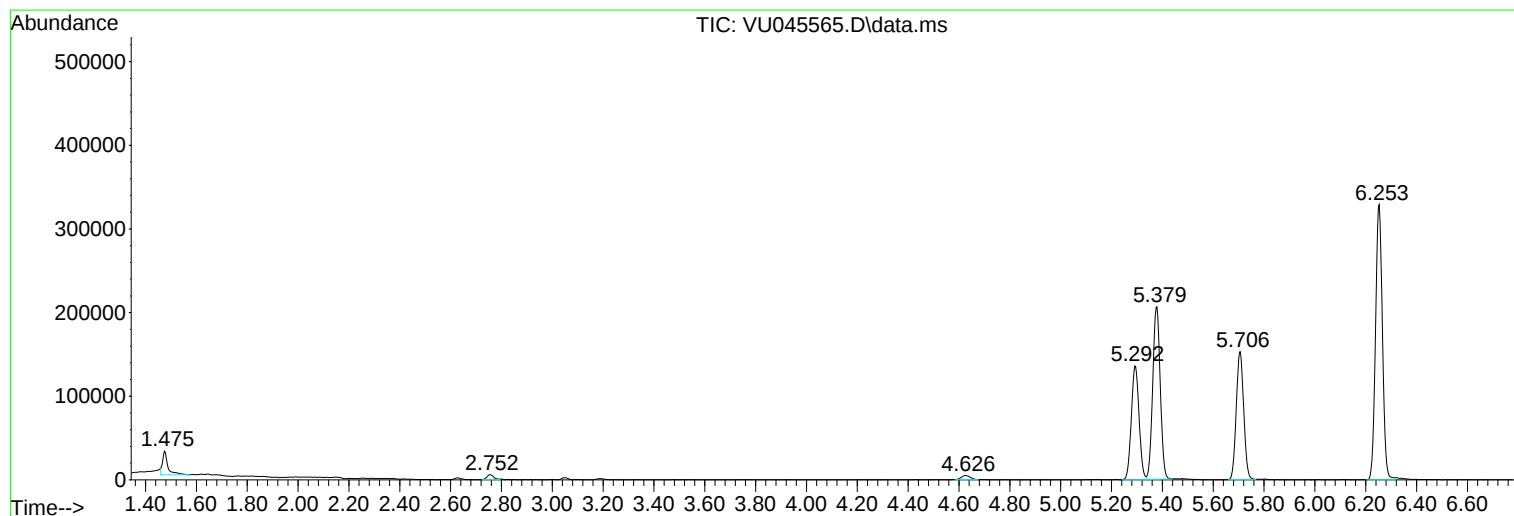

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU110521\  
Data File : VU045565.D  
Acq On : 05 Nov 2021 17:43  
Operator : SY/MD  
Sample : M4475-14  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
FB01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U110521W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU110521\  
Data File : VU045565.D  
Acq On : 05 Nov 2021 17:43  
Operator : SY/MD  
Sample : M4475-14  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
FB01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U110521W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|