


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110521\
 Data File : VU045548.D
 Acq On : 05 Nov 2021 09:56
 Operator : SY/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
 Title : SW846 8260
 Last Update : Fri Nov 05 13:35:16 2021

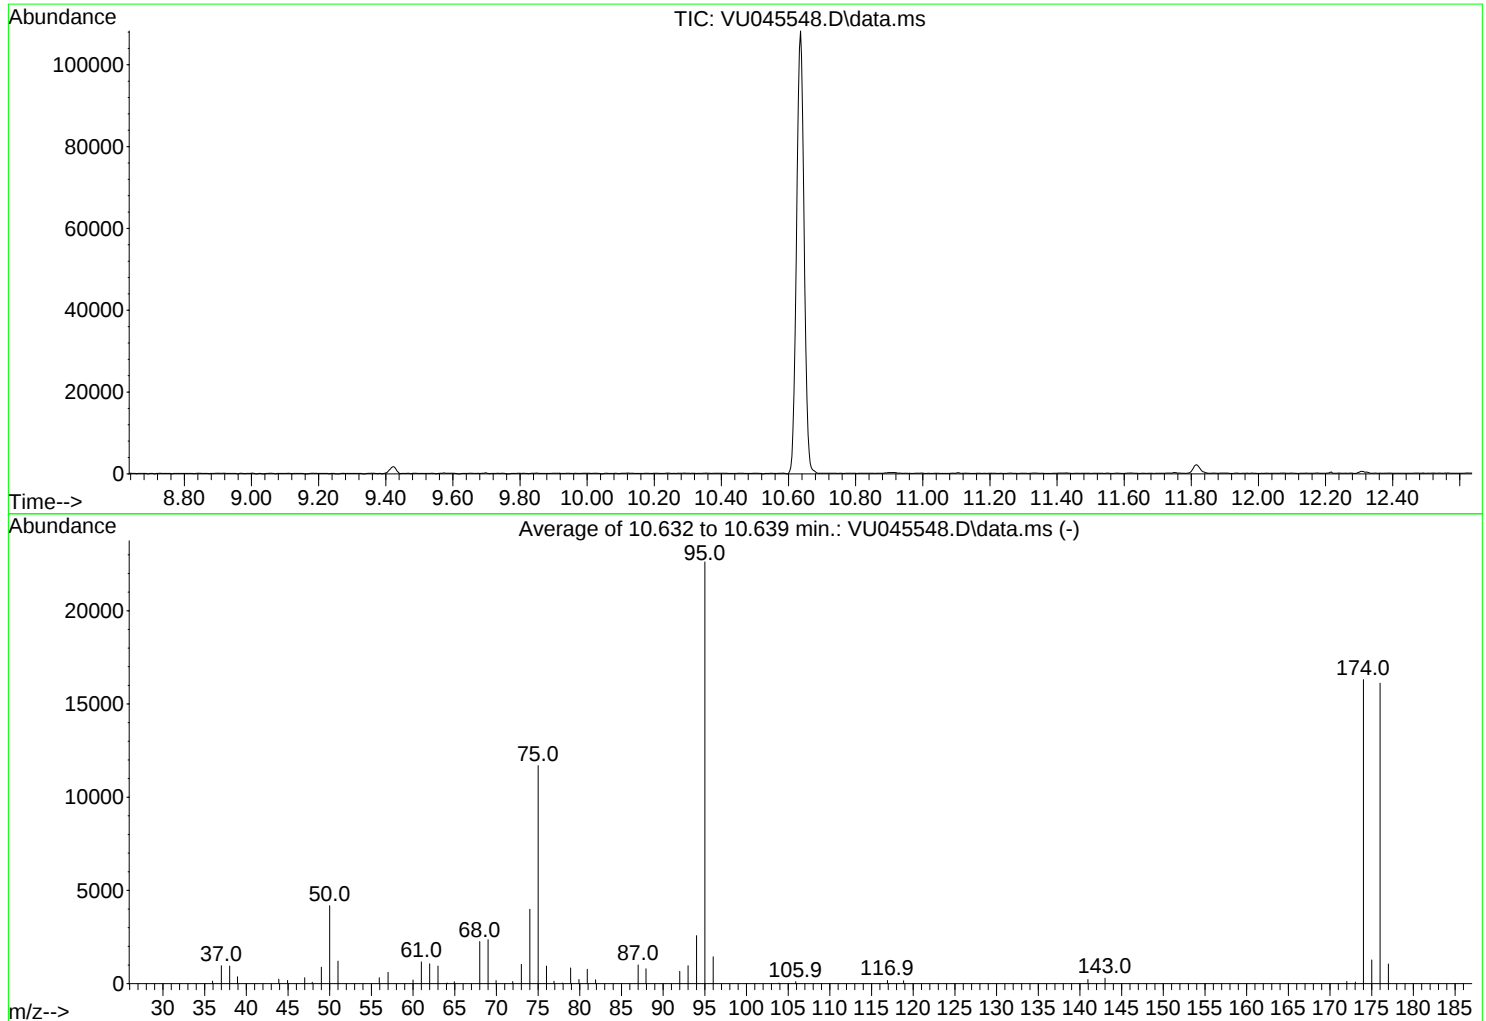

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	4176	PASS
75	95	30	60	51.7	11698	PASS
95	95	100	100	100.0	22624	PASS
96	95	5	9	6.4	1442	PASS
173	174	0.00	2	0.5	89	PASS
174	95	50	100	72.1	16310	PASS
175	174	5	9	7.8	1268	PASS
176	174	95	101	98.8	16120	PASS
177	176	5	9	6.5	1055	PASS