
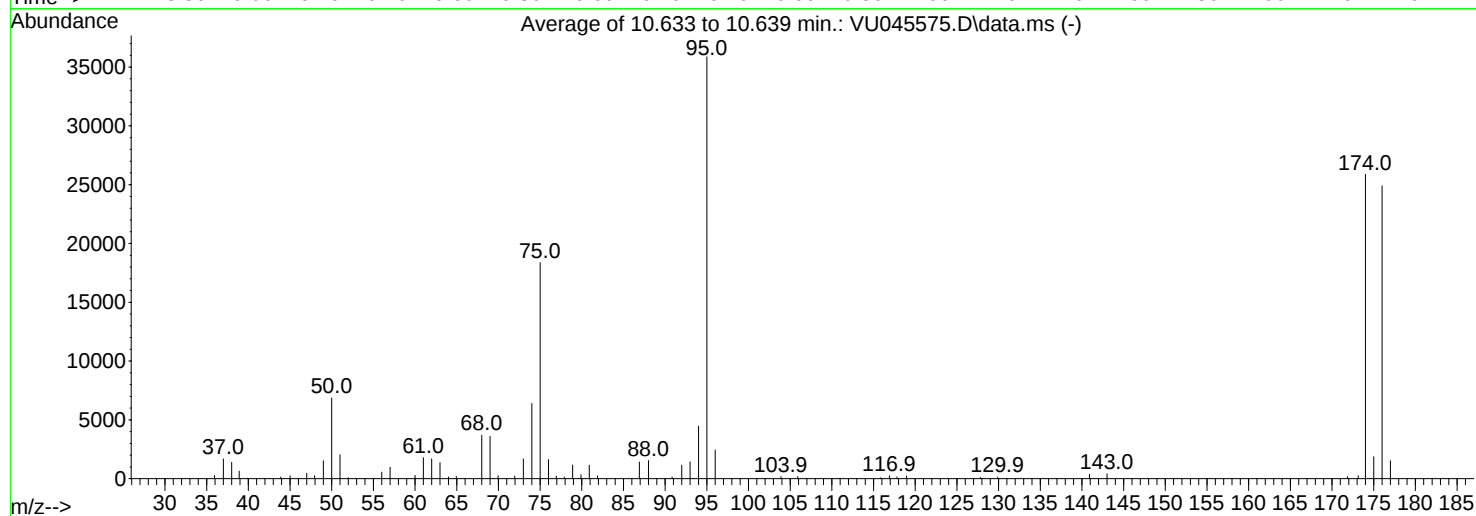


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110521\
 Data File : VU045575.D
 Acq On : 05 Nov 2021 21:33
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U110521W.M
 Title : SW846 8260
 Last Update : Fri Nov 05 13:35:16 2021

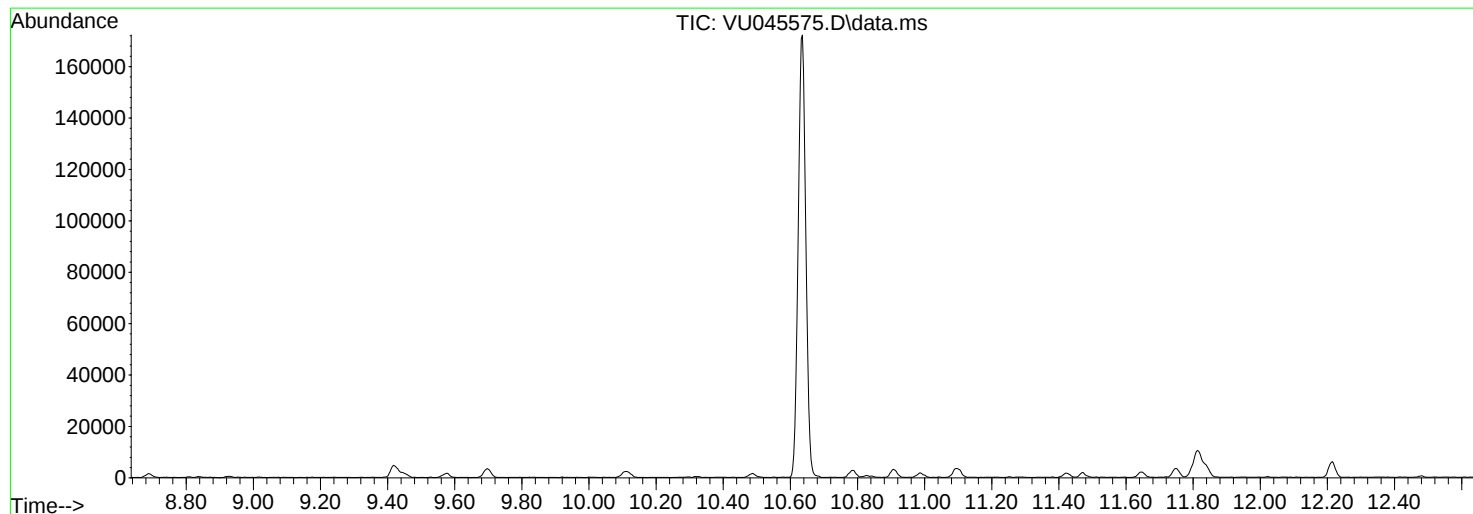

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	6865	PASS
75	95	30	60	51.2	18373	PASS
95	95	100	100	100.0	35872	PASS
96	95	5	9	6.8	2441	PASS
173	174	0.00	2	0.9	242	PASS
174	95	50	100	72.1	25880	PASS
175	174	5	9	7.2	1870	PASS
176	174	95	101	96.2	24896	PASS
177	176	5	9	6.1	1526	PASS