

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110525\
 Data File : VU063668.D
 Acq On : 05 Nov 2025 11:46
 Operator : MD/SY
 Sample : VU1105WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1105WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU063668.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.081	1474	1490	1508	rBV	64713	134406	85.51%	24.763%
2	7.878	2042	2049	2063	rVB7	1856	3596	2.29%	0.663%
3	8.676	2291	2297	2299	rBV5	2368	2088	1.33%	0.385%
4	8.897	2361	2366	2375	rBV9	1069	1670	1.06%	0.308%
5	9.418	2525	2528	2543	rVB8	1965	3354	2.13%	0.618%
6	9.544	2560	2567	2569	rBV6	1583	1731	1.10%	0.319%
7	9.676	2598	2608	2616	rBV5	2561	4020	2.56%	0.741%
8	10.100	2738	2740	2747	rVB6	1787	1723	1.10%	0.317%
9	10.454	2846	2850	2865	rVV8	1692	3194	2.03%	0.588%
10	10.611	2889	2899	2916	rBV2	64171	115885	73.72%	21.350%
11	10.885	2976	2984	2996	rVB3	2611	5062	3.22%	0.933%
12	11.081	3029	3045	3055	rBV3	3494	8927	5.68%	1.645%
13	11.396	3135	3143	3151	rVB7	2526	4025	2.56%	0.742%
14	11.450	3151	3160	3167	rBV4	3105	5208	3.31%	0.960%
15	11.621	3205	3213	3223	rVB4	2905	4931	3.14%	0.908%
16	11.727	3239	3246	3252	rBV8	2650	4265	2.71%	0.786%
17	11.769	3252	3259	3266	rVV3	3566	5926	3.77%	1.092%
18	11.817	3269	3274	3281	rVB5	2882	3856	2.45%	0.710%
19	12.171	3372	3384	3402	rBV3	80966	157186	100.00%	28.959%
20	12.743	3556	3562	3563	rBV5	1971	1587	1.01%	0.292%
21	13.820	3889	3897	3913	rBV4	9231	16299	10.37%	3.003%
22	13.997	3944	3952	3959	rBV9	2469	3331	2.12%	0.614%
23	14.071	3962	3975	3990	rBV	15417	29713	18.90%	5.474%
24	14.306	4040	4048	4061	rVB4	10428	18372	11.69%	3.385%
25	16.251	4646	4653	4658	rBV8	1532	2424	1.54%	0.447%




Sum of corrected areas: 542779

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110525\
Data File : VU063668.D
Acq On : 05 Nov 2025 11:46
Operator : MD/SY
Sample : VU1105WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1105WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

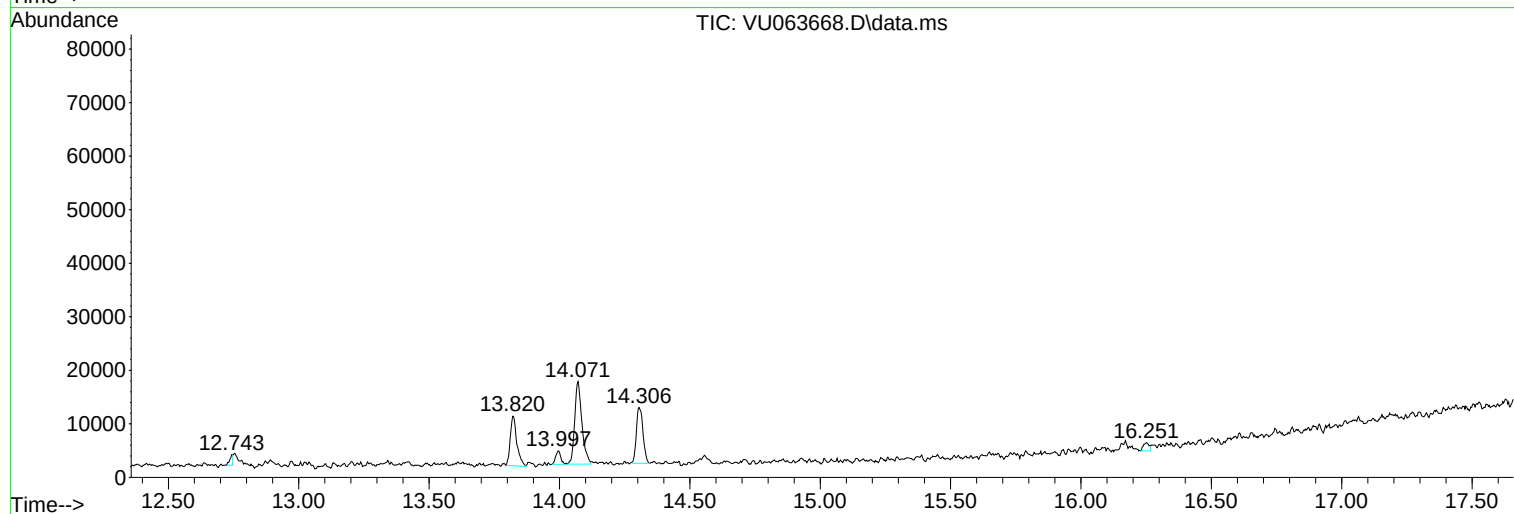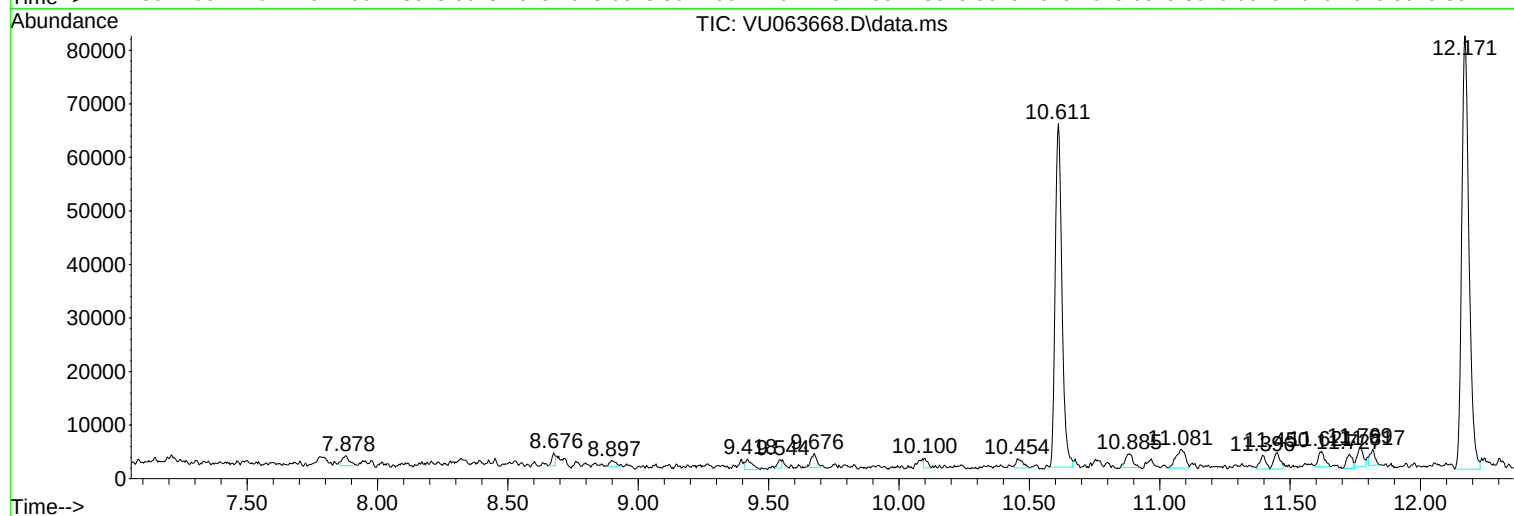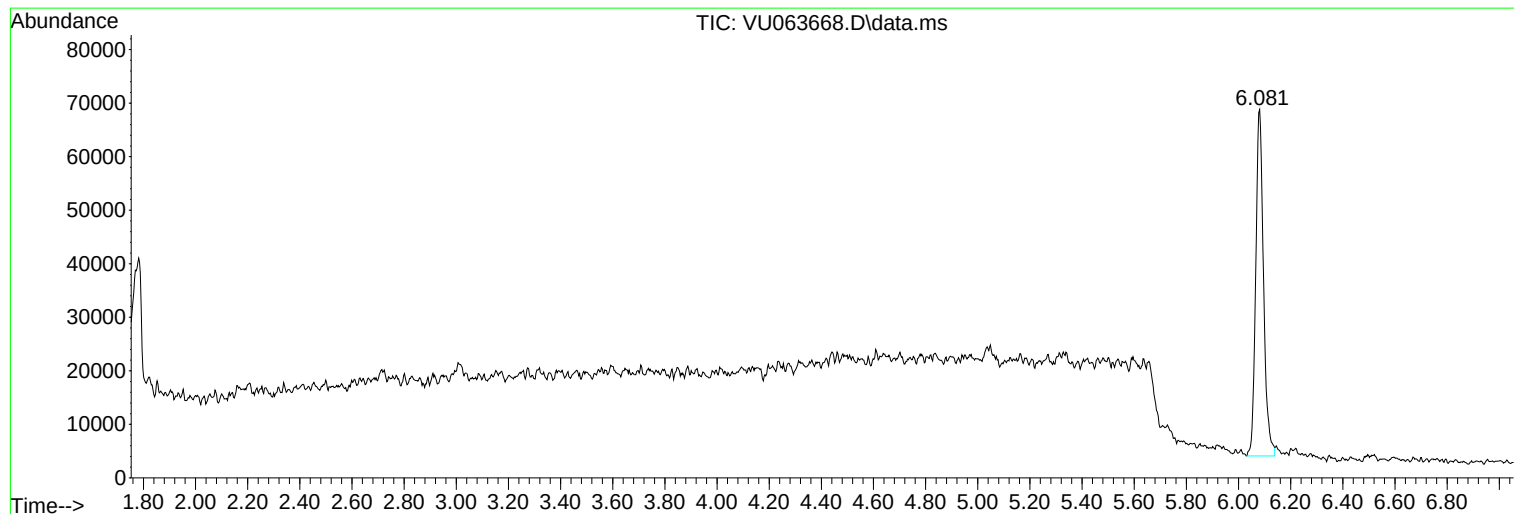

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110525\
Data File : VU063668.D
Acq On : 05 Nov 2025 11:46
Operator : MD/SY
Sample : VU1105WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1105WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110525\
Data File : VU063668.D
Acq On : 05 Nov 2025 11:46
Operator : MD/SY
Sample : VU1105WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1105WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------