
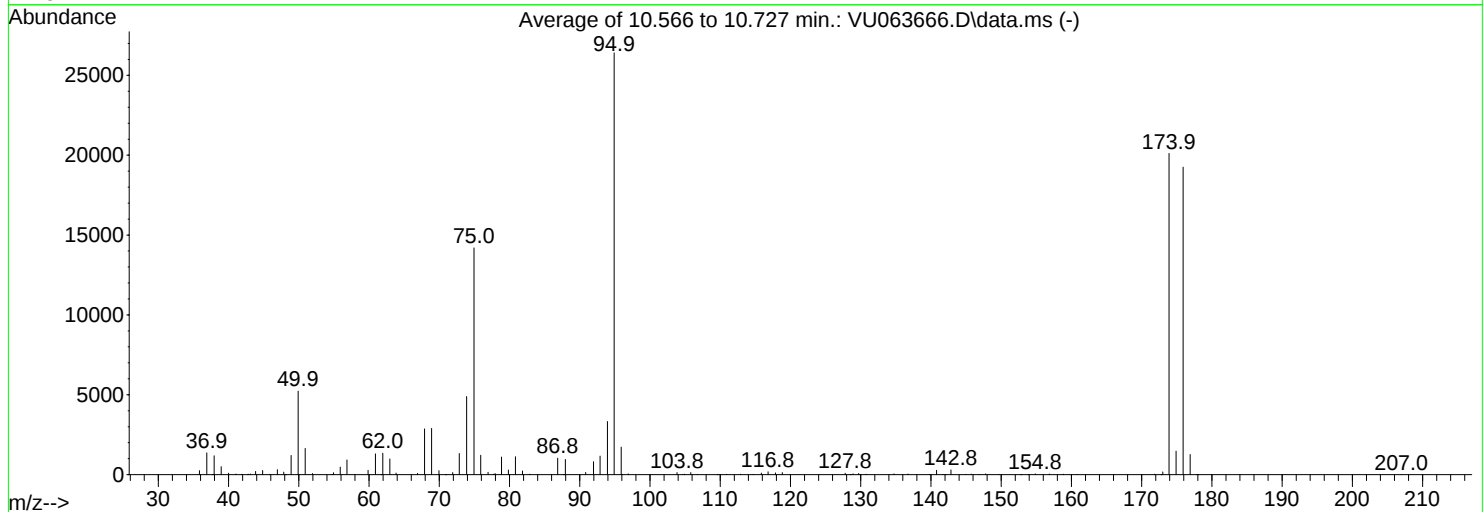


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110525\
Data File : VU063666.D
Acq On : 05 Nov 2025 09:43
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U103125DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Mon Nov 03 00:51:51 2025

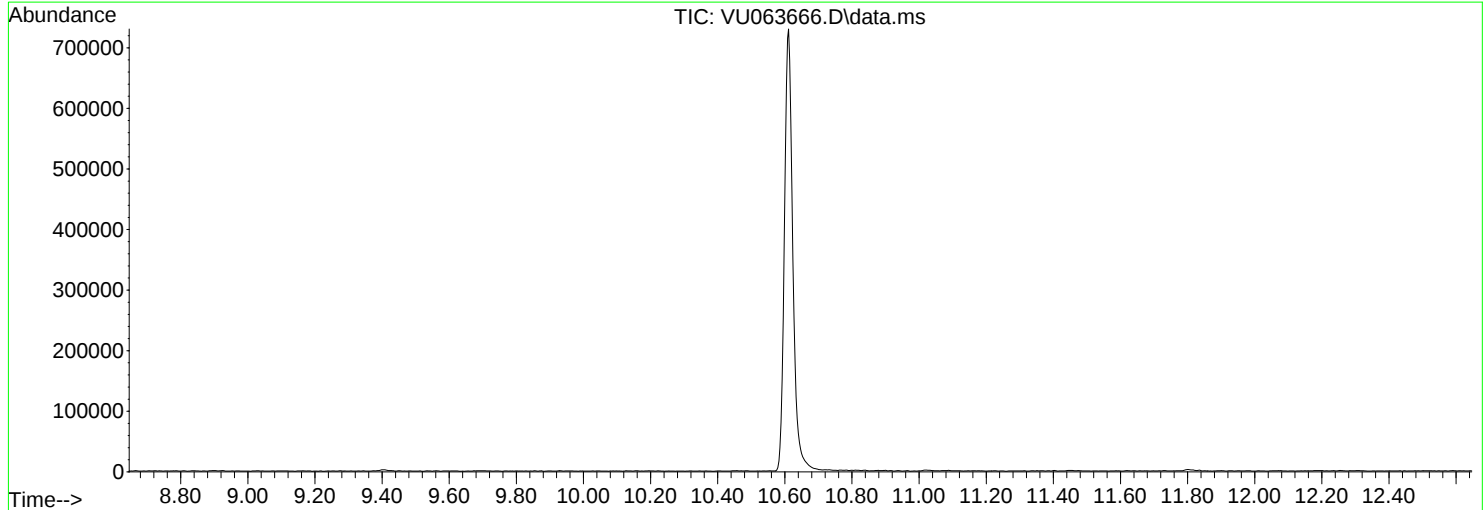

AutoFind: Averaged scan 2885 to 2935; Bkg corrected with scan 2884

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.8	5226	PASS
75	95	30	60	53.8	14195	PASS
95	95	100	100	100.0	26408	PASS
96	95	5	9	6.5	1724	PASS
173	174	0.00	2	0.9	171	PASS
174	95	50	100	76.2	20112	PASS
175	174	5	9	7.3	1469	PASS
176	174	95	101	95.8	19258	PASS
177	176	5	9	6.6	1263	PASS