




Data File : VU035647.D
Acq On : 06 Nov 2019 15:11
Operator : JC/SP
Sample : K5716-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BE894

Manual Integrations
APPROVED

MMDadoda
11/7/2019 8:35:12 AM

Quant Time: Nov 07 04:51:14 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 07 04:46:39 2019
Response via : Initial Calibration

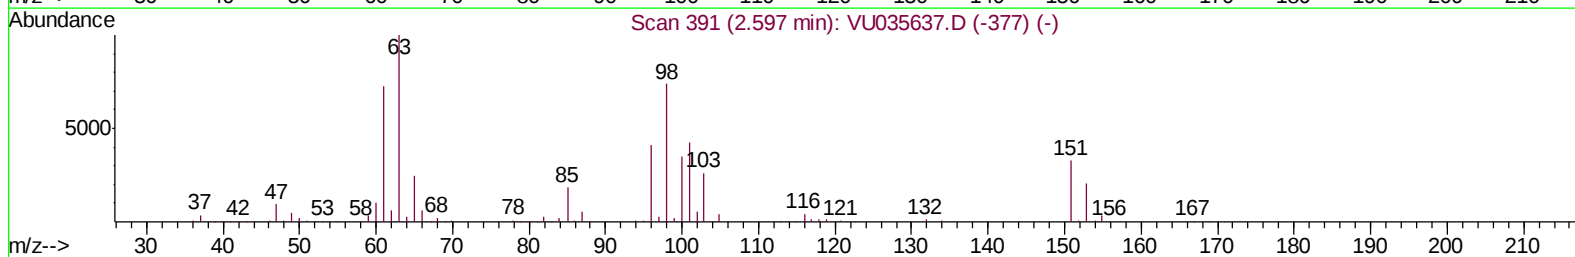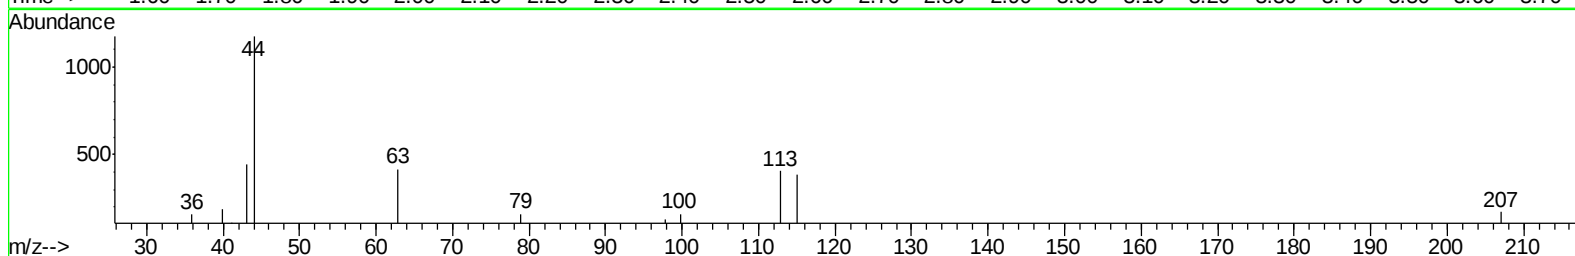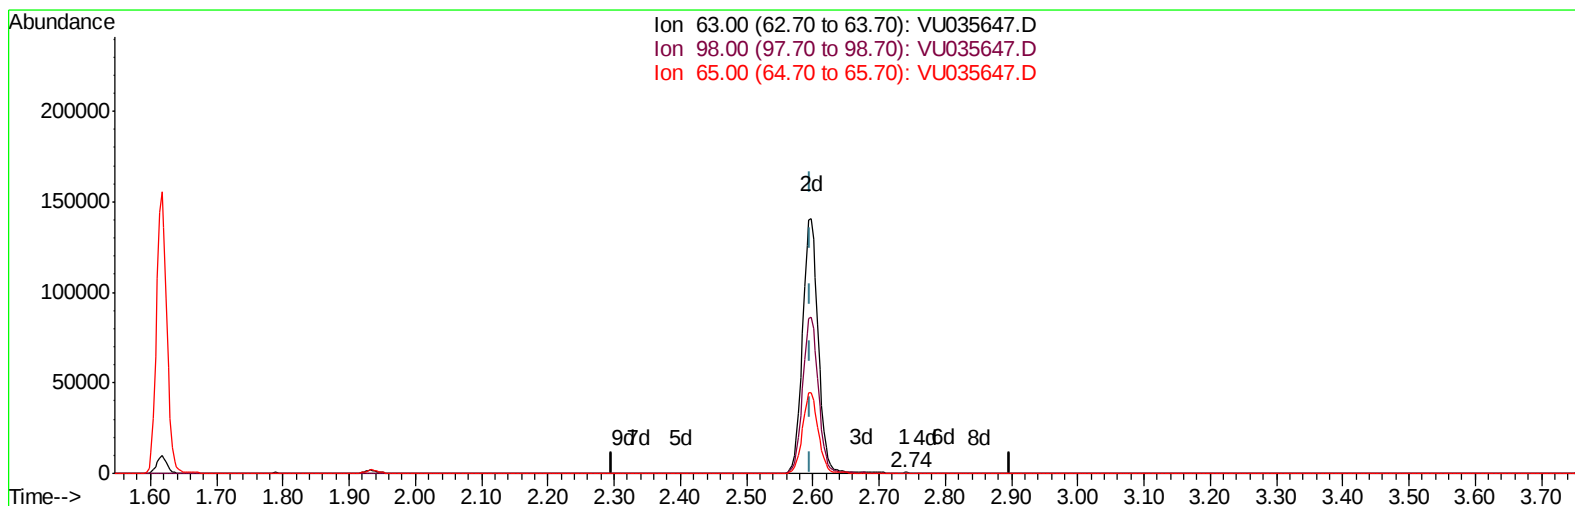

TIC: VU035647.D

(11) 1,1-Dichloroethene-d2 (S)

2.739min (+0.142) 0.03ug/L

response 227

Ion	Exp%	Act%
63.00	100	100
98.00	74.50	60.35
65.00	23.70	18.50
0.00	0.00	0.00




Data File : VU035647.D
Acq On : 06 Nov 2019 15:11
Operator : JC/SP
Sample : K5716-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BE894

Manual Integrations
APPROVED

MMDadoda
11/7/2019 8:35:12 AM

Quant Time: Nov 07 04:51:14 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 07 04:46:39 2019
Response via : Initial Calibration

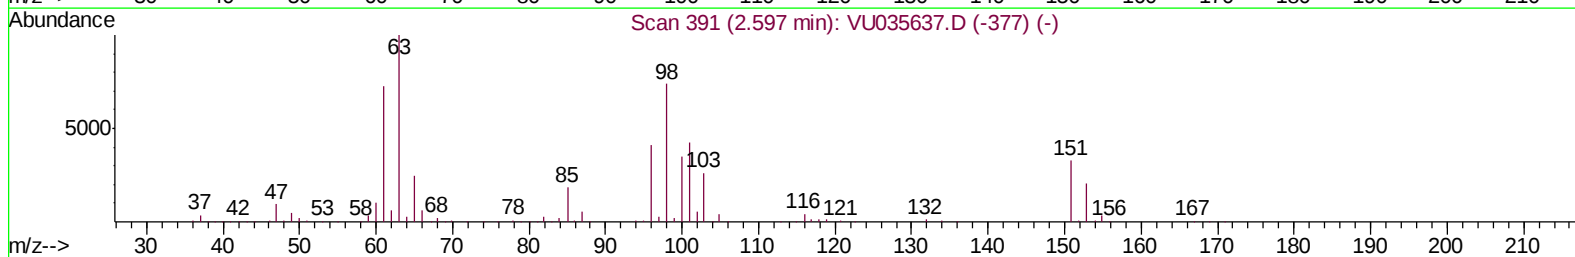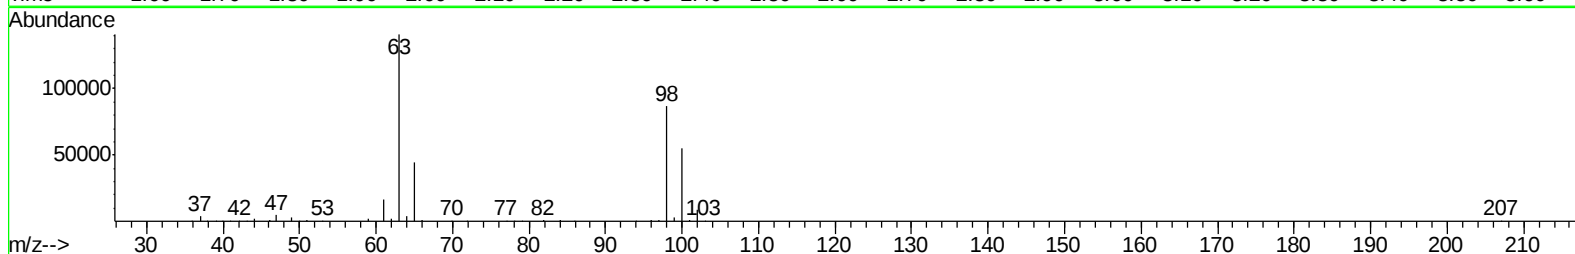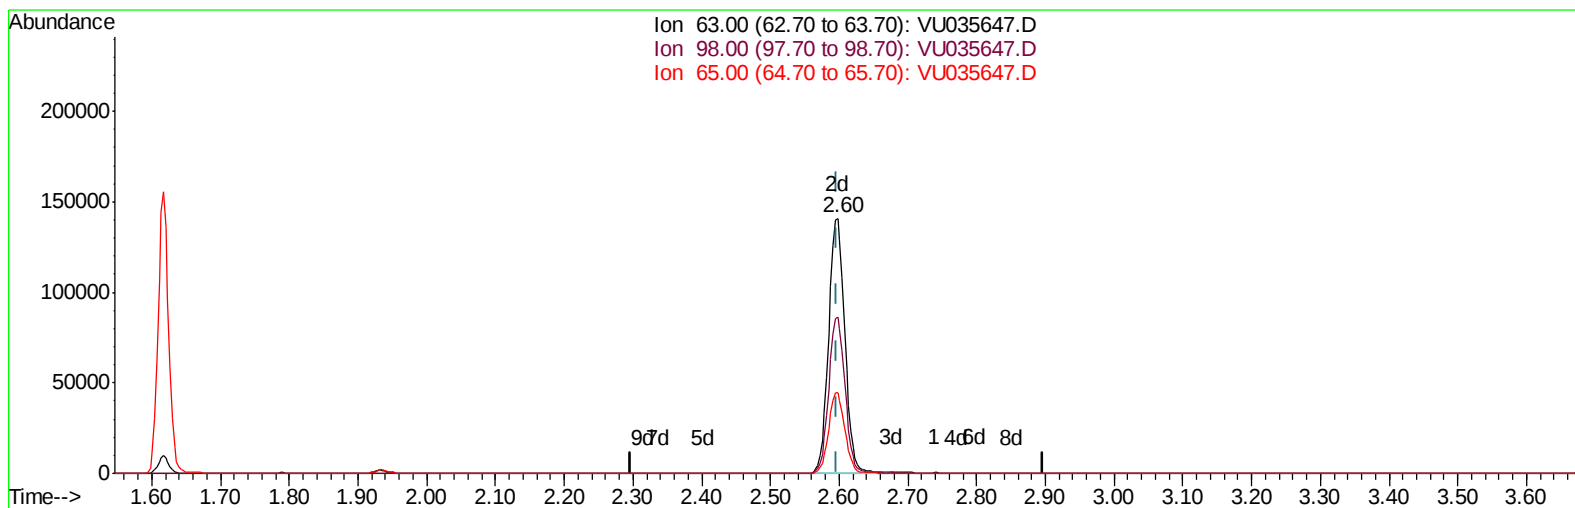

TIC: VU035647.D

(11) 1,1-Dichloroethene-d2 (S)

2.598min (+0.000) 29.15ug/L m

response 229794

Ion	Exp%	Act%
63.00	100	100
98.00	74.50	0.06#
65.00	23.70	0.02#
0.00	0.00	0.00

Data File : VU035647.D
Acq On : 06 Nov 2019 15:11
Operator : JC/SP
Sample : K5716-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BE894

Manual Integrations
APPROVED

MMDadoda
11/7/2019 8:35:12 AM

Quant Time: Nov 07 06:13:41 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 07 04:46:39 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.30	114	627532	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	609948	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	175897	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.62	65	168379	33.22	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	66.44%
7) Chloroethane-d5	1.94	69	161998	40.02	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	80.04%
11) 1,1-Dichloroethene-d2	2.60	63	229794m	29.15	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	58.30%#
21) 2-Butanone-d5	4.69	46	268877	90.82	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	90.82%
24) Chloroform-d	5.12	84	357955	45.73	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.46%
26) 1,2-Dichloroethane-d4	5.75	65	223555	46.62	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.24%
32) Benzene-d6	5.77	84	728485	45.82	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.64%
36) 1,2-Dichloropropane-d6	6.74	67	244839	47.49	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.98%
41) Toluene-d8	7.93	98	662410	44.17	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.34%
43) trans-1,3-Dichloropropene-	8.21	79	106822	44.98	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.96%
47) 2-Hexanone-d5	8.68	63	169738	85.90	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	85.90%
57) 1,1,2,2-Tetrachloroethane-	10.79	84	330687	45.10	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.20%
64) 1,2-Dichlorobenzene-d4	12.22	152	177031	49.90	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.80%

Target Compounds					Qvalue
13) Acetone	2.67	43	17265	6.628 ug/L	96
22) 2-Butanone	4.78	43	10263	2.985 ug/L	99
46) Tetrachloroethene	8.58	164	5721	1.570 ug/L	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU035647.D
Acq On : 06 Nov 2019 15:11
Operator : JC/SP
Sample : K5716-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BE894

Manual Integrations
APPROVED

MMDadoda
11/7/2019 8:35:12 AM

Quant Time: Nov 07 06:13:41 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 07 04:46:39 2019
Response via : Initial Calibration

