


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110619\
 Data File : VU035636.D
 Acq On : 06 Nov 2019 08:27
 Operator : JC/SP
 Sample : BFB50
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB50

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
 Title : VOC Analysis
 Last Update : Fri Nov 15 01:03:04 2019

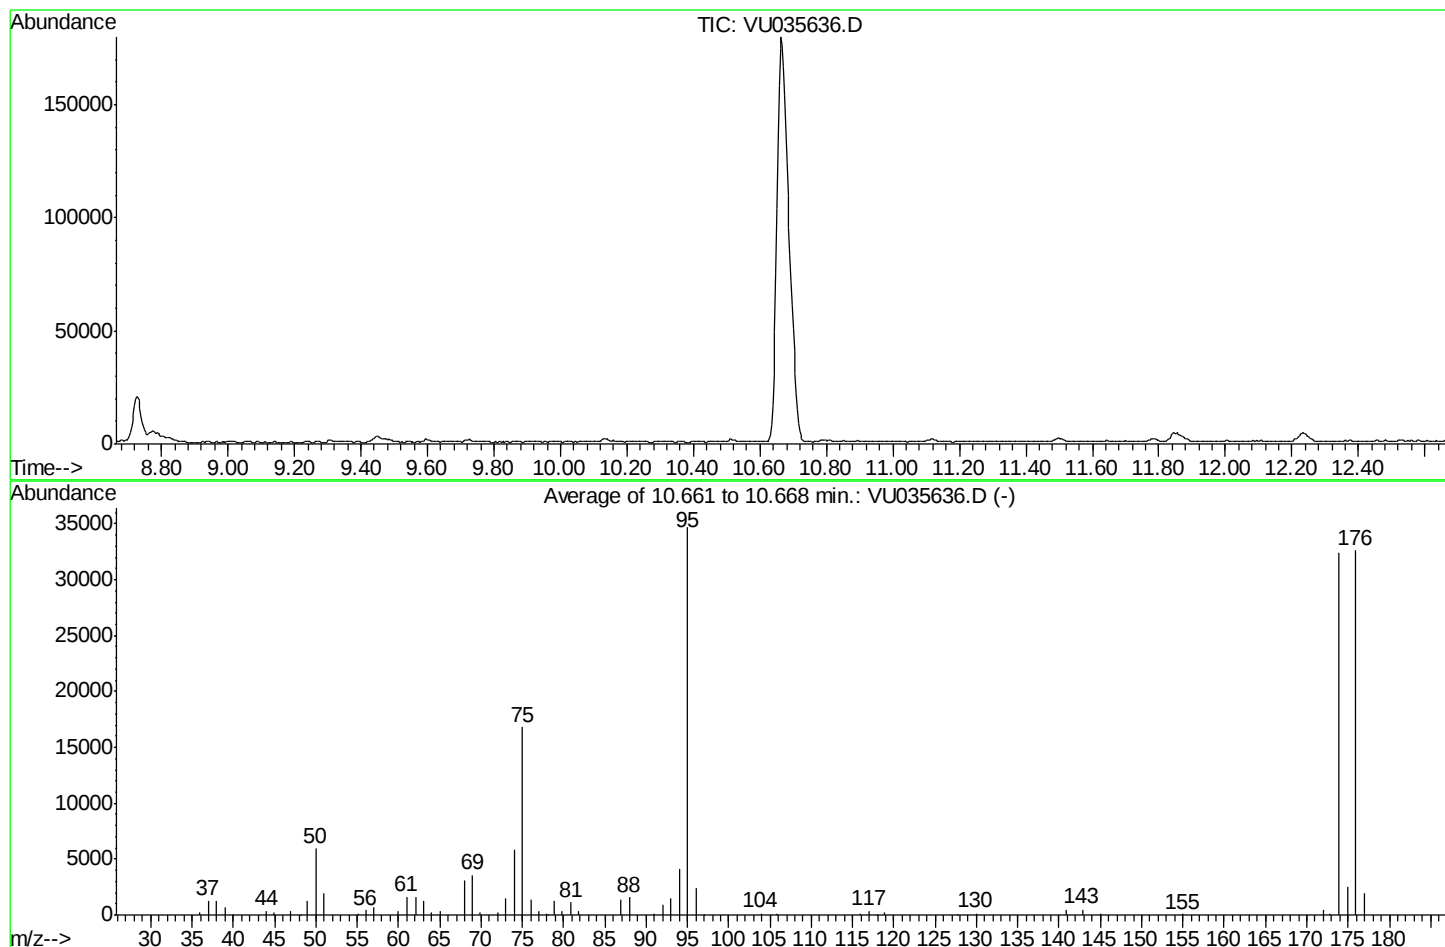

AutoFind: Scans 2899, 2900, 2901; Background Corrected with Scan 2887

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	5921	PASS
75	95	30	80	48.5	16832	PASS
95	95	100	100	100.0	34682	PASS
96	95	5	9	7.1	2452	PASS
173	174	0.00	2	0.4	143	PASS
174	95	50	120	93.6	32466	PASS
175	174	5	9	7.7	2496	PASS
176	174	95	101	100.4	32586	PASS
177	176	5	9	5.8	1901	PASS

Scan 2887 (10.623 min): VU035636.D
BFB50

m/z	Abundance
39.90	258.0
44.00	671.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

m/z	Abundance
35.90	254.0
37.00	1353.0
38.00	1277.0
39.00	659.0
39.90	283.0
44.00	988.0
45.00	239.0
46.90	304.0
48.10	156.0
49.00	1308.0
50.00	6109.0
51.00	2015.0
55.20	108.0
56.00	469.0
57.10	657.0
60.00	312.0
61.00	1685.0
62.00	1541.0
63.00	1235.0
64.00	226.0
65.00	350.0
68.00	3285.0
69.00	3558.0
69.90	270.0
72.10	178.0
73.00	1672.0
74.00	5831.0
75.00	16552.0
76.00	1361.0
76.90	309.0
77.90	229.0
78.90	1382.0
79.80	406.0
80.90	1100.0
81.80	410.0
87.00	1250.0
88.00	1363.0
92.00	991.0
93.00	1481.0
94.00	4069.0
95.00	34480.0
96.00	2521.0
97.00	117.0
103.90	135.0
105.90	112.0
115.90	155.0
117.00	313.0
117.90	113.0
118.90	213.0
130.00	108.0
140.80	435.0
142.80	417.0
144.90	139.0
155.00	115.0
172.00	540.0
173.90	31472.0
175.00	2402.0
175.90	31920.0
176.90	1922.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

m/z	Abundance
35.90	258.0
37.00	1321.0
38.00	1323.0
39.10	761.0
39.90	328.0
44.00	1097.0
45.00	244.0
46.90	302.0
49.00	1297.0
50.00	6043.0
51.00	1948.0
55.10	122.0
56.00	472.0
57.10	731.0
60.00	303.0
61.00	1686.0
62.00	1622.0
63.00	1264.0
64.00	275.0
65.10	333.0
68.00	3179.0
69.00	3661.0
69.90	202.0
72.10	207.0
73.00	1514.0
74.00	5988.0
75.00	17184.0
76.00	1358.0
76.90	319.0
77.90	185.0
78.90	1349.0
79.90	379.0
80.90	1145.0
81.80	352.0
86.90	1363.0
88.00	1614.0
91.00	101.0
92.00	990.0
93.00	1474.0
94.00	4260.0
95.00	35176.0
96.00	2509.0
104.00	157.0
105.90	167.0
115.90	160.0
117.00	396.0
118.90	240.0
127.70	109.0
130.00	153.0
140.90	441.0
142.90	489.0
145.00	125.0
155.00	129.0
172.00	519.0
173.90	33024.0
175.00	2561.0
175.90	33104.0
176.90	1901.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

m/z	Abundance
35.90	235.0
37.00	1274.0
38.00	1315.0
39.10	777.0
39.90	313.0
44.00	1079.0
44.90	294.0
46.90	300.0
49.00	1257.0
50.00	5611.0
51.00	1966.0
55.10	122.0
56.00	414.0
57.00	851.0
60.00	300.0
61.00	1543.0
62.10	1713.0
63.10	1245.0
64.00	239.0
65.10	308.0
68.00	2881.0
69.00	3530.0
70.00	149.0
72.10	230.0
73.00	1395.0
74.00	5584.0
75.00	16760.0
76.00	1293.0
77.00	288.0
78.10	160.0
78.90	1231.0
79.90	394.0
80.90	1172.0
81.80	262.0
86.90	1508.0
88.00	1801.0
90.90	129.0
92.00	903.0
93.00	1369.0
94.00	4216.0
95.00	34392.0
96.00	2328.0
104.00	174.0
105.80	184.0
115.90	148.0
117.00	378.0
118.90	253.0
130.00	135.0
140.80	376.0
142.90	496.0
145.10	125.0
171.90	402.0
172.80	429.0
173.90	32904.0
175.00	2527.0
175.90	32736.0
176.90	1880.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50