

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU110620\
 Data File : VU041130.D
 Acq On : 06 Nov 2020 22:04
 Operator : SY/MD
 Sample : L4646-08
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB0G3

Quant Time: Nov 07 00:34:22 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 06 23:04:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	56072	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	58911	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	25125	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	18692	3.97	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.40%
7) Chloroethane-d5	1.92	69	17188	4.75	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.00%
11) 1,1-Dichloroethene-d2	2.58	63	29582	3.20	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.00%
20) 2-Butanone-d5	4.65	46	81344	52.44	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.88%
24) Chloroform-d	5.08	84	44766	5.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.60%
26) 1,2-Dichloroethane-d4	5.72	65	28790	5.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	111.60%
32) Benzene-d6	5.74	84	79828	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.40%
36) 1,2-Dichloropropane-d6	6.70	67	28260	5.51	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	110.20%
41) Toluene-d8	7.91	98	65187	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.40%
43) trans-1,3-Dichloropropene-	8.19	79	10158	4.57	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.40%
46) 2-Hexanone-d5	8.64	63	57911	48.37	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.74%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	25161	5.28	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.60%
64) 1,2-Dichlorobenzene-d4	12.19	152	27080	6.14	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	122.80%#


Target Compounds					Ovalue
13) Acetone	2.66	43	2629	2.479 ug/L	# 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU110620\
Data File : VU041130.D
Acq On : 06 Nov 2020 22:04
Operator : SY/MD
Sample : L4646-08
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB0G3

Quant Time: Nov 07 00:34:22 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 06 23:04:51 2020
Response via : Initial Calibration

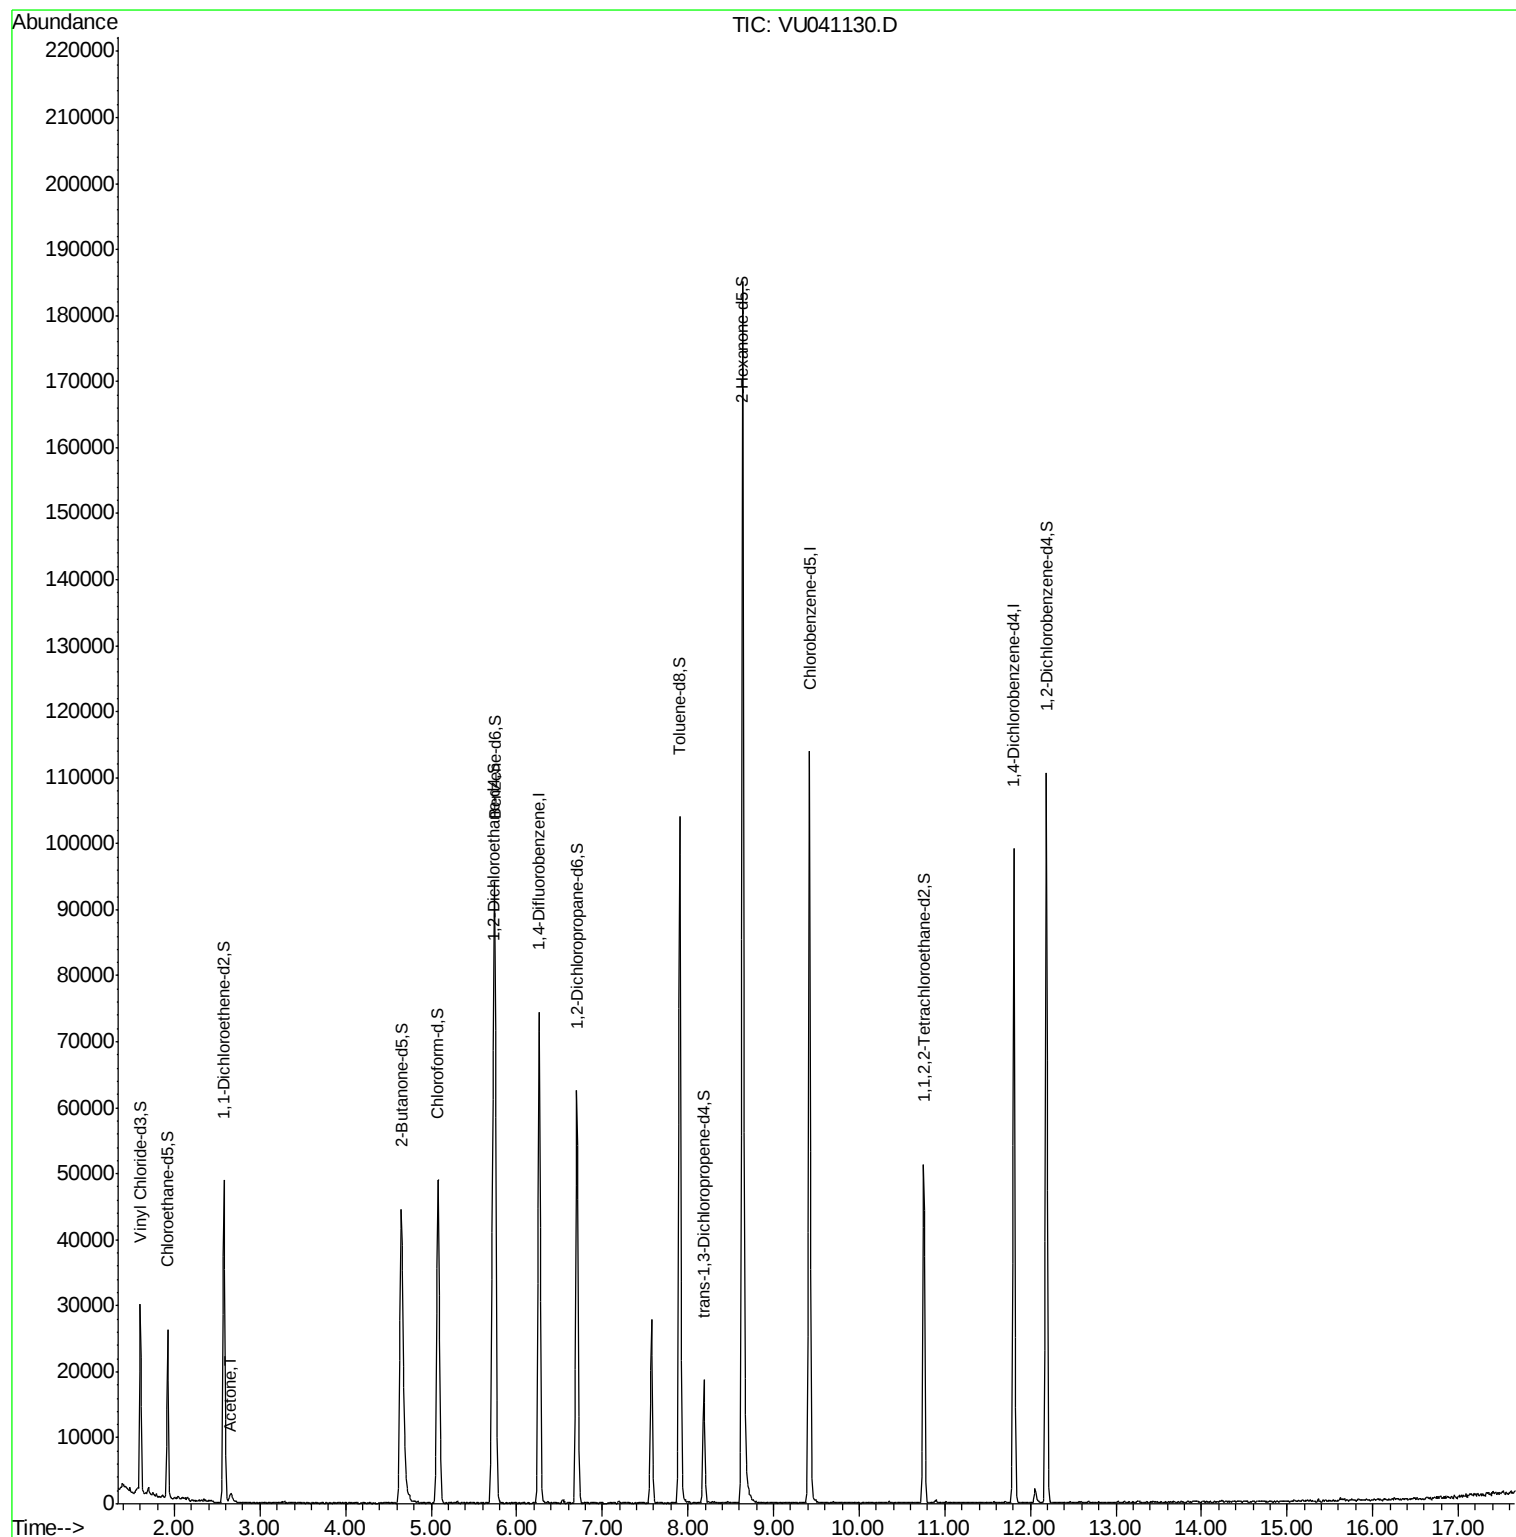

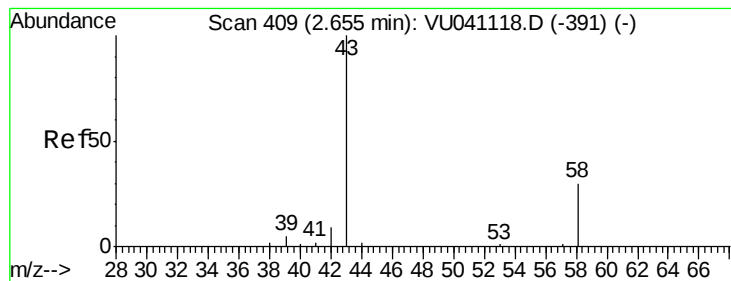

#13
 Acetone
 Concen: 2.479 ug/L
 RT: 2.66 min Scan# 410
 Delta R.T. 0.00 min
 Lab File: VU041130.D
 Acq: 06 Nov 2020 22:04

Instrument :
 MSVOA_U
 ClientSampleId :
 GB0G3

Tot Ion: 43 Resp: 2629
 Ion Ratio Lower Upper
 43 100
 58 25.8 0.0 25.4#

