


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU110620\
 Data File : VU041117.D
 Acq On : 06 Nov 2020 14:38
 Operator : SY/MD
 Sample : BFB07
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB07

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR102620WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Nov 07 02:30:45 2020

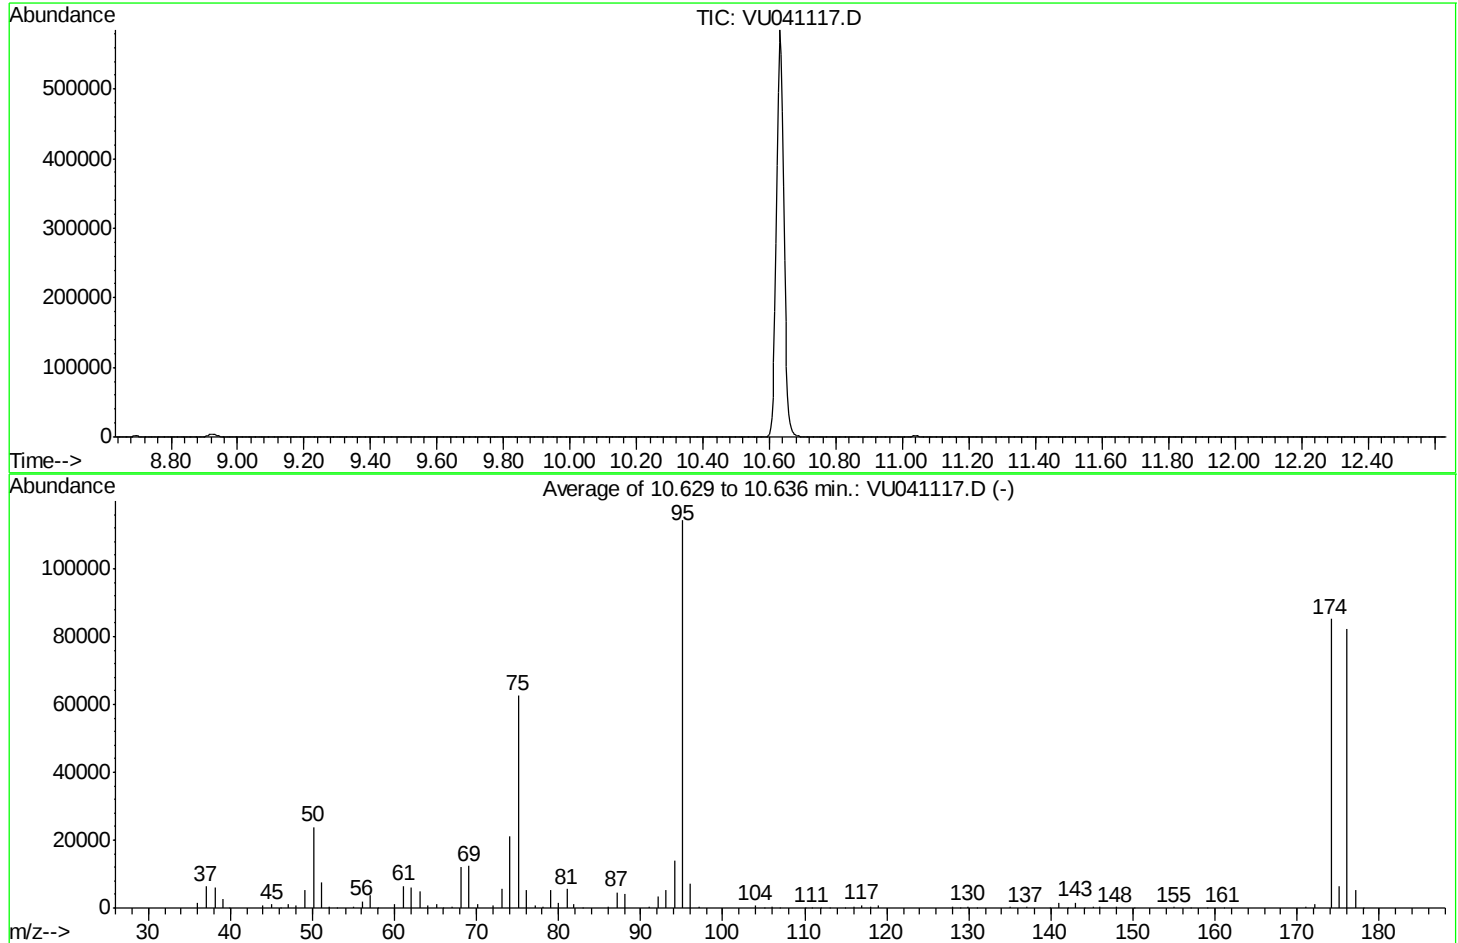

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	23789	PASS
75	95	30	80	54.7	62442	PASS
95	95	100	100	100.0	114242	PASS
96	95	5	9	6.4	7261	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.6	85216	PASS
175	174	5	9	7.7	6571	PASS
176	174	95	101	96.7	82376	PASS
177	176	5	9	6.6	5415	PASS

m/z	Abundance
36.00	1425.0
37.10	6795.0
38.10	6184.0
39.10	2547.0
40.00	157.0
44.00	870.0
45.00	1099.0
46.20	151.0
47.10	1207.0
48.00	784.0
49.10	5568.0
50.10	24280.0
51.10	7522.0
52.00	297.0
55.00	448.0
56.10	2194.0
57.10	3763.0
58.00	173.0
60.00	1087.0
61.10	6424.0
62.10	6283.0
63.10	5118.0
64.10	736.0
65.10	1038.0
66.00	138.0
67.00	325.0
68.10	12408.0
69.10	12601.0
70.10	1153.0
72.10	612.0
73.10	5792.0
74.10	21840.0
75.10	63248.0
76.10	5215.0
77.10	641.0
78.10	479.0
79.00	5495.0
80.00	1574.0
81.00	5532.0
81.90	1194.0
83.00	137.0
86.00	223.0
87.10	4625.0
88.10	4030.0
91.00	506.0
92.10	3623.0
93.10	5429.0
94.10	13891.0
95.10	114360.0
96.10	7128.0
97.10	253.0
104.00	630.0
105.00	176.0
106.00	514.0
107.00	106.0
110.00	101.0
110.80	136.0
111.90	120.0
113.00	141.0
114.80	161.0
116.00	487.0
117.00	961.0
118.00	566.0
119.00	789.0
128.00	379.0
128.90	211.0
129.90	450.0
131.00	214.0
135.00	184.0
137.00	270.0
139.90	120.0
141.00	1326.0
142.00	149.0
143.00	1678.0
144.00	124.0
145.10	465.0
146.00	189.0
147.90	289.0
155.00	291.0
157.00	171.0
159.00	187.0
161.00	153.0
171.10	239.0
172.10	1244.0
174.10	82960.0
175.10	6592.0
176.10	79648.0
177.10	5436.0
178.00	116.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

m/z	Abundance
36.00	1399.0
37.00	6533.0
38.10	6189.0
39.10	2594.0
39.90	144.0
44.00	851.0
45.10	1117.0
46.10	107.0
47.10	1227.0
48.00	772.0
49.10	5604.0
50.10	24504.0
51.10	7819.0
52.00	258.0
52.90	120.0
55.00	420.0
56.10	2069.0
57.10	3901.0
58.00	187.0
60.00	1091.0
61.10	6665.0
62.10	6397.0
63.10	5186.0
64.10	681.0
65.10	1020.0
66.00	108.0
67.10	381.0
68.10	12509.0
69.10	12627.0
70.10	1102.0
72.10	557.0
73.10	5880.0
74.10	21992.0
75.10	64704.0
76.10	5417.0
77.10	653.0
78.10	511.0
79.00	5429.0
80.00	1579.0
81.00	5720.0
81.90	1184.0
83.00	162.0
86.00	235.0
87.10	4918.0
88.10	4213.0
91.00	495.0
92.00	3502.0
93.10	5640.0
94.10	14593.0
95.10	117776.0
96.10	7488.0
97.00	206.0
104.00	653.0
105.00	152.0
106.00	591.0
107.00	126.0
110.00	116.0
110.80	149.0
111.90	116.0
113.00	148.0
114.90	146.0
116.10	480.0
117.00	983.0
117.90	585.0
119.00	790.0
127.90	399.0
128.90	181.0
129.90	491.0
130.90	214.0
135.10	226.0
137.00	287.0
141.00	1406.0
142.10	154.0
143.00	1623.0
144.00	106.0
145.10	456.0
146.00	216.0
147.90	271.0
155.00	244.0
156.90	173.0
159.00	165.0
161.00	146.0
171.10	223.0
172.10	1179.0
174.10	87816.0
175.10	6760.0
176.10	85032.0
177.10	5603.0
178.00	139.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

m/z	Abundance
36.00	1190.0
37.00	5824.0
38.10	5572.0
39.10	2409.0
39.90	134.0
44.00	911.0
45.10	1044.0
47.00	1219.0
48.00	729.0
49.00	5139.0
50.10	22584.0
51.10	7134.0
52.00	223.0
52.90	117.0
55.00	394.0
56.10	1824.0
57.10	3535.0
58.00	174.0
60.00	970.0
61.10	6162.0
62.10	6014.0
63.10	4758.0
64.10	558.0
65.10	874.0
67.10	387.0
68.10	11698.0
69.10	11776.0
70.10	949.0
72.00	579.0
73.10	5353.0
74.10	20016.0
75.10	59376.0
76.10	5028.0
77.10	625.0
78.10	462.0
79.00	4766.0
80.00	1439.0
81.00	5322.0
81.90	1126.0
83.00	160.0
86.10	239.0
87.10	4602.0
88.00	3971.0
91.00	446.0
92.00	3056.0
93.10	5207.0
94.10	13904.0
95.10	110592.0
96.10	7169.0
97.00	156.0
104.00	607.0
105.00	129.0
106.00	584.0
107.00	110.0
110.00	131.0
110.90	147.0
111.90	109.0
113.00	112.0
115.00	110.0
116.00	423.0
117.00	914.0
117.90	510.0
119.00	750.0
127.90	378.0
128.90	161.0
129.90	461.0
131.00	165.0
135.10	222.0
137.00	281.0
141.00	1346.0
142.10	132.0
143.00	1598.0
145.10	412.0
146.00	228.0
147.90	239.0
150.10	102.0
155.10	227.0
157.00	168.0
159.10	160.0
161.00	108.0
171.10	174.0
172.10	1022.0
174.10	84872.0
175.10	6361.0
176.10	82448.0
177.10	5206.0
178.10	165.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

m/z	Abundance
44.00	184.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07