
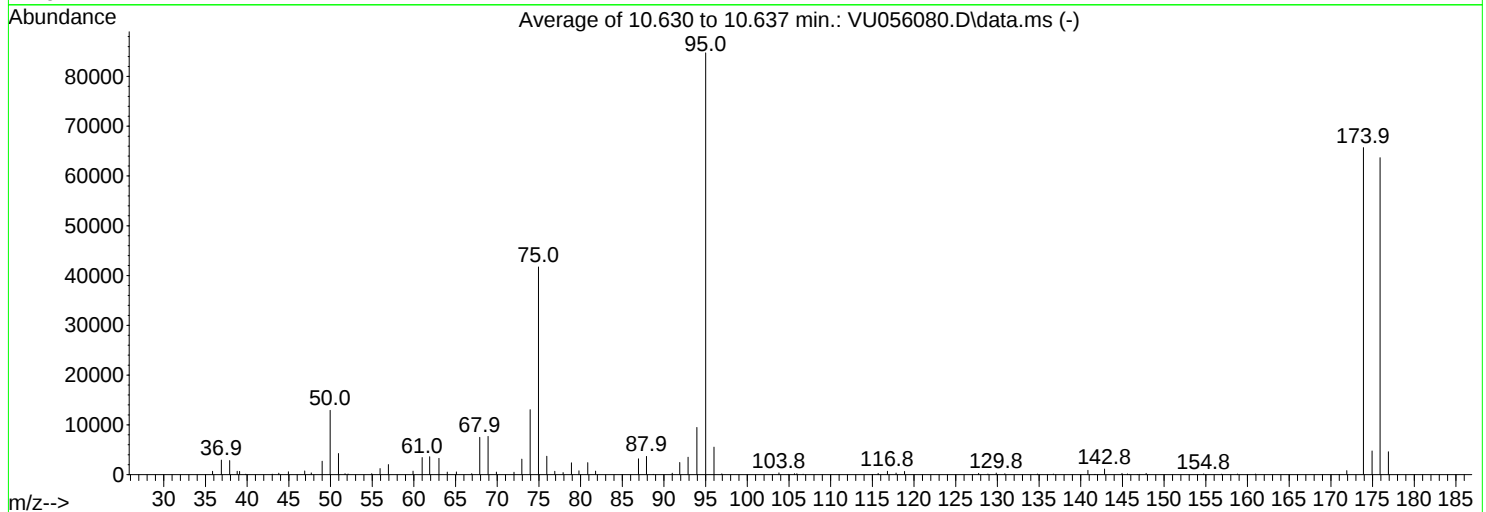


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU110623\
Data File : VU056080.D
Acq On : 06 Nov 2023 09:04
Operator : MD/SY
Sample : BFB066
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB066

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR102423WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Nov 07 04:07:55 2023

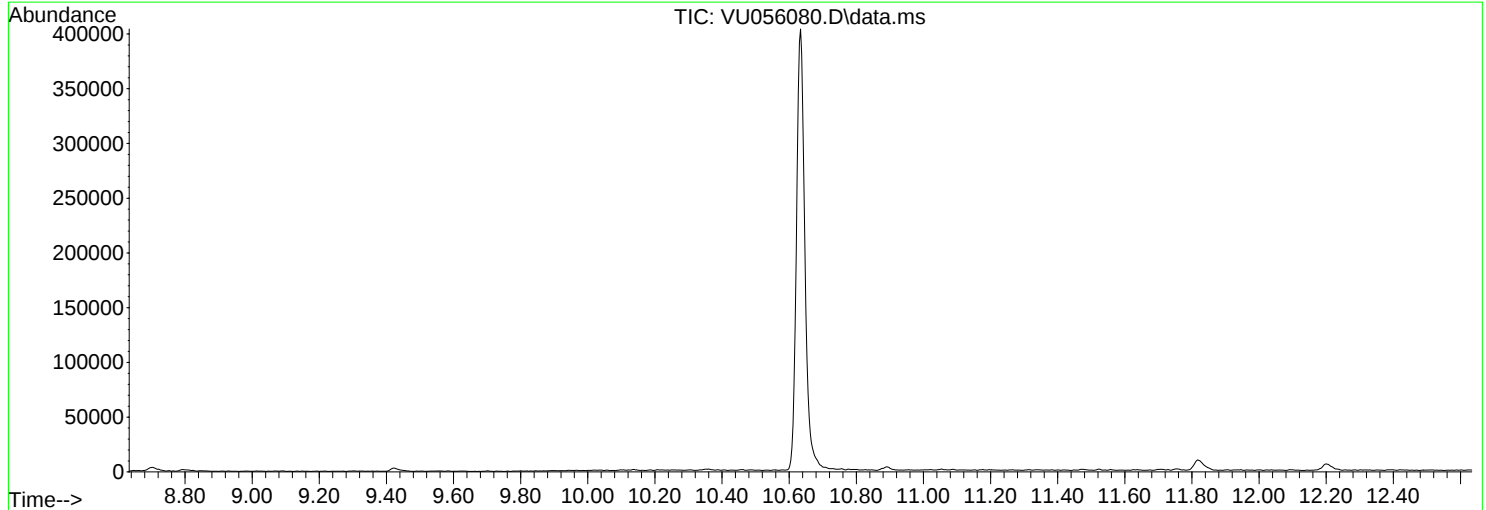

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.3	12932	PASS
75	95	30	80	49.2	41715	PASS
95	95	100	100	100.0	84739	PASS
96	95	5	9	6.5	5544	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.5	65696	PASS
175	174	5	9	7.2	4749	PASS
176	174	95	101	96.9	63691	PASS
177	176	5	9	7.2	4602	PASS

m/z	Abundance
35.90	783.0
37.80	169.0
39.80	191.0
43.80	516.0

Instrument :
MSVOA_U
ClientSampleId :
BFB066

m/z	Abundance
35.90	1443.0
36.90	3136.0
37.90	3021.0
38.80	1099.0
39.90	269.0
43.90	868.0
44.90	513.0
46.90	782.0
47.70	350.0
49.00	2754.0
49.90	12873.0
51.00	4258.0
51.80	219.0
54.90	191.0
56.00	1139.0
56.90	2071.0
59.90	735.0
61.00	3530.0
61.90	3615.0
63.00	3463.0
64.10	408.0
65.10	518.0
67.00	137.0
67.90	7522.0
68.90	7939.0
69.90	548.0
72.00	523.0
72.90	3328.0
73.90	13349.0
75.00	41760.0
76.00	3866.0
76.90	624.0
77.90	516.0
78.90	2526.0
79.80	803.0
80.80	2344.0
81.80	744.0
87.00	3374.0
87.90	3829.0
88.70	158.0
91.00	305.0
91.90	2317.0
92.90	3418.0
93.90	9354.0
95.00	85208.0
96.00	5690.0
96.90	116.0
103.80	359.0
104.90	134.0
105.70	362.0
106.70	142.0
111.00	133.0
115.70	210.0
116.80	729.0
117.90	313.0
118.90	597.0
127.90	309.0
128.80	198.0
129.90	359.0
130.90	150.0
134.90	165.0
136.70	111.0
140.90	754.0
141.70	107.0
142.80	1092.0
144.90	217.0
145.60	231.0
146.80	108.0
147.80	241.0
154.80	136.0
158.80	125.0
160.90	165.0
171.90	710.0
173.90	64576.0
174.90	4821.0
175.90	62792.0
176.90	4585.0

Instrument :
MSVOA_U
ClientSampleId :
BFB066

m/z	Abundance
35.90	1540.0
36.90	3005.0
38.00	3060.0
38.80	915.0
39.10	965.0
39.90	312.0
43.00	122.0
43.90	832.0
45.00	594.0
46.90	789.0
47.70	372.0
49.00	2735.0
50.00	13397.0
51.00	4372.0
51.70	191.0
52.10	167.0
54.90	185.0
55.90	1293.0
57.00	2075.0
59.90	770.0
61.00	3509.0
61.90	3720.0
63.00	3357.0
64.00	501.0
65.10	571.0
66.90	204.0
67.90	7690.0
68.90	7827.0
69.90	518.0
72.00	526.0
72.90	3146.0
74.00	13430.0
75.00	42856.0
75.90	3736.0
76.90	692.0
77.90	457.0
78.90	2454.0
79.80	783.0
80.80	2474.0
81.80	750.0
87.00	3216.0
87.90	3860.0
91.00	311.0
91.90	2578.0
92.90	3522.0
93.90	9755.0
95.00	86984.0
96.00	5662.0
96.90	160.0
103.80	364.0
104.90	111.0
105.90	311.0
106.70	113.0
115.70	275.0
116.80	734.0
117.80	321.0
118.80	663.0
127.70	248.0
128.90	162.0
129.90	352.0
130.90	200.0
134.80	137.0
136.70	142.0
140.80	894.0
141.70	112.0
142.90	1147.0
144.90	281.0
145.60	253.0
147.00	102.0
147.80	242.0
154.70	159.0
156.90	127.0
158.80	159.0
160.90	132.0
171.00	107.0
171.90	882.0
173.90	67696.0
174.90	4900.0
175.90	65416.0
176.90	4834.0

Instrument :
MSVOA_U
ClientSampleId :
BFB066

m/z	Abundance
35.90	1450.0
36.90	2674.0
38.00	2948.0
39.10	926.0
39.90	272.0
43.00	154.0
43.80	748.0
45.00	611.0
46.90	705.0
47.70	373.0
49.00	2655.0
50.00	12525.0
50.90	4146.0
51.80	172.0
52.10	190.0
55.00	222.0
55.90	1255.0
57.00	1891.0
59.90	675.0
61.00	3308.0
61.90	3451.0
63.00	3045.0
63.90	591.0
65.10	538.0
66.90	242.0
67.90	7265.0
68.90	7298.0
69.90	468.0
72.00	404.0
73.00	2863.0
73.90	12390.0
74.90	40528.0
75.90	3495.0
76.90	676.0
77.80	319.0
78.90	2157.0
79.80	712.0
80.90	2414.0
81.80	682.0
86.90	2937.0
87.90	3342.0
91.00	304.0
91.90	2449.0
92.90	3540.0
94.00	9295.0
95.00	82024.0
96.00	5281.0
97.00	181.0
103.80	389.0
105.60	264.0
106.00	292.0
115.70	299.0
116.80	595.0
117.80	306.0
118.90	655.0
127.70	262.0
129.80	301.0
130.90	222.0
134.70	129.0
136.70	134.0
140.80	975.0
142.90	1179.0
145.00	316.0
145.80	234.0
147.10	107.0
147.90	282.0
154.80	153.0
156.90	171.0
158.80	134.0
161.00	113.0
171.90	803.0
173.90	64816.0
175.00	4525.0
175.90	62864.0
176.90	4386.0

Instrument :
MSVOA_U
ClientSampleId :
BFB066