

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU110718\
 Data File : VU028004.D
 Acq On : 07 Nov 2018 14:36
 Operator : MD/SY
 Sample : J5839-08
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 SB-6

Quant Time: Nov 07 15:08:44 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U110218W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 02 02:28:20 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	4.99	168	192408	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	5.89	114	364146	50.00	ug/l	0.00
63) Chlorobenzene-d5	9.09	117	325983	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.48	152	135207	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.31	65	160514	56.11	ug/l	0.00
Spiked Amount 50.000			Recovery	=	112.22%	
35) Dibromofluoromethane	4.89	113	121246	52.81	ug/l	0.00
Spiked Amount 50.000			Recovery	=	105.62%	
50) Toluene-d8	7.57	98	474291	53.48	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.96%	
62) 4-Bromofluorobenzene	10.31	95	154161	47.12	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.24%	
Target Compounds						
16) Acetone	2.32	43	17533	9.879	ug/l	97
18) Methyl Acetate	2.62	43	5472	1.121	ug/l	97
20) Methylene Chloride	2.70	84	22040	8.505	ug/l	94
25) 2-Butanone	4.29	43	3523	1.248	ug/l	98
43) Isopropyl Acetate	5.55	43	220129	25.143	ug/l	98
95) Naphthalene	13.74	128	121299	10.795	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU110718\
Data File : VU028004.D
Acq On : 07 Nov 2018 14:36
Operator : MD/SY
Sample : J5839-08
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
SB-6

Quant Time: Nov 07 15:08:44 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\82U110218W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 02 02:28:20 2018
Response via : Initial Calibration

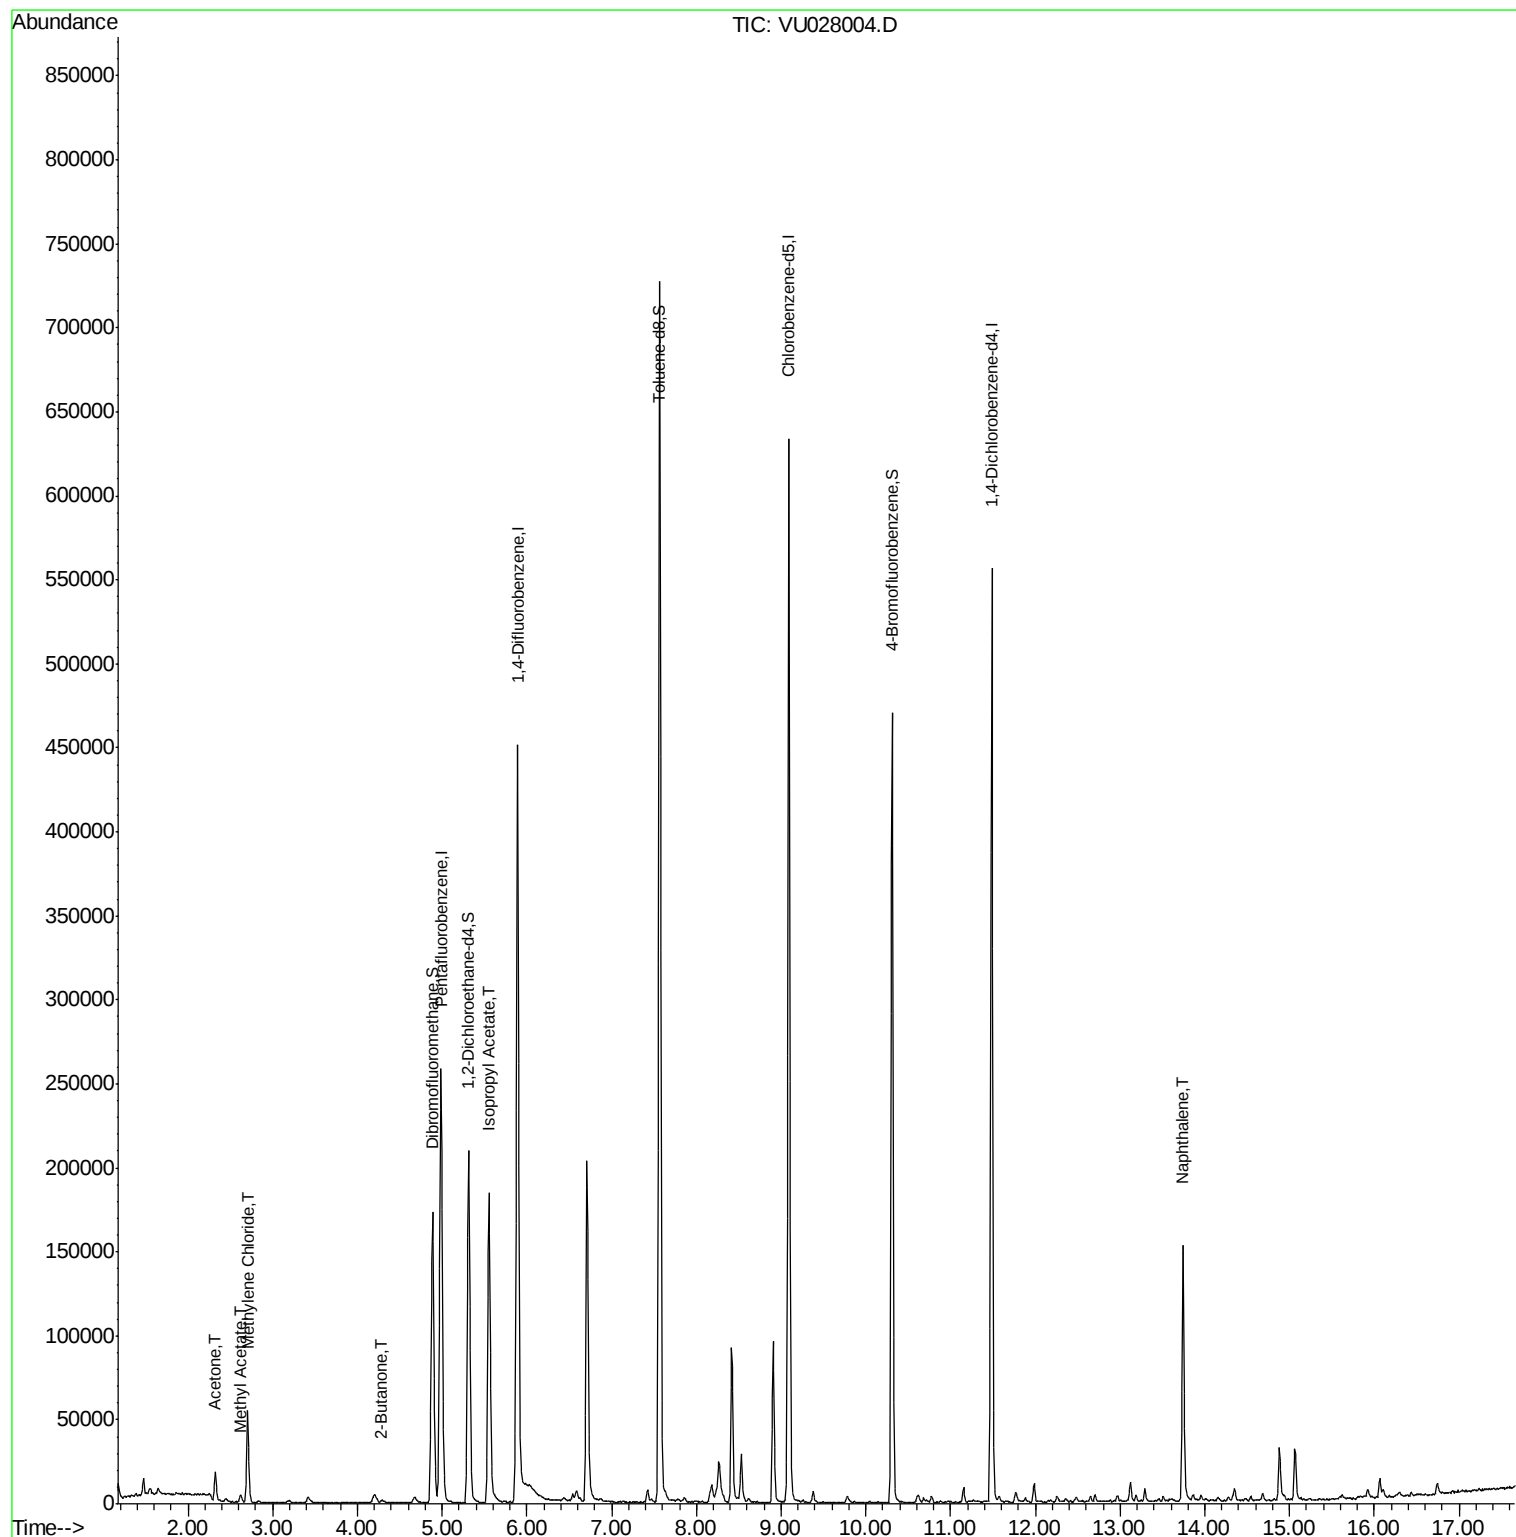

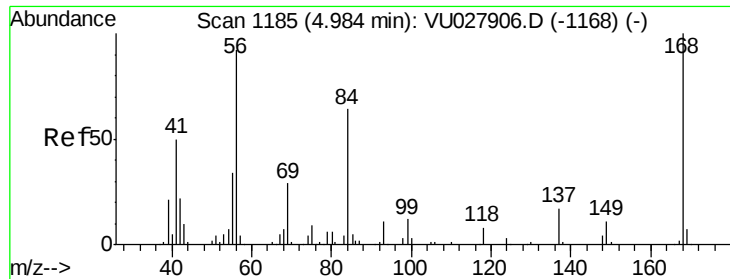

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 4.99 min Scan# 1186

Delta R.T. 0.00 min

Lab File: VU028004.D

Acq: 07 Nov 2018 14:36

Instrument :

MSVOA_U

ClientSampleId :


SB-6

Tot Ion:168 Resp: 192408

Ion Ratio Lower Upper




168 100

99 59.6 47.9 71.9

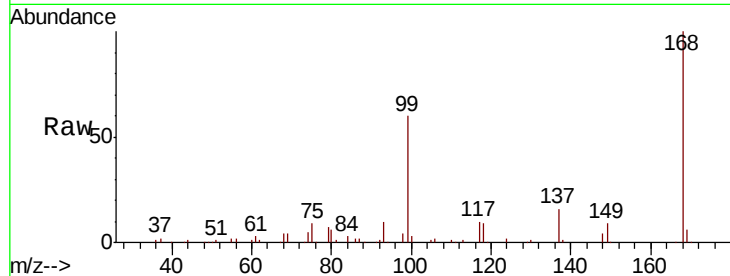

Abundance Ion 167.90 (167.60 to 168.60): VU027906.D (-1168) (-)

Ion 98.90 (98.60 to 99.60): VU028004.D (-1092) (-)

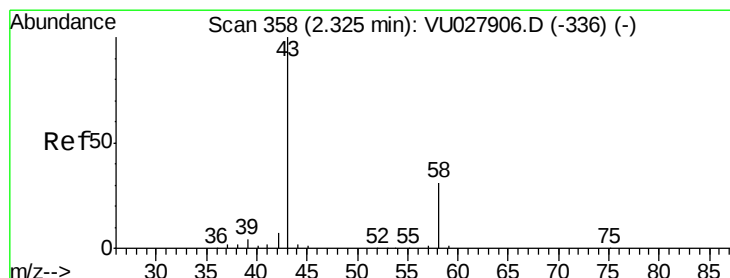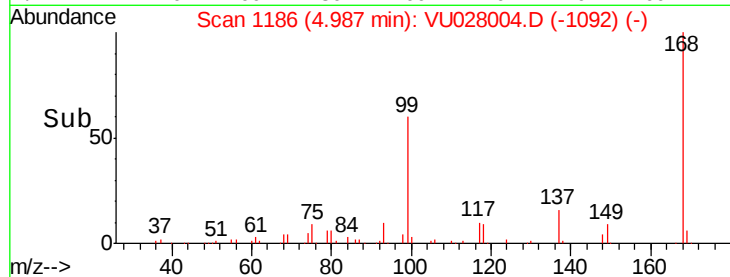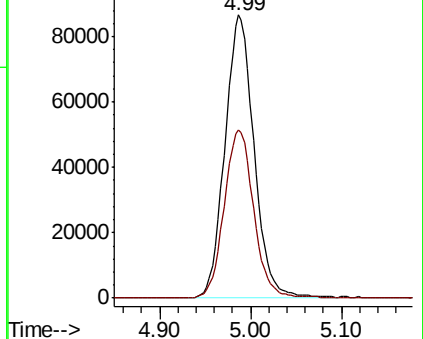

#16

Acetone

Concen: 9.879 ug/l

RT: 2.32 min Scan# 358

Delta R.T. -0.00 min

Lab File: VU028004.D


Acq: 07 Nov 2018 14:36

Tgt Ion: 43 Resp: 17533

Ion Ratio Lower Upper



43 100


58 29.4 24.6 37.0

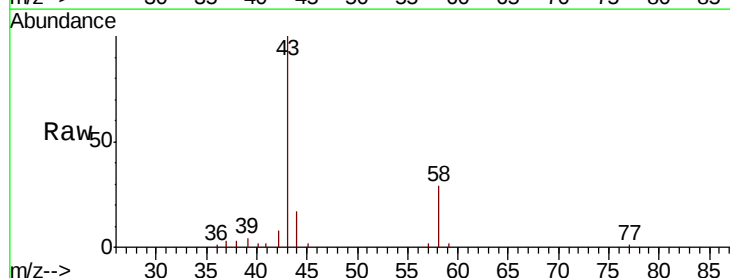

Abundance Ion 43.00 (42.70 to 43.70): VU027906.D (-336) (-)

Ion 58.00 (57.70 to 58.70): VU028004.D (-265) (-)



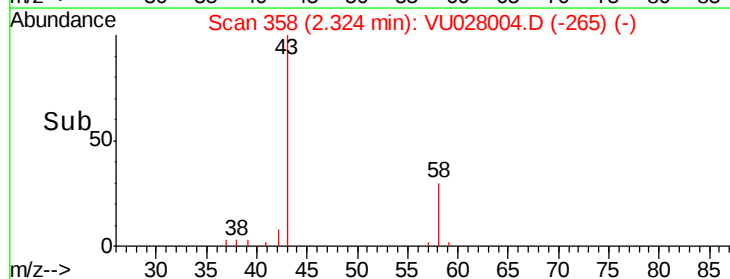
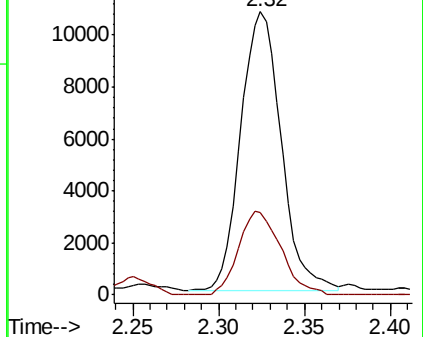


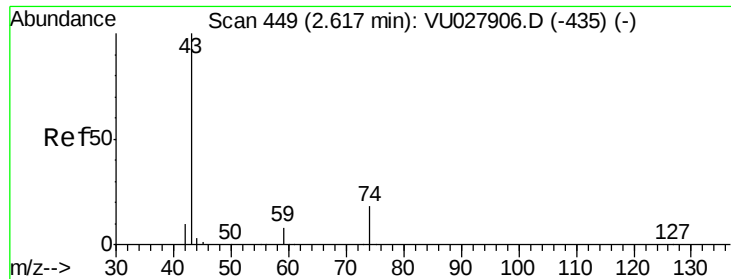

#18
Methyl Acetate
Concen: 1.121 ug/l
RT: 2.62 min Scan# 450
Delta R.T. 0.00 min
Lab File: VU028004.D
Acq: 07 Nov 2018 14:36




Instrument :
MSVOA_U
ClientSampleId :
SB-6


Tot Ion: 43 Resp: 5472
Ion Ratio Lower Upper
43 100
74 17.5 14.9 22.3

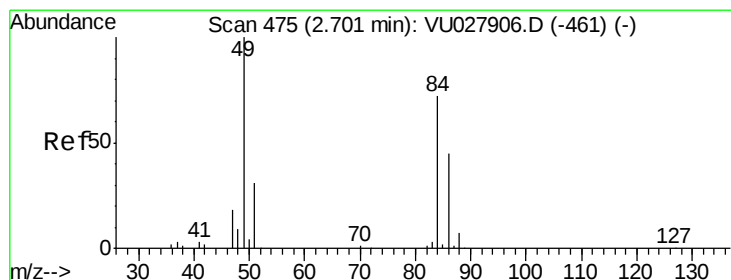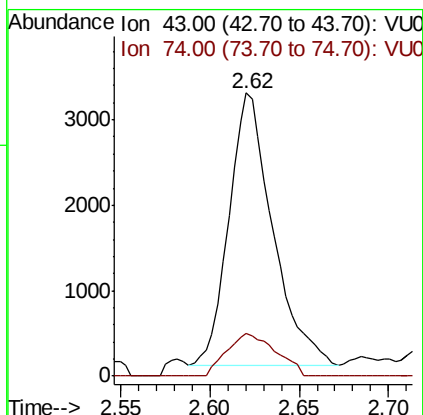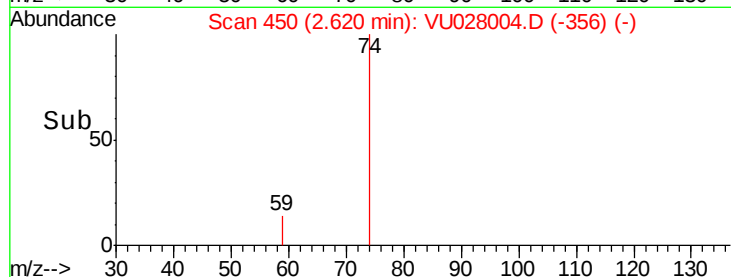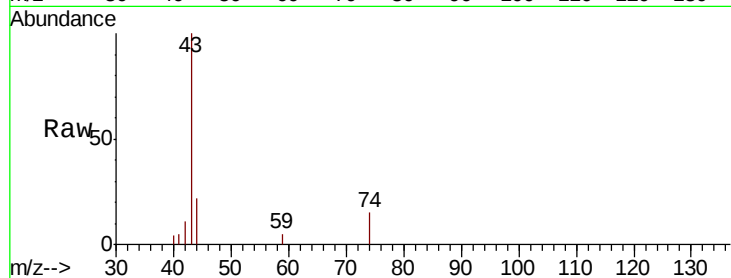

#20
Methylene Chloride
Concen: 8.505 ug/l
RT: 2.70 min Scan# 476
Delta R.T. 0.00 min
Lab File: VU028004.D
Acq: 07 Nov 2018 14:36

Tgt Ion: 84 Resp: 22040
Ion Ratio Lower Upper
84 100
49 146.9 111.6 167.4
51 45.1 34.8 52.2
86 69.3 50.1 75.1

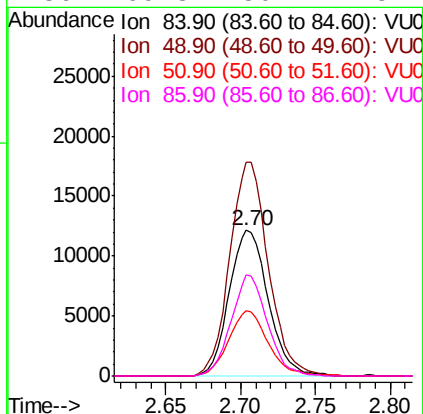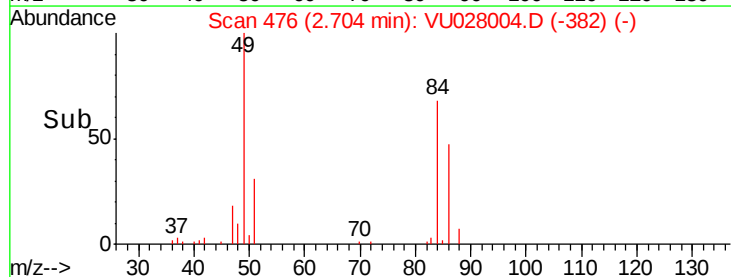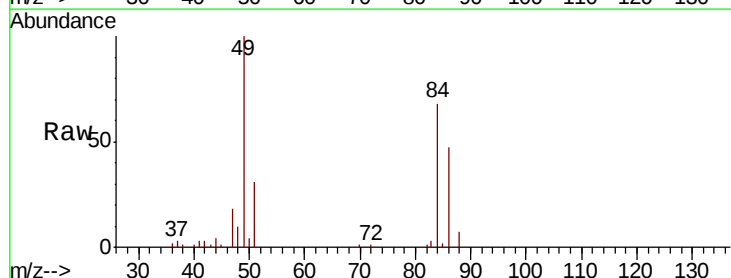

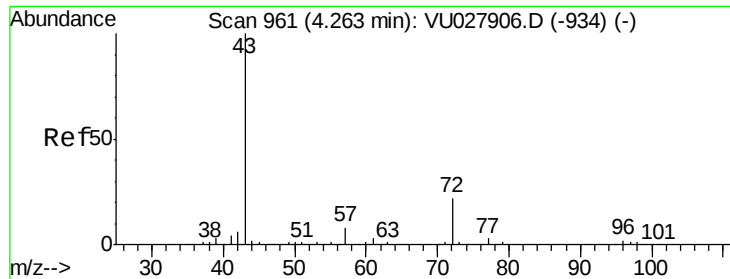

#25

2-Butanone

Concen: 1.248 ug/l

RT: 4.29 min Scan# 970

Delta R.T. 0.03 min

Lab File: VU028004.D

Acq: 07 Nov 2018 14:36

Instrument :

MSVOA_U

ClientSampleId :


SB-6

Tot Ion: 43 Resp: 3523

Ion Ratio Lower Upper




43 100

72 21.1 17.7 26.5

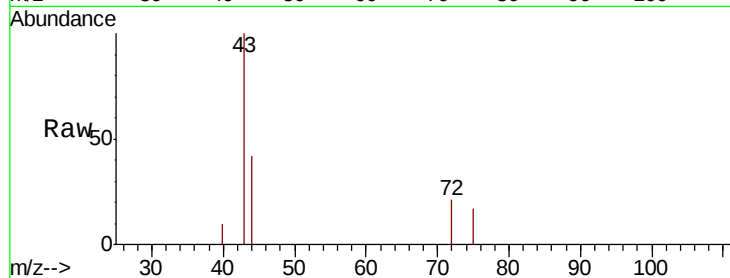

Abundance Ion 43.00 (42.70 to 43.70): VU027906.D (-934) (-)

Ion 72.00 (71.70 to 72.70): VU027906.D (-934) (-)

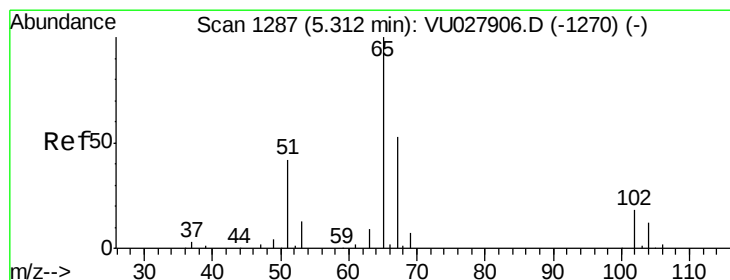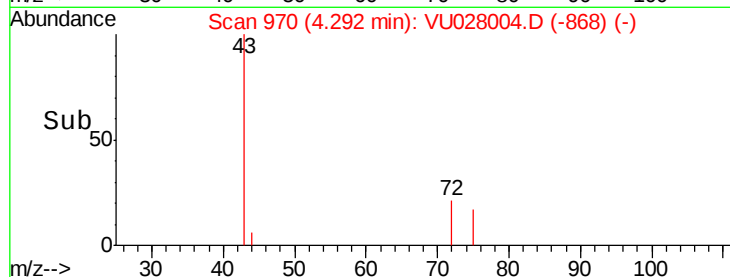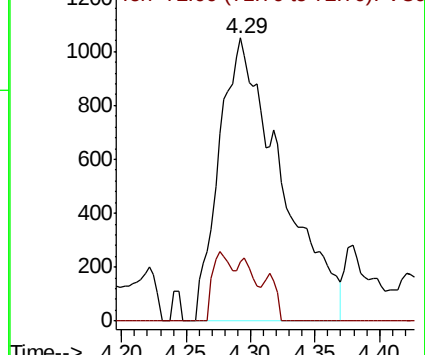

#33

1,2-Dichloroethane-d4

Concen: 56.111 ug/l

RT: 5.31 min Scan# 1287

Delta R.T. -0.00 min

Lab File: VU028004.D


Acq: 07 Nov 2018 14:36

Tgt Ion: 65 Resp: 160514

Ion Ratio Lower Upper



65 100


67 55.2 0.0 109.0

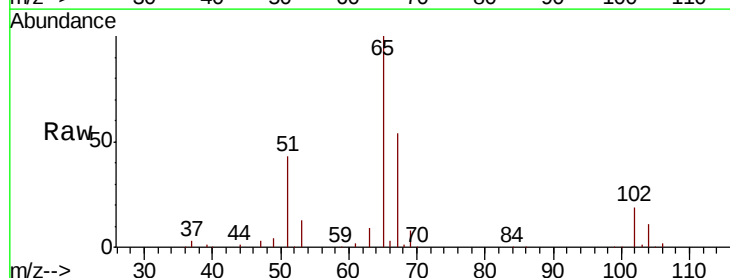

Abundance Ion 64.90 (64.60 to 65.60): VU027906.D (-1270) (-)

Ion 66.90 (66.60 to 67.60): VU027906.D (-1270) (-)

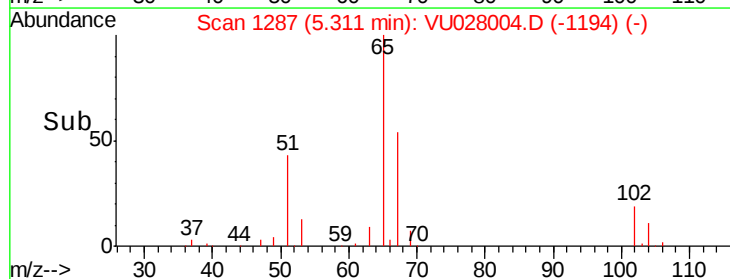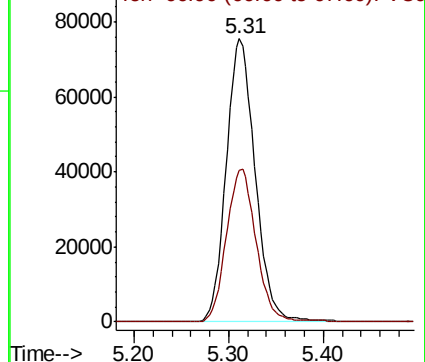


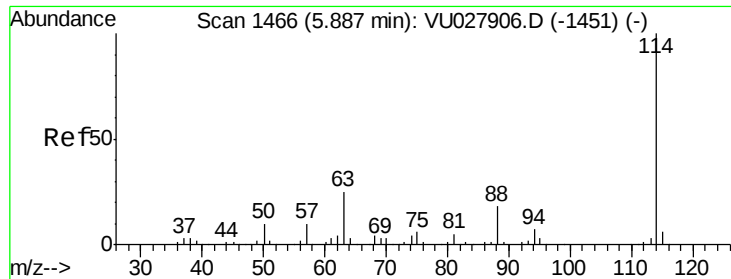




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 5.89 min Scan# 1467
 Delta R.T. 0.00 min
 Lab File: VU028004.D
 Acq: 07 Nov 2018 14:36

Instrument :
 MSVOA_U
 ClientSampleId :
 SB-6

Tot Ion:114 Resp: 364146
 Ion Ratio Lower Upper
 114 100
 63 24.8 0.0 50.8
 88 16.5 0.0 35.8

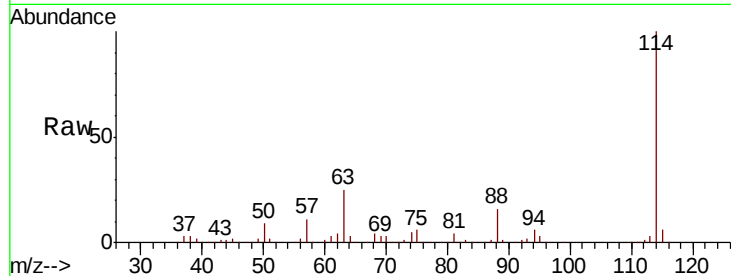


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VU0
 Ion 87.90 (87.60 to 88.60): VU0

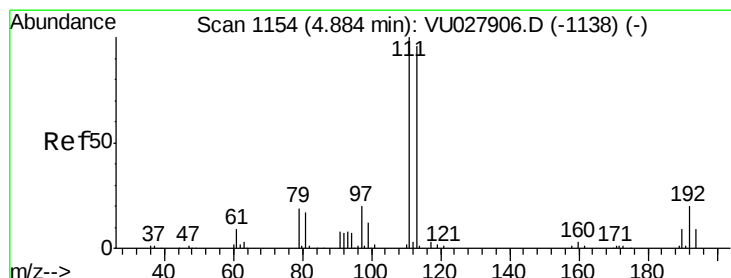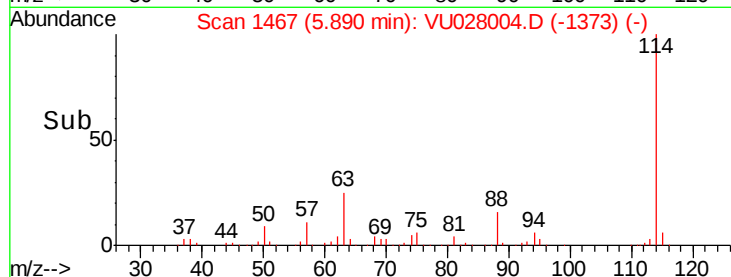
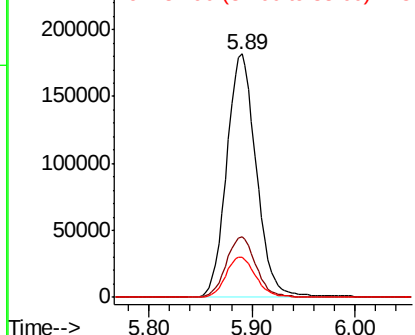



#35
 Dibromofluoromethane
 Concen: 52.808 ug/l
 RT: 4.89 min Scan# 1155
 Delta R.T. 0.00 min
 Lab File: VU028004.D
 Acq: 07 Nov 2018 14:36

Tgt Ion:113 Resp: 121246
 Ion Ratio Lower Upper
 113 100
 111 102.4 83.0 124.6
 192 19.4 15.6 23.4

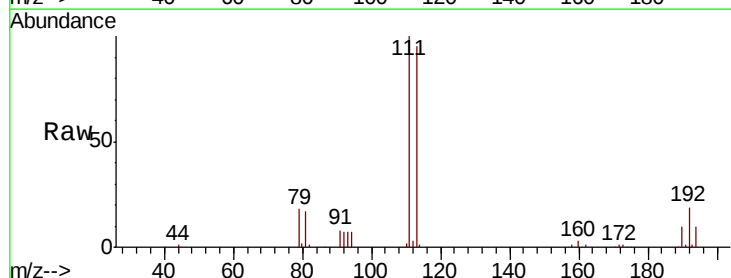

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

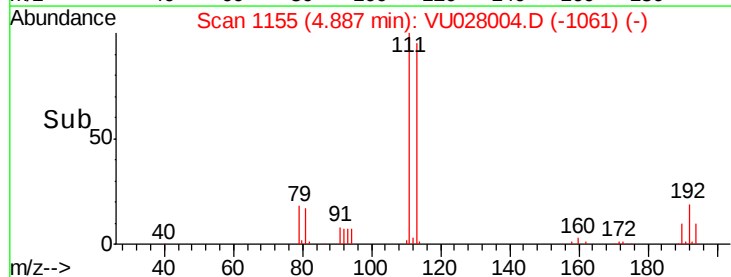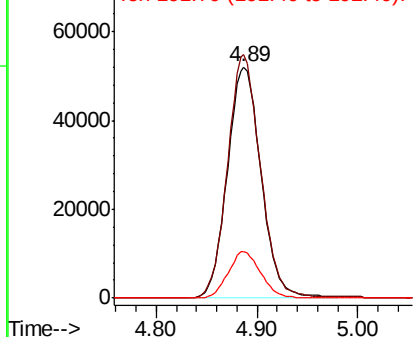

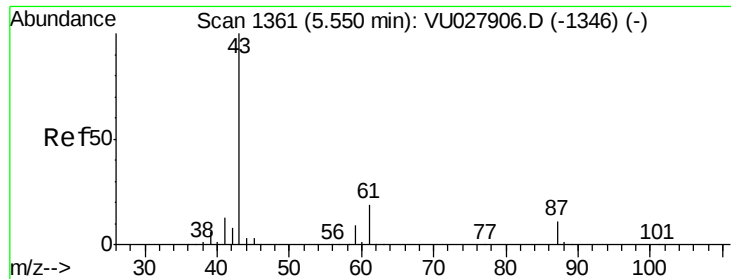

#43

Isopropyl Acetate

Concen: 25.143 ug/l

RT: 5.55 min Scan# 1362

Delta R.T. 0.00 min

Lab File: VU028004.D

Acq: 07 Nov 2018 14:36

Instrument :

MSVOA_U

ClientSampled :

SB-6


Tot Ion: 43 Resp: 220129

Ion Ratio Lower Upper

43 100

61 19.5 15.0 22.4




87 11.1 8.6 12.8

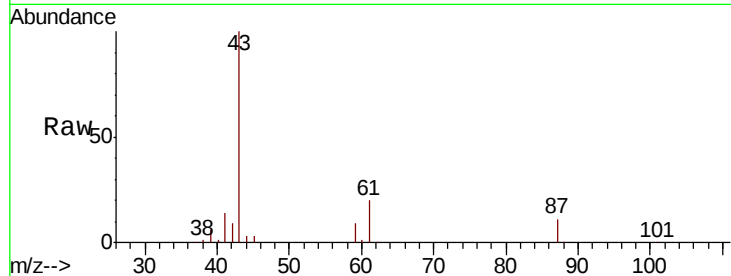

Abundance Ion 43.00 (42.70 to 43.70): VU027906.D (-1346) (-)

Ion 61.00 (60.70 to 61.70): VU027906.D (-1346) (-)

Ion 87.00 (86.70 to 87.70): VU027906.D (-1346) (-)

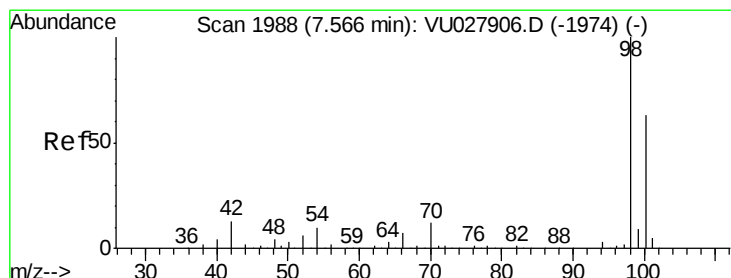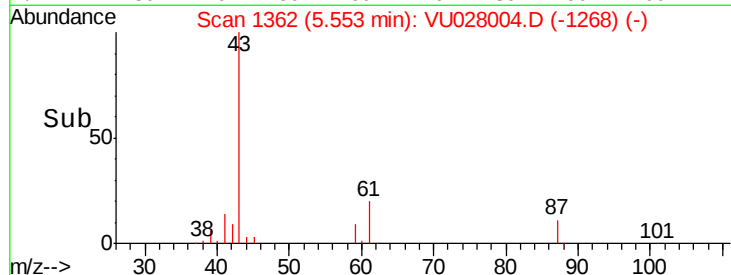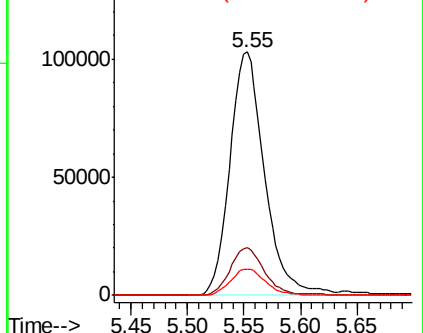

#50

Toluene-d8

Concen: 53.476 ug/l

RT: 7.57 min Scan# 1988

Delta R.T. -0.00 min

Lab File: VU028004.D


Acq: 07 Nov 2018 14:36

Tgt Ion: 98 Resp: 474291

Ion Ratio Lower Upper



98 100


100 63.5 50.1 75.1

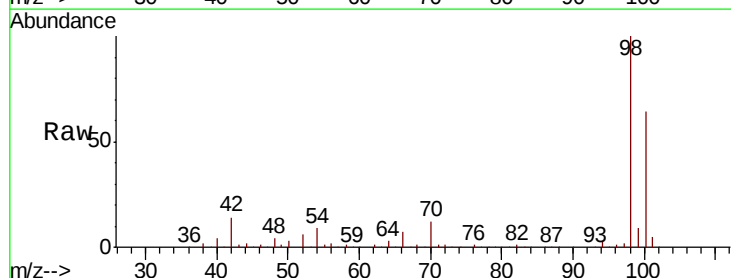

Abundance Ion 98.00 (97.70 to 98.70): VU027906.D (-1974) (-)

Ion 100.00 (99.70 to 100.70): VU027906.D (-1974) (-)



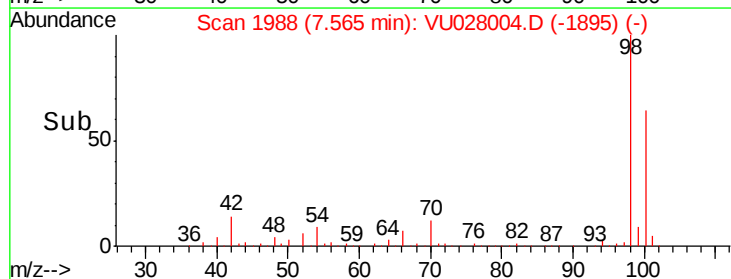
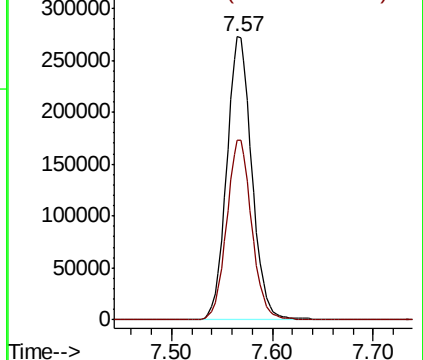


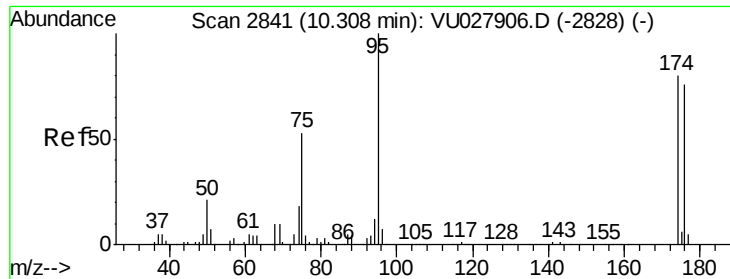

#62
4-Bromofluorobenzene
Concen: 47.124 ug/l
RT: 10.31 min Scan# 2841
Delta R.T. -0.00 min
Lab File: VU028004.D
Acq: 07 Nov 2018 14:36




Instrument :
MSVOA_U
ClientSampleId :
SB-6


Tot Ion: 95 Resp: 154161
Ion Ratio Lower Upper
95 100
174 76.5 0.0 156.4
176 74.2 0.0 150.8

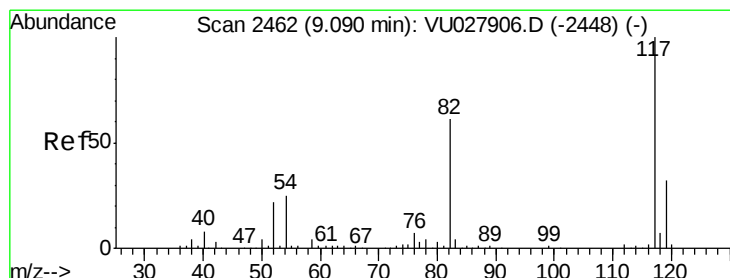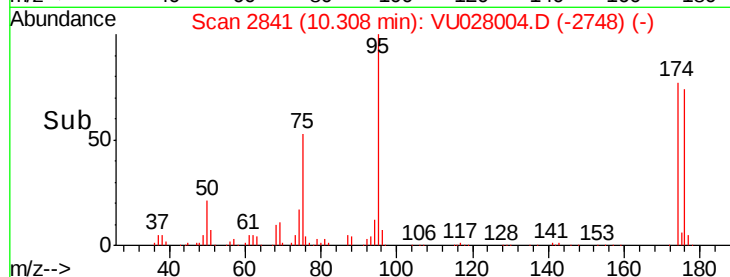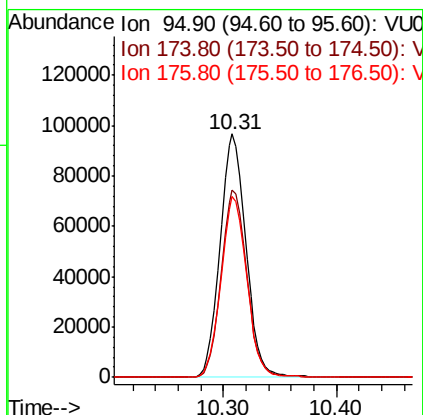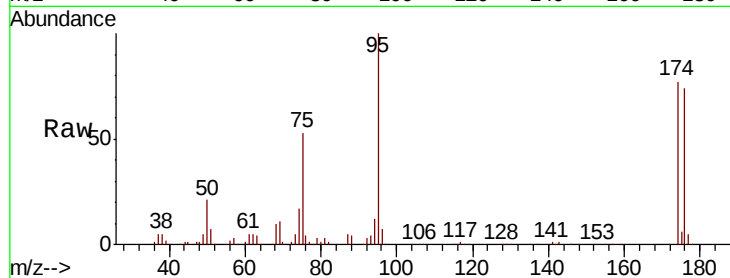

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.09 min Scan# 2462
Delta R.T. -0.00 min
Lab File: VU028004.D
Acq: 07 Nov 2018 14:36

Tgt Ion: 117 Resp: 325983
Ion Ratio Lower Upper
117 100
82 62.5 48.6 73.0
119 31.8 25.8 38.8

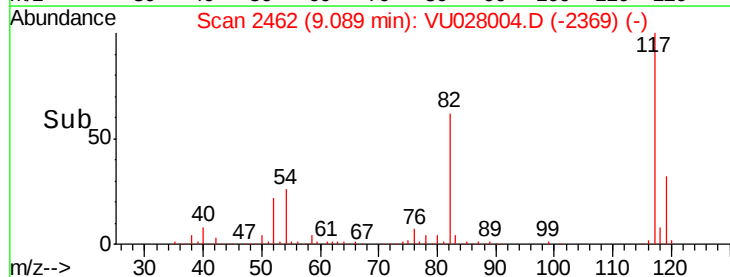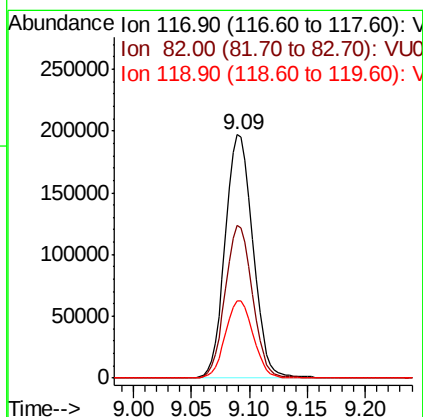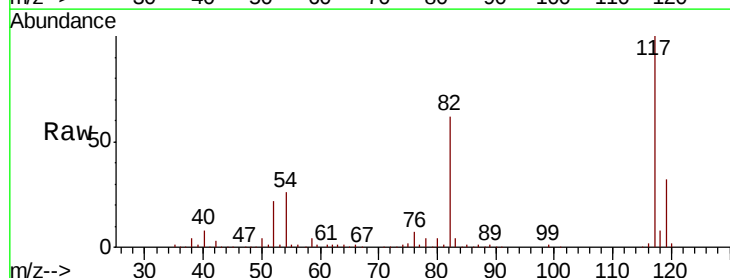

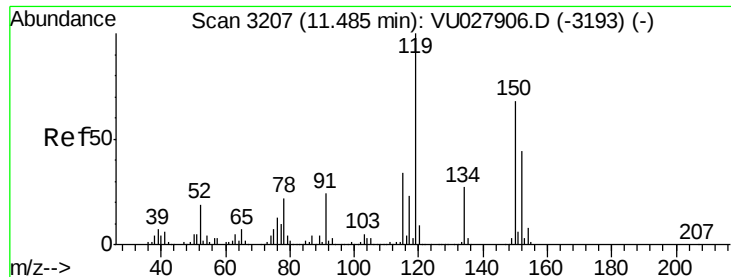

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 11.48 min Scan# 3207

Delta R.T. -0.00 min

Lab File: VU028004.D

Acq: 07 Nov 2018 14:36

Instrument :

MSVOA_U

ClientSampleId :

SB-6


Tot Ion:152 Resp: 135207

Ion Ratio Lower Upper

152 100

115 59.4 43.0 129.0




150 156.0 0.0 349.4

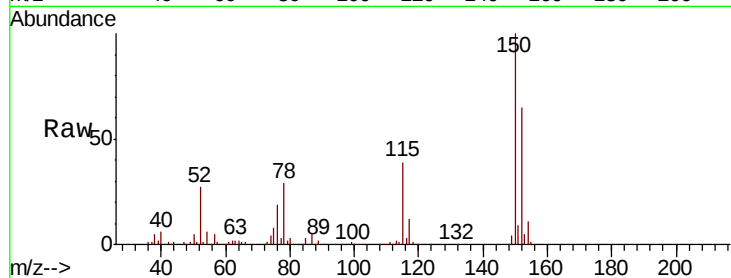

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

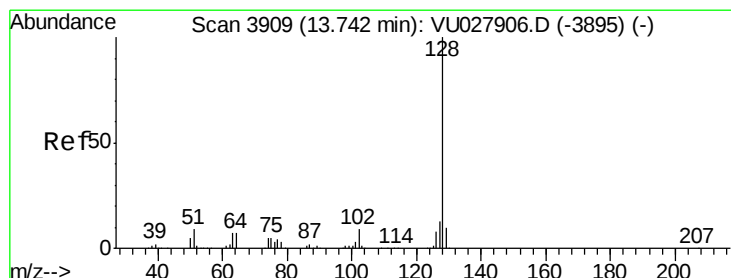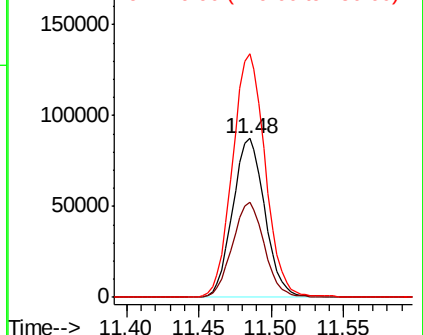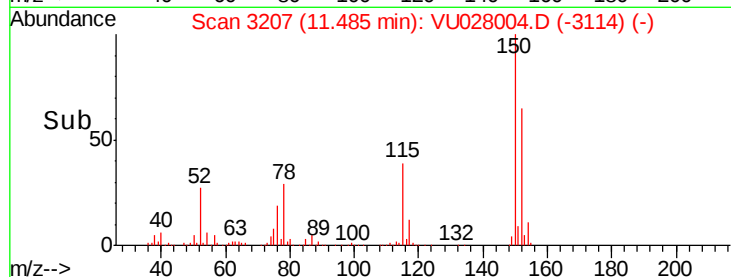

#95

Naphthalene

Concen: 10.795 ug/l

RT: 13.74 min Scan# 3909

Delta R.T. -0.00 min

Lab File: VU028004.D

Acq: 07 Nov 2018 14:36


Tgt Ion:128 Resp: 121299

Ion Ratio Lower Upper

128 100

127 13.1 10.4 15.6

129 11.1 8.3 12.5

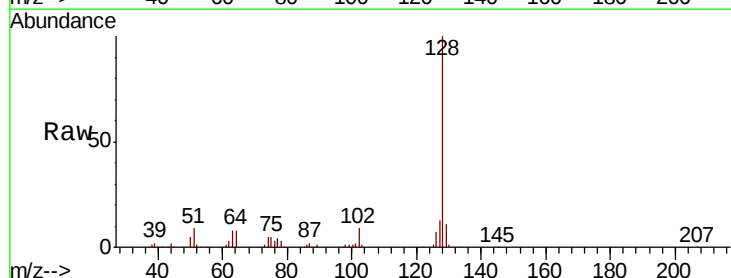

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

