

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU110719\
 Data File : VU035670.D
 Acq On : 07 Nov 2019 19:22
 Operator : JC/SP
 Sample : K5739-03DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CR1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.617	78	86	102	rBV	375296	409316	16.45%	2.232%
2	1.935	176	185	202	rVB	288666	388078	15.60%	2.116%
3	2.597	378	391	406	rBV	522467	864480	34.75%	4.713%
4	2.813	449	458	475	rVB4	3899	8907	0.36%	0.049%
5	3.080	535	541	544	rBV4	1410	1751	0.07%	0.010%
6	3.176	568	571	573	rBV2	619	401	0.02%	0.002%
7	3.234	575	589	608	rVB	44026	96908	3.90%	0.528%
8	3.346	617	624	626	rBV3	581	536	0.02%	0.003%
9	3.398	636	640	642	rBV2	552	348	0.01%	0.002%
10	3.443	651	654	657	rBV3	444	327	0.01%	0.002%
11	3.543	681	685	689	rVB2	634	414	0.02%	0.002%
12	3.594	698	701	708	rVB2	414	458	0.02%	0.002%
13	3.626	708	711	713	rBV	638	305	0.01%	0.002%
14	3.665	720	723	725	rBV2	396	285	0.01%	0.002%
15	3.729	739	743	747	rVB3	501	445	0.02%	0.002%
16	3.764	747	754	755	rBV2	450	467	0.02%	0.003%
17	3.774	755	757	761	rVB2	406	277	0.01%	0.002%
18	3.861	779	784	790	rVB4	514	585	0.02%	0.003%
19	3.948	808	811	815	rVV3	335	259	0.01%	0.001%
20	4.035	830	838	841	rBV3	308	366	0.01%	0.002%
21	4.407	950	954	957	rBV2	423	333	0.01%	0.002%
22	4.443	962	965	969	rBV	318	279	0.01%	0.002%
23	4.465	969	972	979	rVB2	412	359	0.01%	0.002%
24	4.504	979	984	988	rBV3	589	592	0.02%	0.003%
25	4.623	1018	1021	1023	rBV	442	295	0.01%	0.002%
26	4.694	1026	1043	1062	rBV	222934	548663	22.06%	2.992%
27	5.057	1150	1156	1157	rBV3	616	552	0.02%	0.003%
28	5.115	1158	1174	1200	rVV	437062	956288	38.44%	5.214%
29	5.321	1236	1238	1239	rBV2	671	276	0.01%	0.002%
30	5.475	1282	1286	1291	rBV3	494	557	0.02%	0.003%
31	5.549	1305	1309	1316	rVB3	513	578	0.02%	0.003%
32	5.581	1316	1319	1324	rBV2	362	385	0.02%	0.002%
33	5.681	1348	1350	1356	rVB	376	267	0.01%	0.001%
34	5.771	1356	1378	1422	rBV2	941621	2487517	100.00%	13.563%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU110719\
 Data File : VU035670.D
 Acq On : 07 Nov 2019 19:22
 Operator : JC/SP
 Sample : K5739-03DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CR1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
 Title : VOC Analysis

35	6.292	1525	1540	1572	rBV	818121	1578823	63.47%	8.608%
36	6.658	1651	1654	1662	rVB2	667	523	0.02%	0.003%
37	6.735	1662	1678	1706	rBV	560308	1108497	44.56%	6.044%
38	6.938	1739	1741	1744	rVB2	929	448	0.02%	0.002%
39	6.954	1744	1746	1748	rBV3	437	287	0.01%	0.002%
40	7.163	1807	1811	1814	rBV2	386	281	0.01%	0.002%
41	7.224	1818	1830	1837	rBV6	3171	5603	0.23%	0.031%
42	7.282	1845	1848	1852	rVB2	352	289	0.01%	0.002%
43	7.311	1855	1857	1861	rVB	533	257	0.01%	0.001%
44	7.372	1872	1876	1880	rVB3	390	383	0.02%	0.002%
45	7.411	1885	1888	1892	rBV2	350	371	0.01%	0.002%
46	7.604	1934	1948	1974	rBV	289906	534942	21.51%	2.917%
47	7.880	2029	2034	2036	rBV2	487	426	0.02%	0.002%
48	7.935	2036	2051	2083	rBV	1139858	2040599	82.03%	11.126%
49	8.214	2124	2138	2164	rBV	201691	369312	14.85%	2.014%
50	8.404	2195	2197	2200	rBV3	424	325	0.01%	0.002%
51	8.456	2211	2213	2218	rVB2	505	316	0.01%	0.002%
52	8.584	2247	2253	2257	rBV6	1260	1737	0.07%	0.009%
53	8.620	2261	2264	2267	rBV	498	384	0.02%	0.002%
54	8.677	2268	2282	2342	rVV	379920	1129988	45.43%	6.161%
55	8.993	2378	2380	2384	rVB3	412	307	0.01%	0.002%
56	9.301	2473	2476	2481	rBV3	388	364	0.01%	0.002%
57	9.333	2481	2486	2491	rVB2	290	326	0.01%	0.002%
58	9.449	2508	2522	2558	rVV	1063652	1970763	79.23%	10.745%
59	9.600	2566	2569	2571	rBV2	592	374	0.02%	0.002%
60	9.645	2580	2583	2587	rBV	380	291	0.01%	0.002%
61	9.668	2587	2590	2596	rBV2	521	497	0.02%	0.003%
62	9.716	2599	2605	2606	rBV3	1073	856	0.03%	0.005%
63	9.806	2630	2633	2635	rVB2	562	301	0.01%	0.002%
64	10.089	2717	2721	2723	rBV2	314	281	0.01%	0.002%
65	10.134	2728	2735	2736	rBV3	681	577	0.02%	0.003%
66	10.224	2761	2763	2767	rVB2	410	243	0.01%	0.001%
67	10.484	2841	2844	2847	rVB2	400	254	0.01%	0.001%
68	10.510	2847	2852	2854	rBV2	566	480	0.02%	0.003%
69	10.619	2882	2886	2888	rBV2	362	282	0.01%	0.002%
70	10.787	2924	2938	2960	rVB	697517	1212176	48.73%	6.609%
71	10.883	2966	2968	2971	rVV2	350	247	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU110719\
 Data File : VU035670.D
 Acq On : 07 Nov 2019 19:22
 Operator : JC/SP
 Sample : K5739-03DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0CR1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
 Title : VOC Analysis

72	10.902	2972	2974	2984	rVB3	915	1135	0.05%	0.006%
73	10.947	2984	2988	2993	rBV2	438	530	0.02%	0.003%
74	10.983	2996	2999	3001	rBV2	421	302	0.01%	0.002%
75	11.111	3036	3039	3042	rBV	447	395	0.02%	0.002%
76	11.378	3116	3122	3127	rBV3	447	534	0.02%	0.003%
77	11.407	3128	3131	3137	rVB2	352	296	0.01%	0.002%
78	11.446	3138	3143	3146	rBV3	782	679	0.03%	0.004%
79	11.709	3221	3225	3228	rBV	400	347	0.01%	0.002%
80	11.774	3238	3245	3246	rBV4	2367	2305	0.09%	0.013%
81	11.844	3253	3267	3287	rVB	649694	1179982	47.44%	6.434%
82	11.947	3297	3299	3306	rVB2	527	494	0.02%	0.003%
83	12.224	3370	3385	3404	rVV2	719242	1370246	55.08%	7.471%
84	12.336	3416	3420	3425	rBV2	717	820	0.03%	0.004%
85	12.359	3425	3427	3432	rVV2	543	418	0.02%	0.002%
86	12.398	3436	3439	3442	rBV	384	347	0.01%	0.002%
87	12.462	3456	3459	3464	rVB2	562	316	0.01%	0.002%
88	12.880	3586	3589	3592	rBV2	543	406	0.02%	0.002%
89	13.047	3638	3641	3648	rVB3	703	716	0.03%	0.004%
90	13.179	3678	3682	3685	rBV2	633	668	0.03%	0.004%
91	13.233	3690	3699	3708	rVV2	8261	13474	0.54%	0.073%
92	13.372	3739	3742	3749	rBV3	751	604	0.02%	0.003%
93	13.799	3873	3875	3879	rBV2	450	291	0.01%	0.002%
94	13.864	3886	3895	3904	rVB4	6965	10887	0.44%	0.059%
95	14.018	3940	3943	3947	rBV3	743	562	0.02%	0.003%
96	14.069	3957	3959	3962	rBV2	499	402	0.02%	0.002%
97	14.147	3980	3983	3986	rBV4	891	664	0.03%	0.004%
98	14.352	4040	4047	4056	rVB3	7633	11156	0.45%	0.061%
99	14.709	4155	4158	4162	rBV3	1120	835	0.03%	0.005%
100	14.748	4162	4170	4180	rBV7	3610	6593	0.27%	0.036%


Sum of corrected areas: 18340668

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU110719\
Data File : VU035670.D
Acq On : 07 Nov 2019 19:22
Operator : JC/SP
Sample : K5739-03DL 5X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CR1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

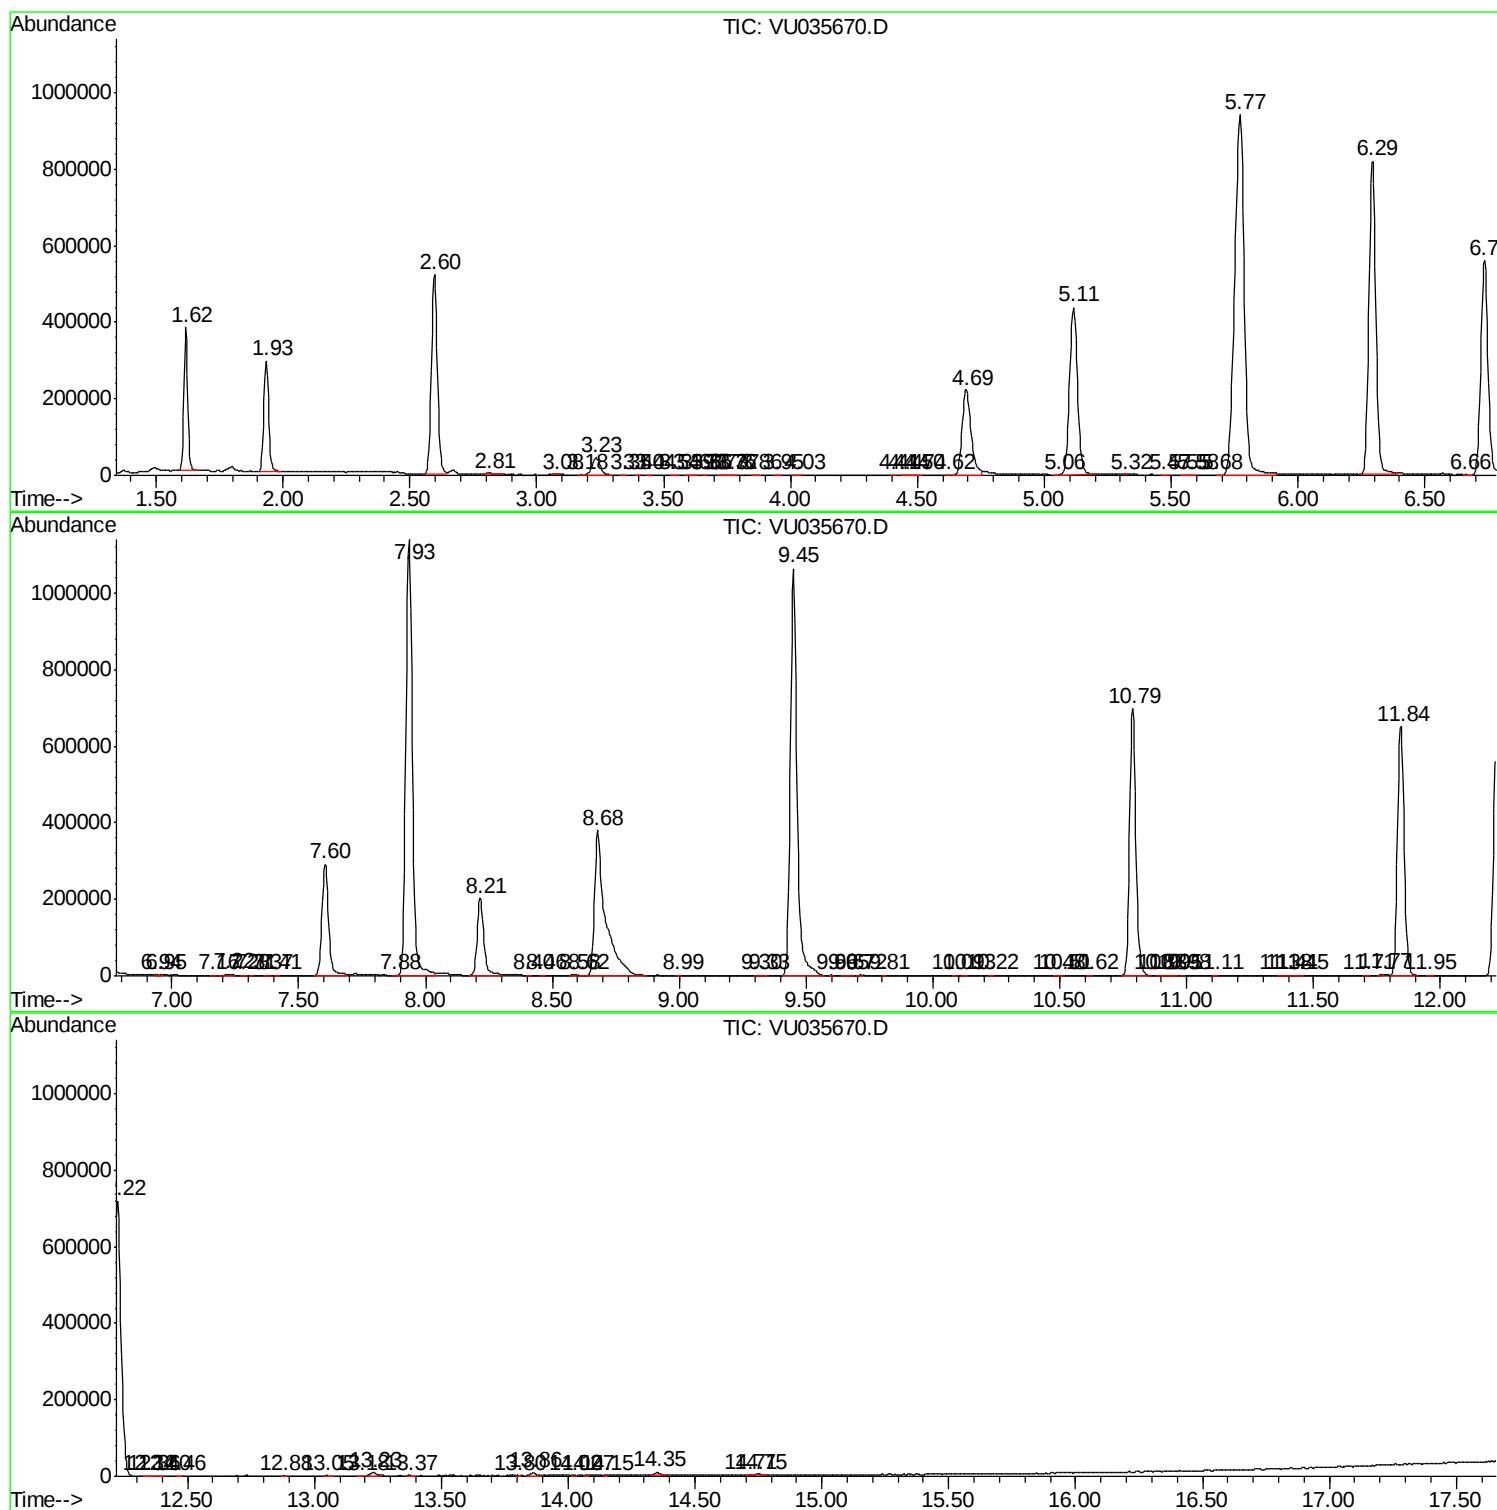

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU110719\
Data File : VU035670.D
Acq On : 07 Nov 2019 19:22
Operator : JC/SP
Sample : K5739-03DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CR1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU110719\
Data File : VU035670.D
Acq On : 07 Nov 2019 19:22
Operator : JC/SP
Sample : K5739-03DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0CR1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc