


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU110719\
Data File : VU035659.D
Acq On : 07 Nov 2019 14:53
Operator : JC/SP
Sample : BFB51
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB51

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM103119WMA.M
Title : VOC Analysis
Last Update : Fri Nov 08 16:37:31 2019

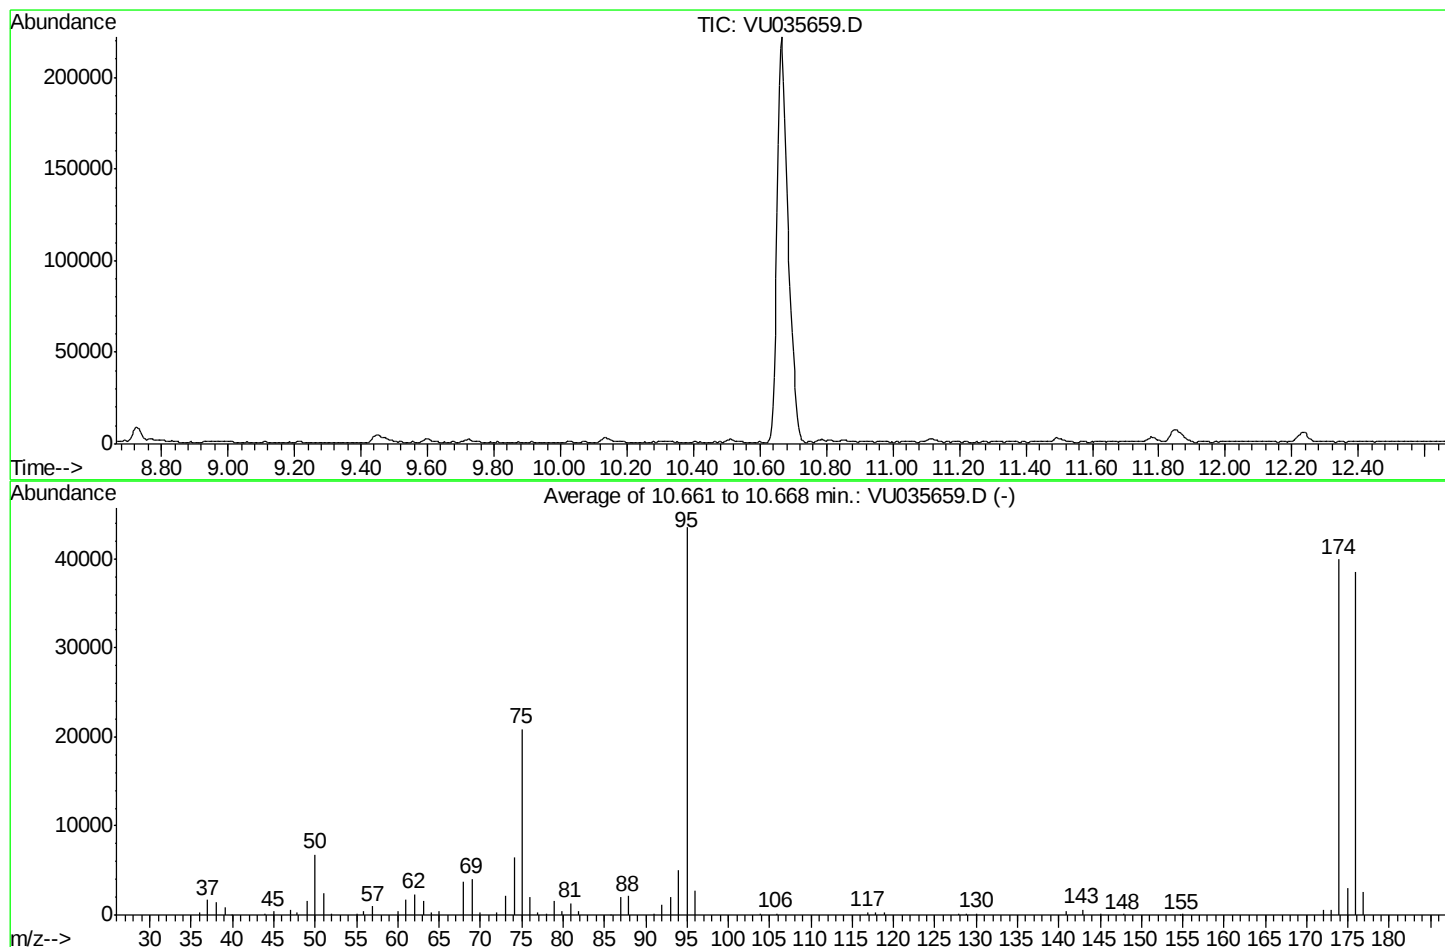

AutoFind: Scans 2899, 2900, 2901; Background Corrected with Scan 2886

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	6789	PASS
75	95	30	80	47.9	20866	PASS
95	95	100	100	100.0	43546	PASS
96	95	5	9	6.3	2763	PASS
173	174	0.00	2	1.4	579	PASS
174	95	50	120	91.7	39936	PASS
175	174	5	9	7.5	2984	PASS
176	174	95	101	96.5	38544	PASS
177	176	5	9	6.6	2529	PASS

Scan 2886 (10.620 min): VU035659.D
BFB51

m/z	Abundance
40.00	234.0
43.90	796.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
35.90	369.0
37.00	1681.0
38.00	1526.0
39.10	784.0
39.90	284.0
44.00	1029.0
45.00	354.0
47.00	534.0
47.90	275.0
49.00	1604.0
50.00	6734.0
51.00	2465.0
52.00	142.0
55.90	480.0
57.00	1023.0
60.00	413.0
61.00	1872.0
62.00	2372.0
63.00	1538.0
64.00	267.0
65.00	323.0
68.00	3801.0
69.00	4130.0
70.00	290.0
72.00	182.0
73.00	2112.0
74.10	6533.0
75.00	21032.0
76.00	1977.0
76.90	343.0
77.90	235.0
78.90	1537.0
79.90	400.0
80.90	1271.0
81.90	419.0
87.00	2204.0
87.90	2125.0
91.00	208.0
92.00	1129.0
93.00	1949.0
94.00	4905.0
95.00	43160.0
96.00	2770.0
103.90	126.0
105.90	166.0
116.90	265.0
117.90	291.0
118.90	239.0
127.80	154.0
128.70	157.0
130.00	233.0
140.90	465.0
142.90	631.0
147.90	126.0
155.00	125.0
172.00	560.0
172.90	582.0
173.90	39504.0
175.00	2981.0
175.90	37392.0
176.90	2720.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
35.90	335.0
37.00	1695.0
38.00	1524.0
39.00	817.0
39.90	292.0
44.00	990.0
45.00	380.0
47.00	639.0
47.80	247.0
49.00	1637.0
50.00	6855.0
51.00	2542.0
52.00	136.0
55.10	145.0
55.90	428.0
57.00	1001.0
60.00	380.0
61.00	1786.0
62.00	2346.0
63.00	1680.0
64.00	268.0
65.00	402.0
68.00	3842.0
69.00	4063.0
69.90	305.0
72.00	235.0
73.00	2180.0
74.10	6459.0
75.00	21512.0
76.00	2074.0
76.90	315.0
78.00	208.0
78.90	1571.0
79.90	428.0
80.90	1328.0
81.90	492.0
85.80	100.0
86.90	2082.0
87.90	2184.0
90.90	215.0
92.00	1233.0
93.00	1974.0
94.00	5128.0
95.00	44384.0
96.00	2736.0
103.80	143.0
105.80	166.0
116.90	333.0
117.90	308.0
118.90	282.0
127.80	167.0
128.80	141.0
130.10	231.0
140.90	464.0
142.90	662.0
145.00	118.0
147.80	114.0
154.70	138.0
155.00	129.0
172.00	518.0
172.90	590.0
173.90	40912.0
175.00	3107.0
175.90	39336.0
176.90	2596.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
36.00	265.0
37.00	1744.0
38.00	1409.0
39.00	804.0
40.00	276.0
44.00	1000.0
45.00	358.0
47.00	628.0
47.70	251.0
49.00	1442.0
50.00	6780.0
51.00	2390.0
52.00	102.0
55.00	152.0
55.90	402.0
57.00	882.0
60.00	321.0
61.00	1665.0
62.00	2196.0
63.10	1734.0
64.00	221.0
65.00	416.0
68.00	3716.0
69.00	3996.0
70.00	313.0
72.00	276.0
73.00	2024.0
74.00	6437.0
75.00	20056.0
76.00	1912.0
76.90	301.0
78.00	200.0
78.90	1450.0
79.90	445.0
80.90	1425.0
81.90	484.0
86.90	1864.0
87.90	2041.0
90.90	194.0
92.00	1296.0
93.00	1942.0
94.00	5042.0
95.00	43096.0
96.00	2785.0
103.80	154.0
105.80	179.0
116.90	360.0
117.80	257.0
118.90	290.0
127.90	172.0
130.10	175.0
140.90	410.0
142.90	649.0
145.00	174.0
147.90	105.0
154.90	107.0
171.90	475.0
172.90	566.0
173.90	39392.0
174.90	2865.0
175.90	38904.0
176.90	2271.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51